

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 19:00
 Operator : AR\AJ
 Sample : M2323-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AST2-COPR2-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 08:03:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	18505878	223.8E6	20.812	19.331
28)	SA Decachlor...	8.201	9.031	20558438	227.8E6	19.418	19.738
Target Compounds							
7)	B delta-BHC	0.000	5.008f	0 96934092	N.D.	5.370	#
8)	B Heptachlo...	0.000	5.852	0 21370103	N.D.	1.338	#
14)	MA Endrin	0.000	6.705f	0 282.8E6	N.D.	20.116	#
15)	B Endosulfa...	0.000	6.894	0 6190720	N.D.	0.463	#
17)	MA 4,4'-DDT	0.000	7.079f	0 18772825	N.D.	1.474	#
27)	Chlordane-5	0.000	6.948	0 5251929	N.D.	10.678	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 19:00
Operator : AR\AJ
Sample : M2323-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
AST2-COPR2-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 08:03:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

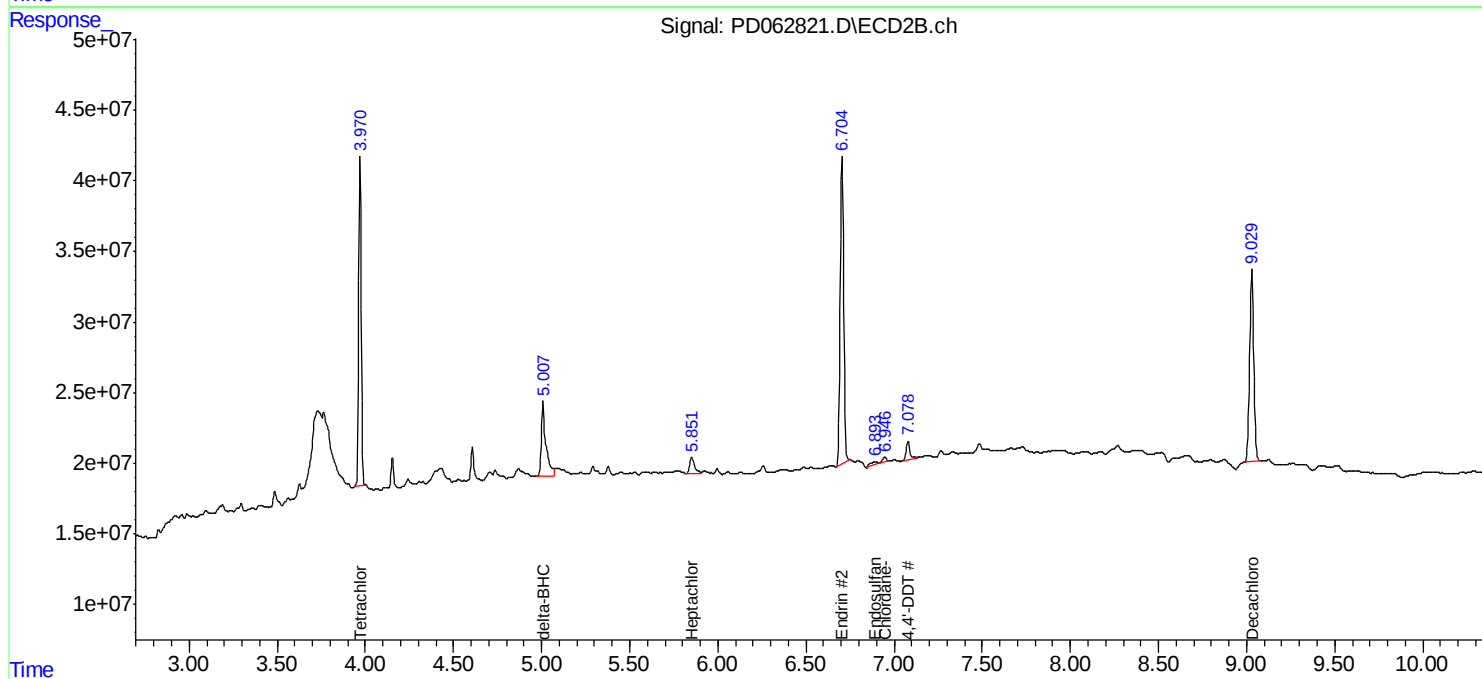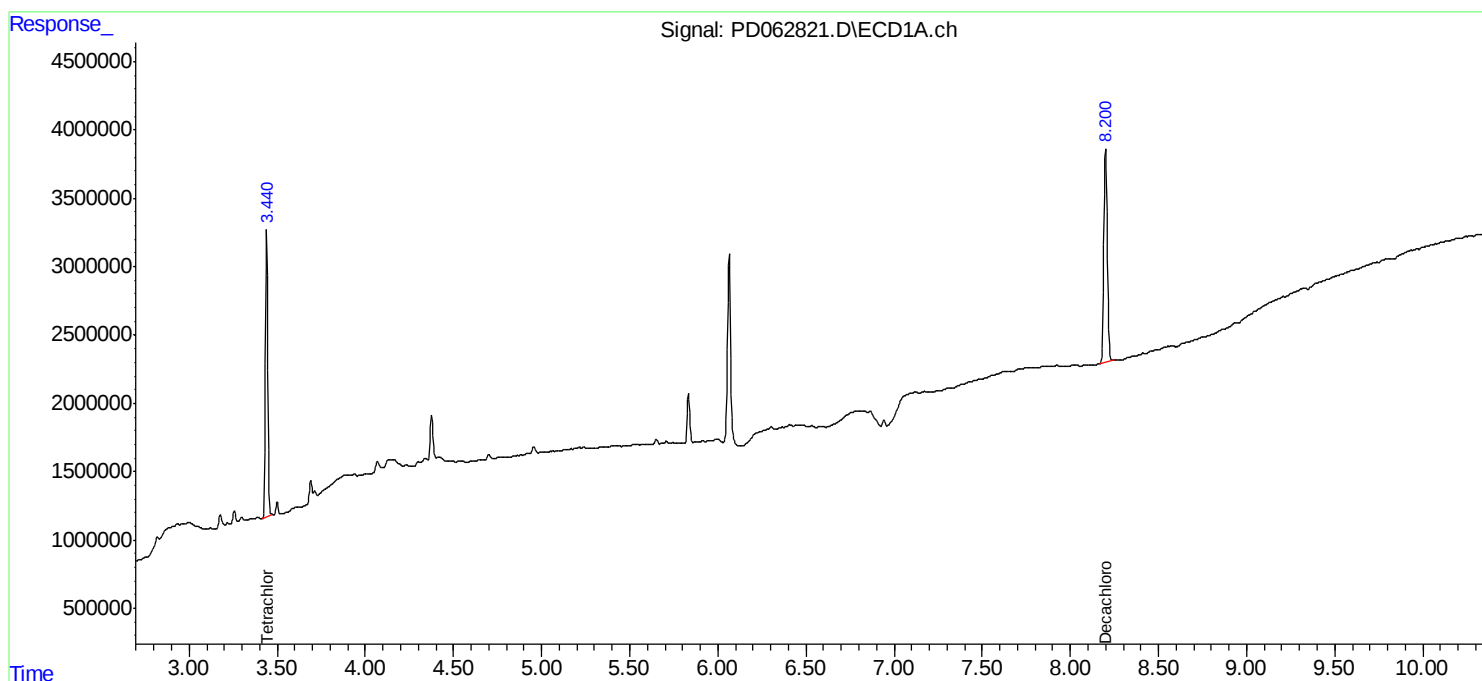


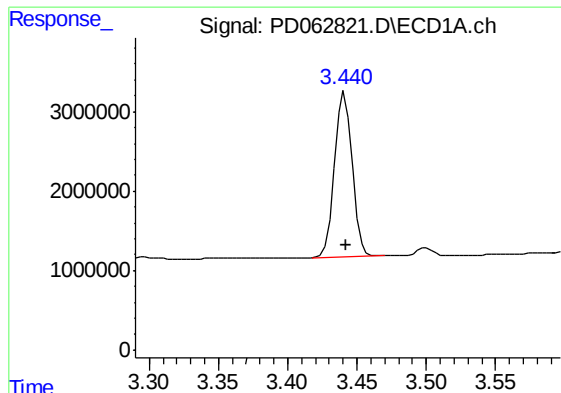

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 18505878
Conc: 20.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
AST2-COPR2-1

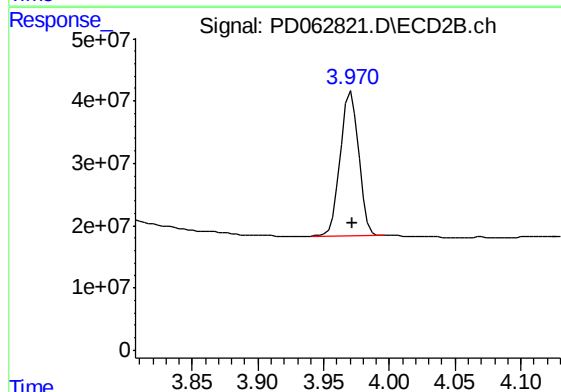


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 223792460
Conc: 19.33 ng/ml

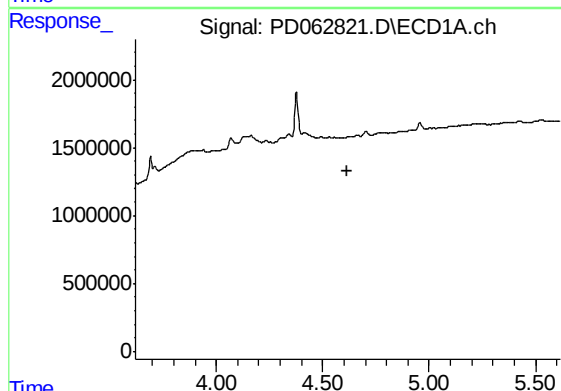


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

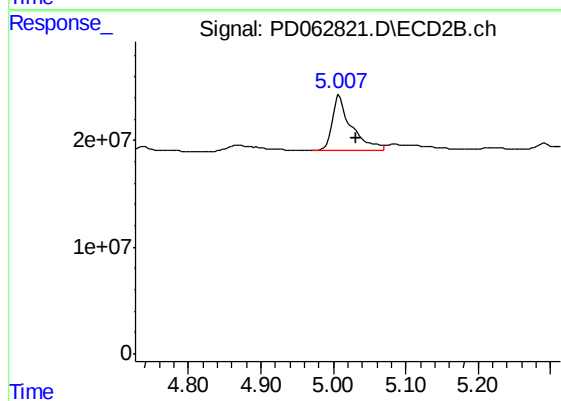

#7 delta-BHC


R.T.: 5.008 min
Delta R.T.: -0.024 min
Response: 96934092
Conc: 5.37 ng/ml

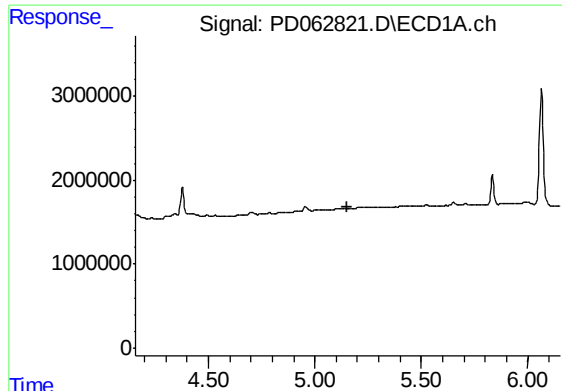

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
AST2-COPR2-1

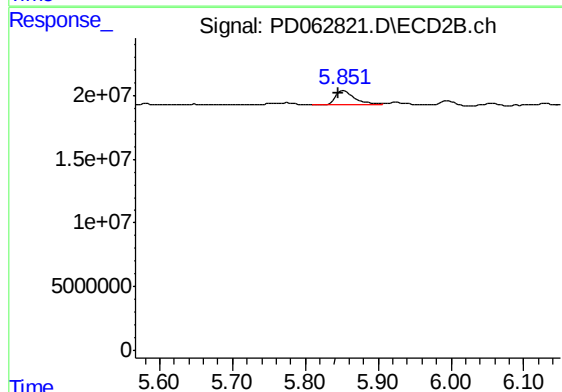


#8 Heptachlor epoxide

R.T.: 5.852 min
Delta R.T.: 0.007 min
Response: 21370103
Conc: 1.34 ng/ml

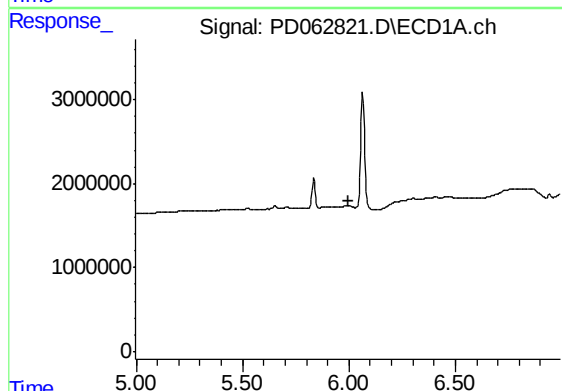


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

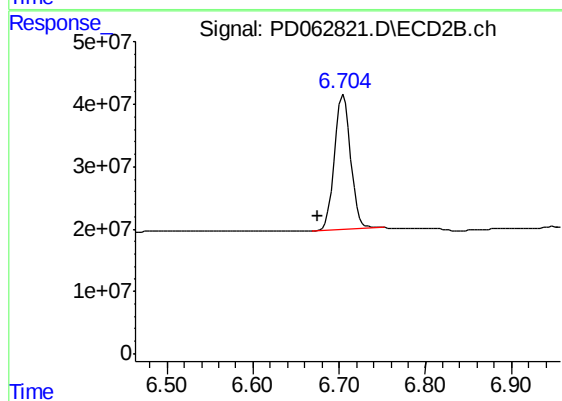

#14 Endrin


R.T.: 6.705 min
Delta R.T.: 0.029 min
Response: 282816612
Conc: 20.12 ng/ml

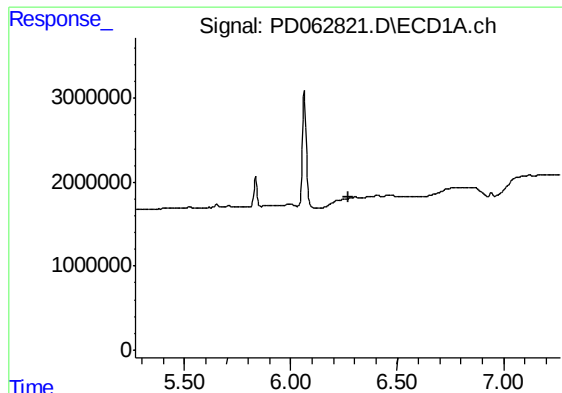

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
AST2-COPR2-1

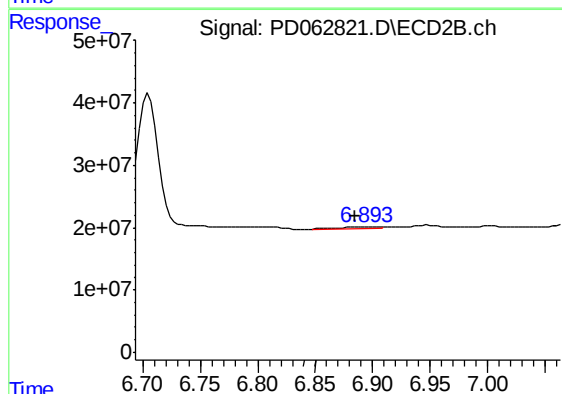


#15 Endosulfan II

R.T.: 6.894 min
Delta R.T.: 0.010 min
Response: 6190720
Conc: 0.46 ng/ml

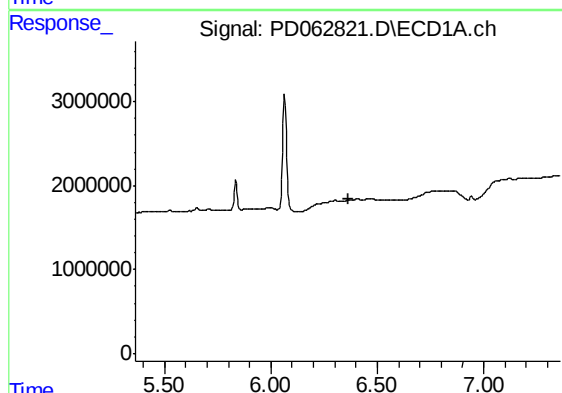


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

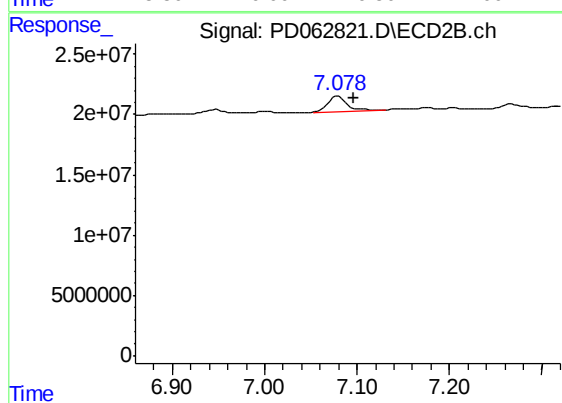

#17 4,4'-DDT


R.T.: 7.079 min
Delta R.T.: -0.018 min
Response: 18772825
Conc: 1.47 ng/ml

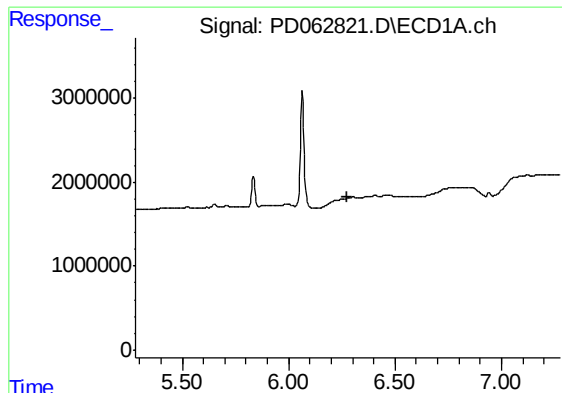

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
AST2-COPR2-1

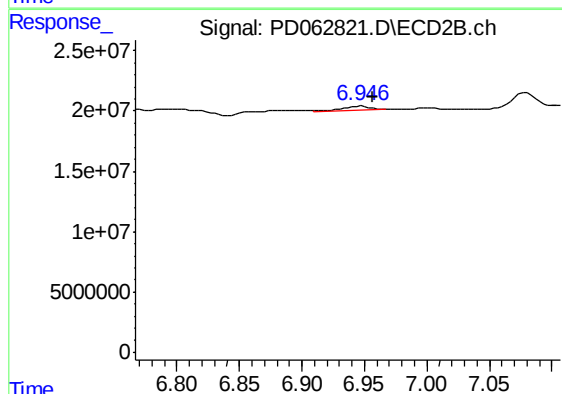


#27 Chlordane-5

R.T.: 6.948 min
Delta R.T.: -0.009 min
Response: 5251929
Conc: 10.68 ng/ml

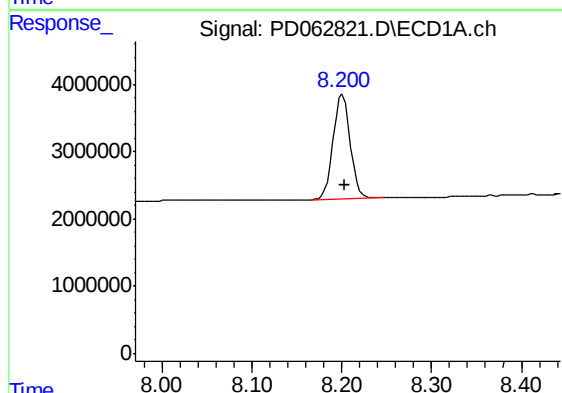

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.002 min
Response: 20558438
Conc: 19.42 ng/ml

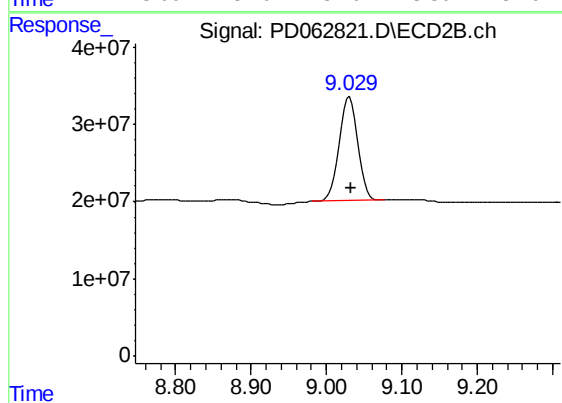

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.001 min
Response: 227755819
Conc: 19.74 ng/ml