

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 19:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 08:03:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	21090064	261.7E6	23.718	22.608
28)	SA Decachlor...	8.201	9.031	25771872	279.7E6	24.343	24.242
Target Compounds							
5)	MB Aldrin	0.000	5.463	0	122542	N.D.	0.007 #
7)	B delta-BHC	0.000	5.007f	0	19647844	N.D.	1.088 #
8)	B Heptachlo...	0.000	5.838	0	35983401	N.D.	2.253 #
14)	MA Endrin	0.000	6.675	0	48540214	N.D.	3.452 #
17)	MA 4,4'-DDT	0.000	7.095	0	5260390	N.D.	0.413 #
18)	B Endrin al...	6.467f	0.000	1437004	0	1.540	N.D. #
21)	B Endrin ke...	0.000	7.722f	0	4035926	N.D.	0.297 #
23)	Chlordane-1	0.000	4.959	0	1354102	N.D.	2.361 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 19:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 08:03:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

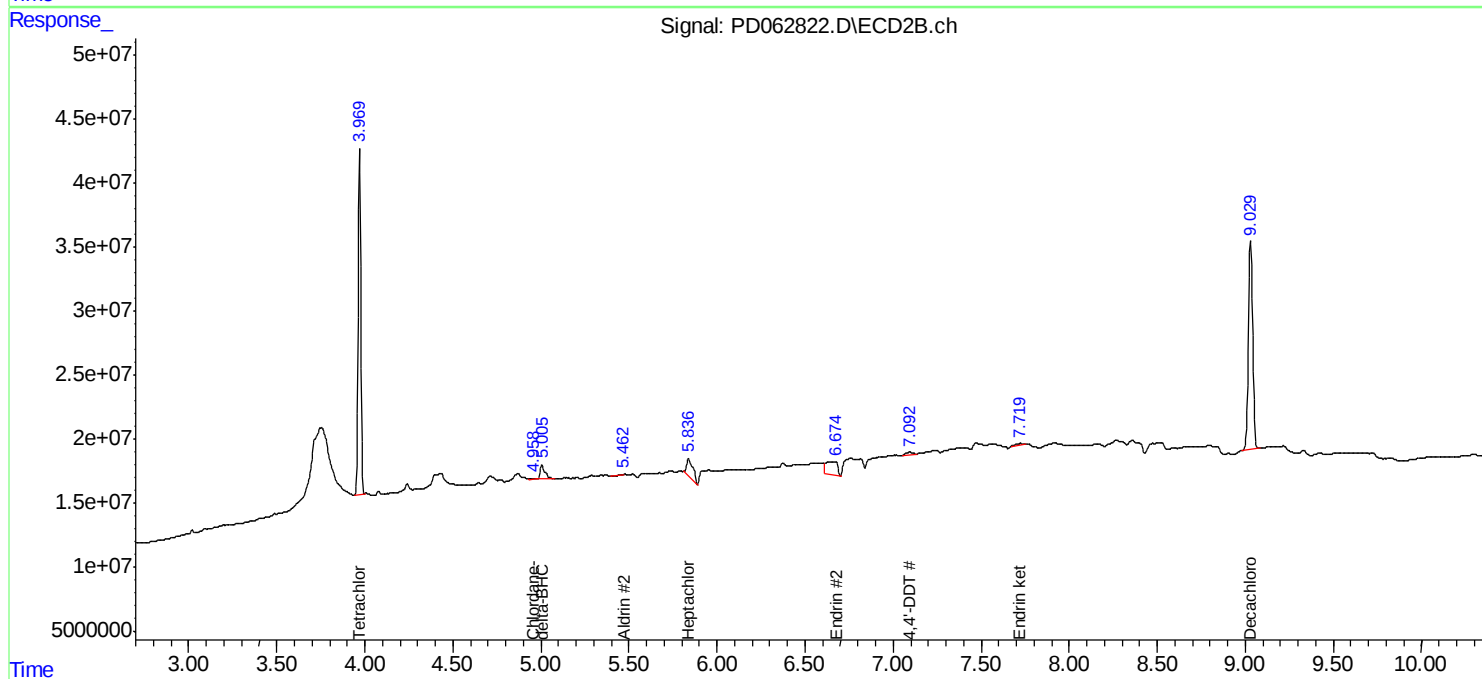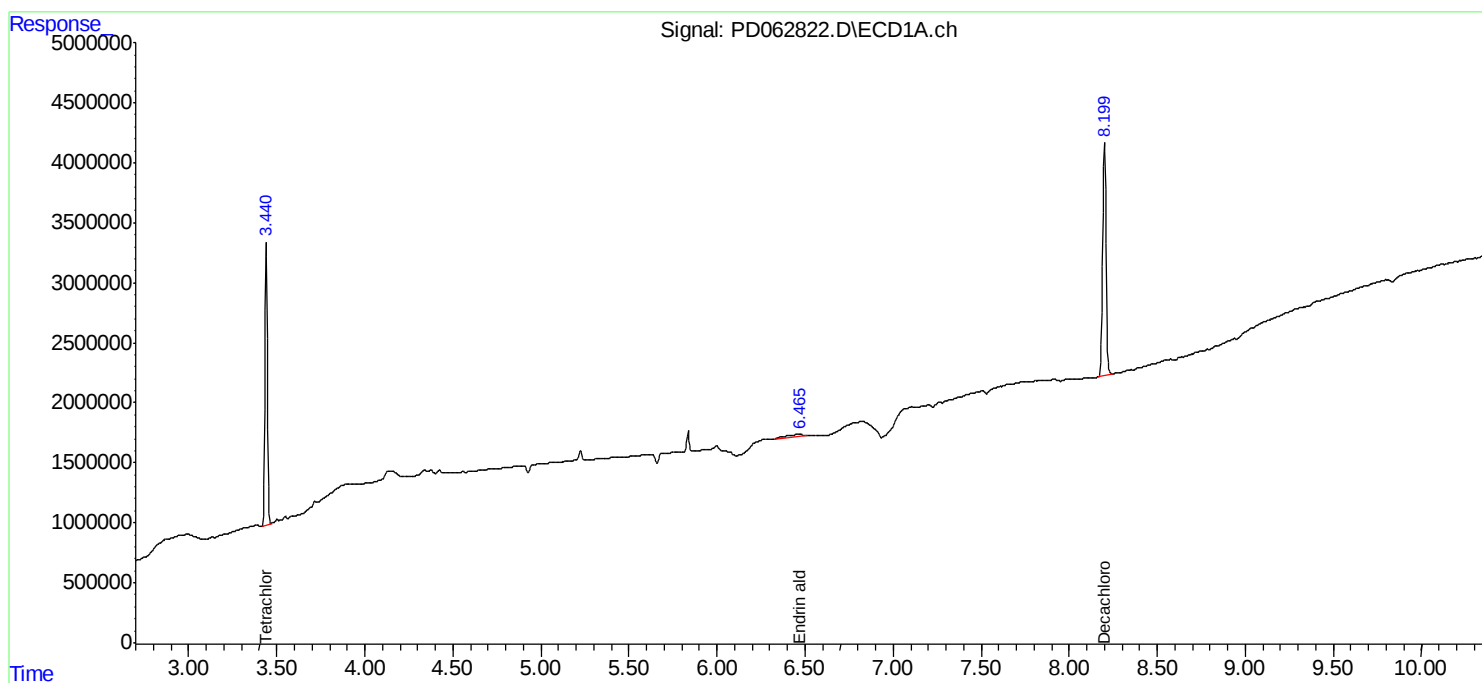


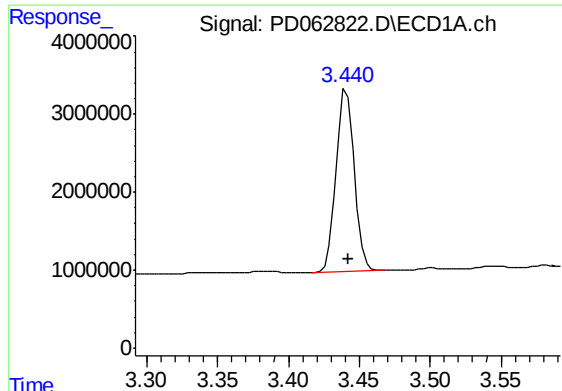

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 21090064
Conc: 23.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

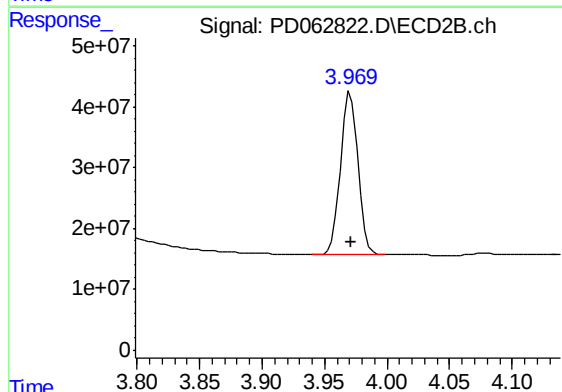


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 261735942
Conc: 22.61 ng/ml

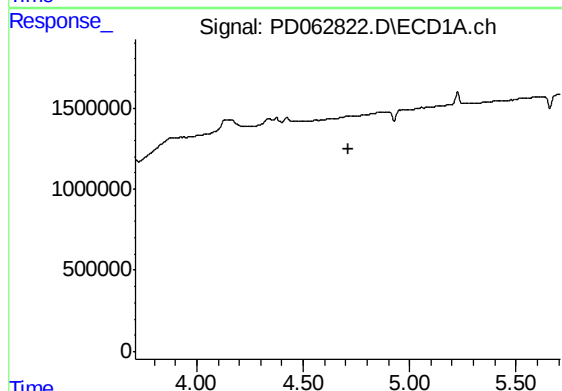


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

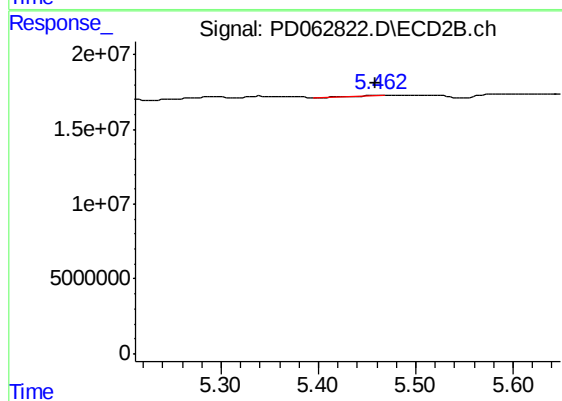

#5 Aldrin


R.T.: 5.463 min
Delta R.T.: 0.005 min
Response: 122542
Conc: 0.01 ng/ml

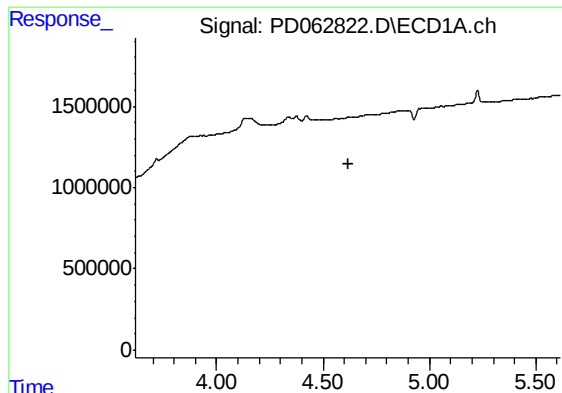

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

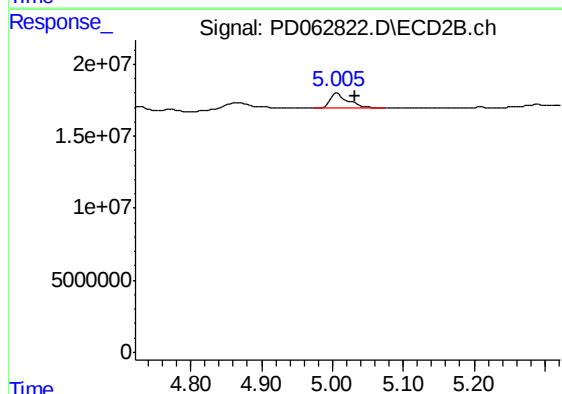


#7 delta-BHC

R.T.: 5.007 min
Delta R.T.: -0.025 min
Response: 19647844
Conc: 1.09 ng/ml

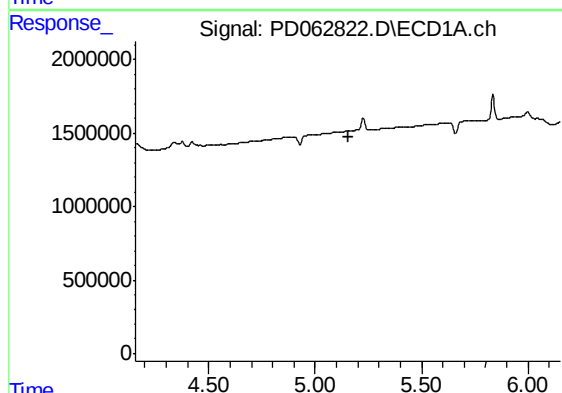


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

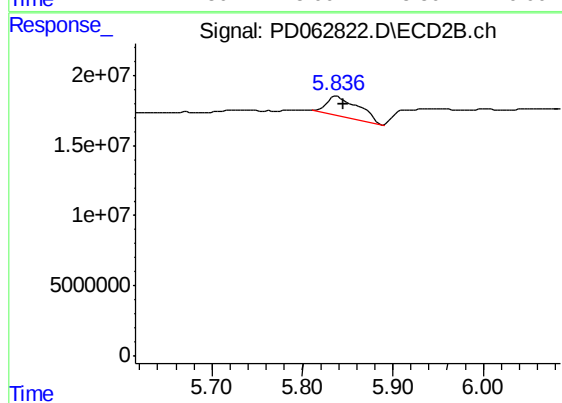

#8 Heptachlor epoxide


R.T.: 5.838 min
Delta R.T.: -0.007 min
Response: 35983401
Conc: 2.25 ng/ml

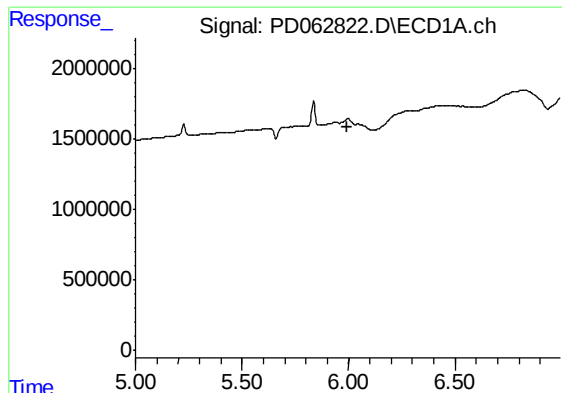

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

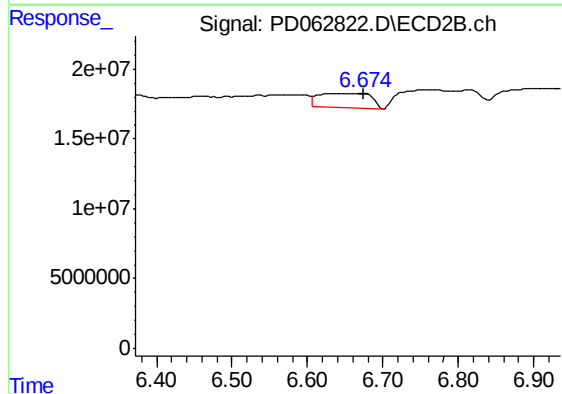


#14 Endrin

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 48540214
Conc: 3.45 ng/ml

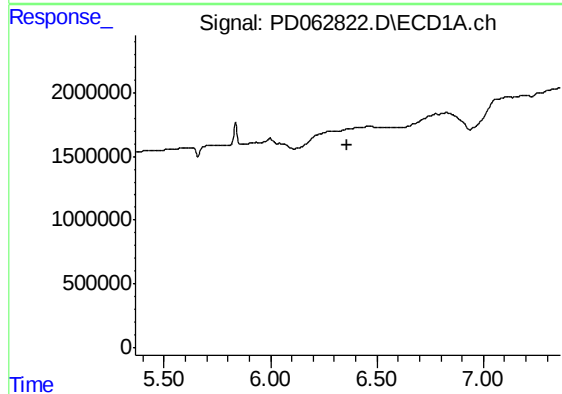


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

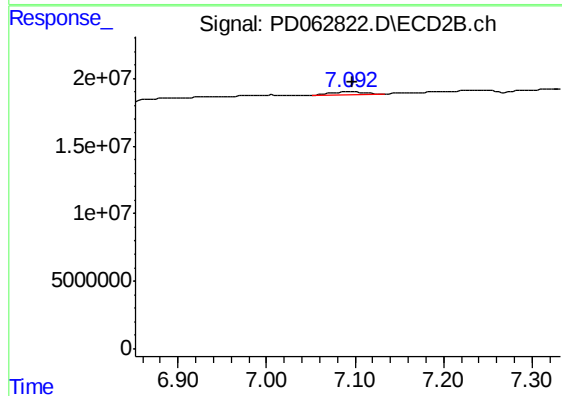

#17 4,4'-DDT


R.T.: 7.095 min
Delta R.T.: -0.001 min
Response: 5260390
Conc: 0.41 ng/ml

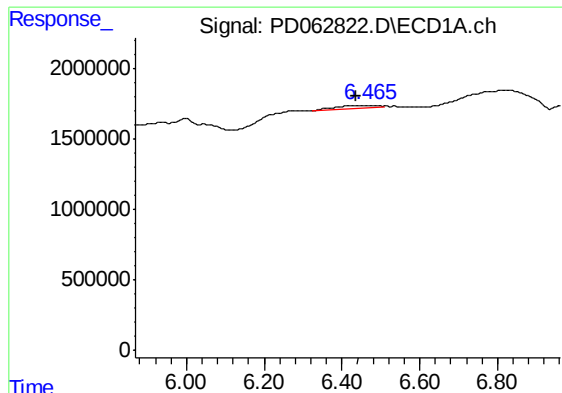

#18 Endrin aldehyde


R.T.: 6.467 min
Delta R.T.: 0.030 min
Response: 1437004
Conc: 1.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

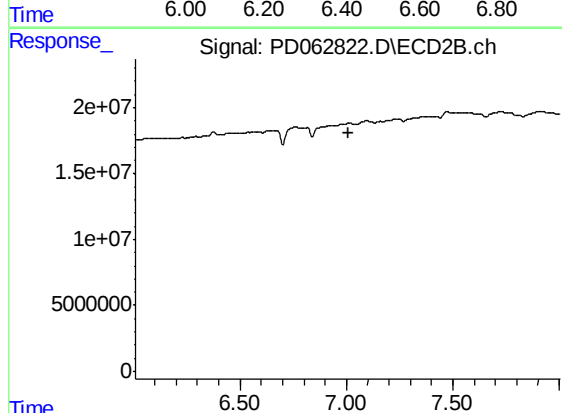


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

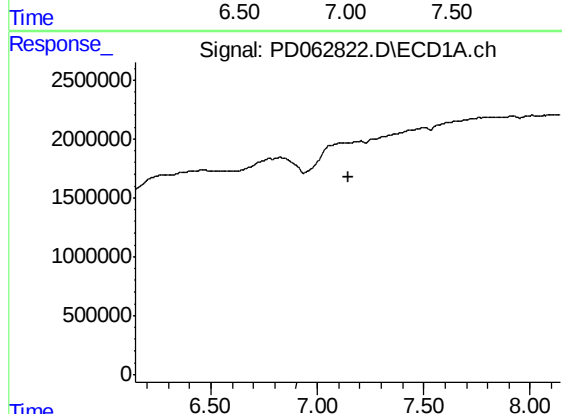


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

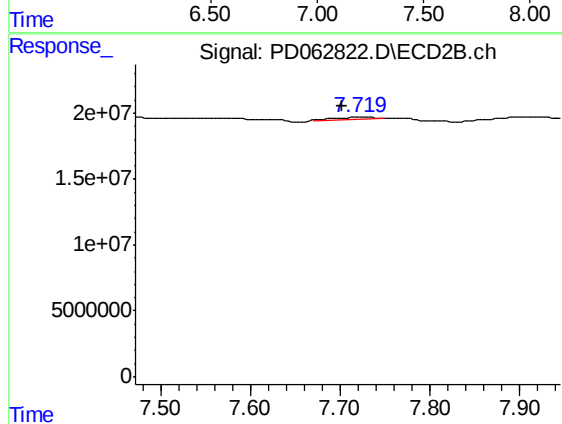

#21 Endrin ketone


R.T.: 7.722 min
Delta R.T.: 0.019 min
Response: 4035926
Conc: 0.30 ng/ml

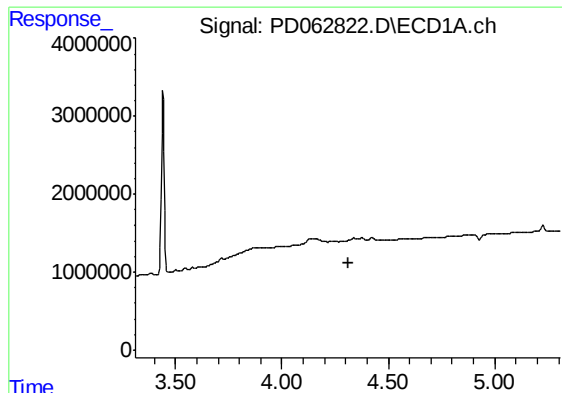

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.311 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

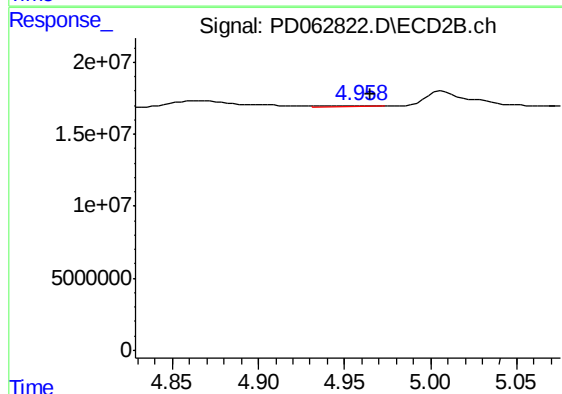


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 1354102
Conc: 2.36 ng/ml

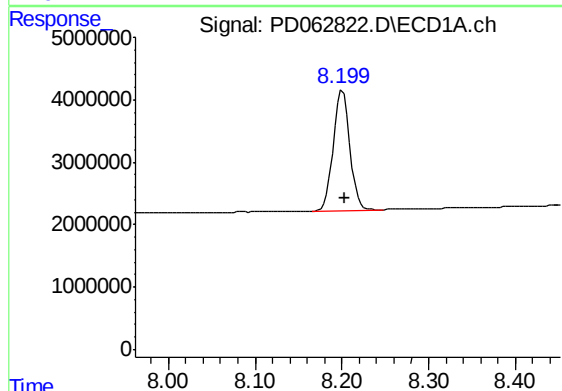

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.003 min
Response: 25771872
Conc: 24.34 ng/ml

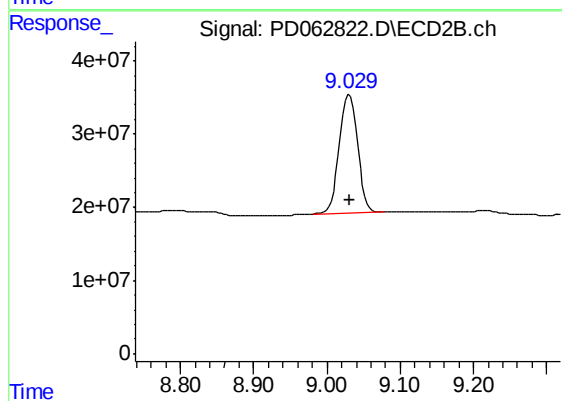

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.001 min
Response: 279724889
Conc: 24.24 ng/ml