

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 22:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 08:08:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	21349940	254.4E6	24.010	21.977
28)	SA Decachlor...	8.202	9.030	23898443	260.7E6	22.573	22.595
Target Compounds							
7)	B delta-BHC	0.000	5.027	0 17331392	N.D.	0.960	#
8)	B Heptachlo...	0.000	5.839	0 50996686	N.D.	3.192	#
14)	MA Endrin	5.998	0.000	813094	0	0.732	N.D. #
15)	B Endosulfa...	0.000	6.900f	0 6588688	N.D.	0.493	#
17)	MA 4,4'-DDT	0.000	7.104	0 4825607	N.D.	0.379	#
21)	B Endrin ke...	0.000	7.726f	0 7276623	N.D.	0.536	#
23)	Chlordane-1	4.338f	0.000	289478	0	8.209	N.D. #
27)	Chlordane-5	0.000	6.949	0 2049130	N.D.	4.166	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 22:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 08:08:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

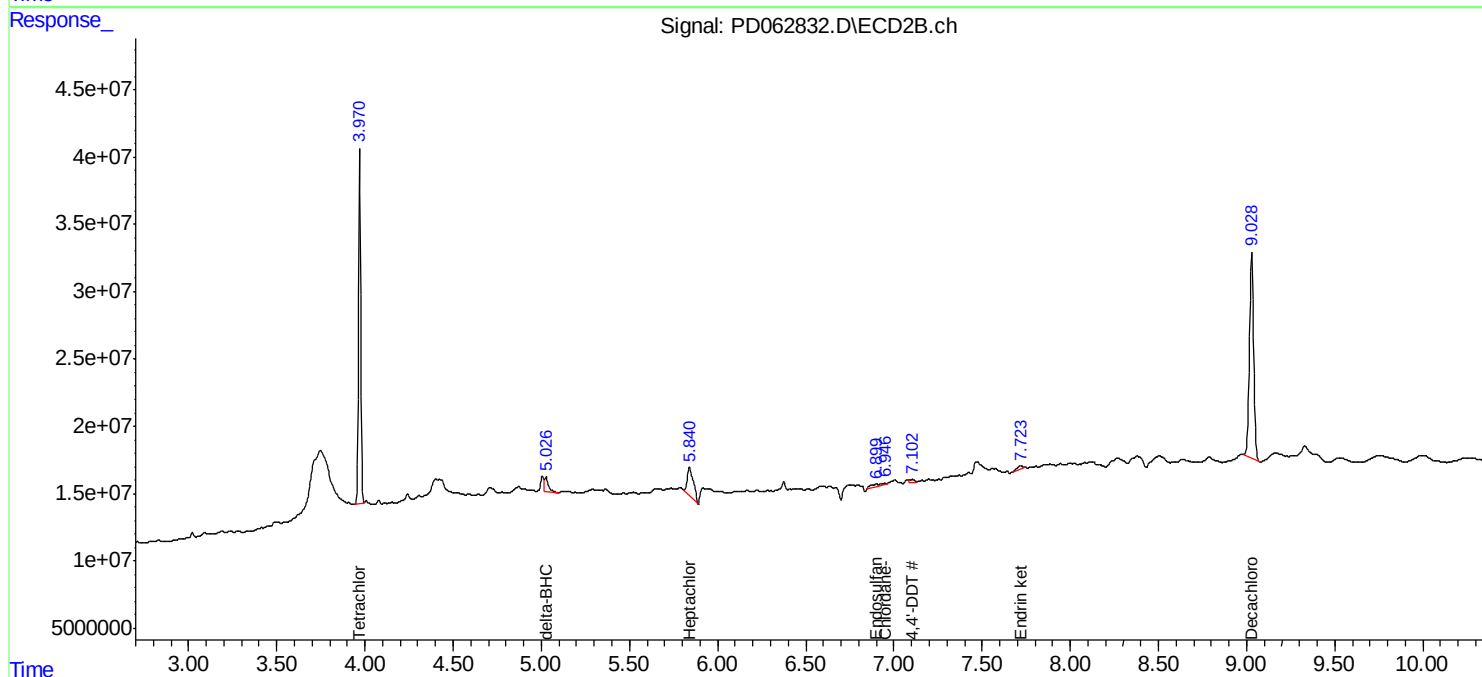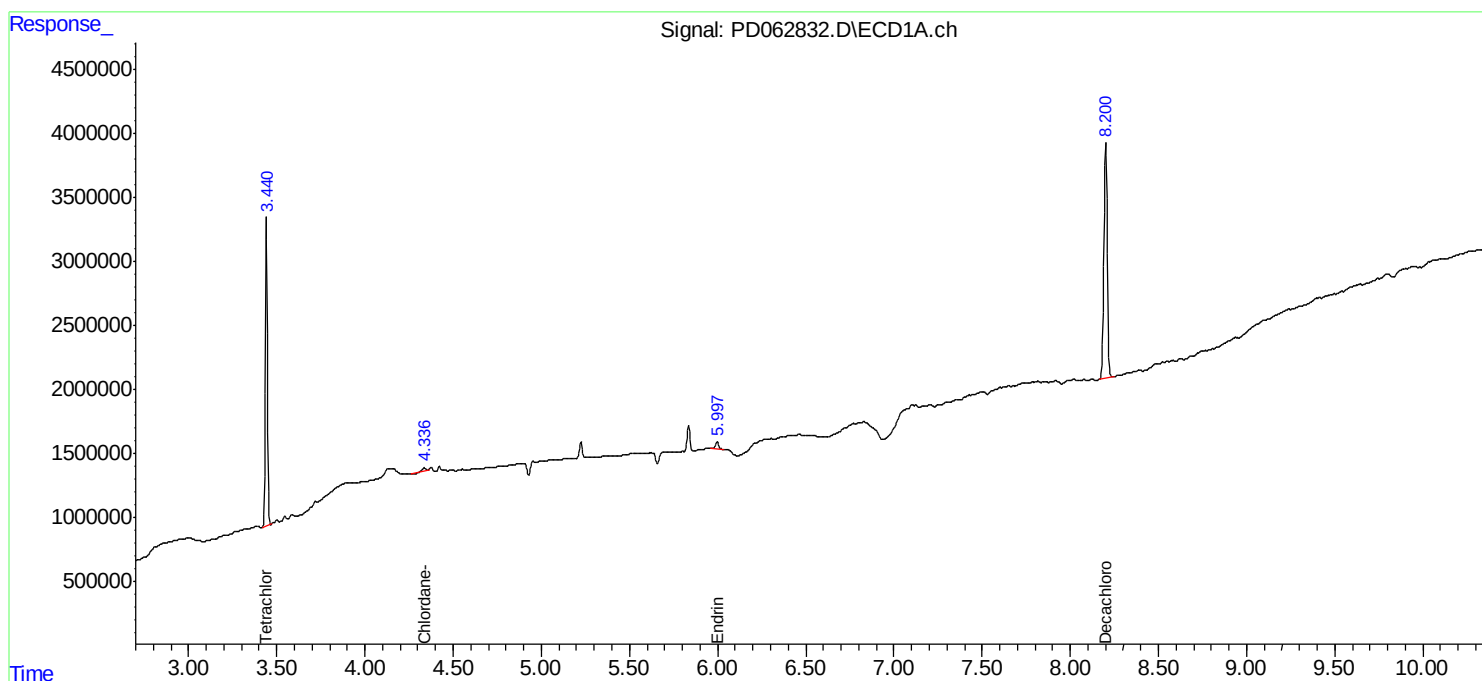


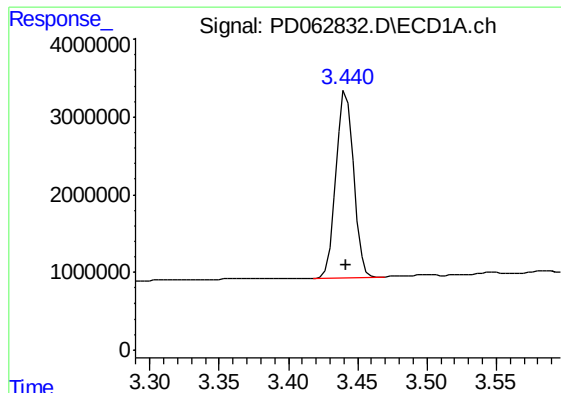

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 21349940
Conc: 24.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

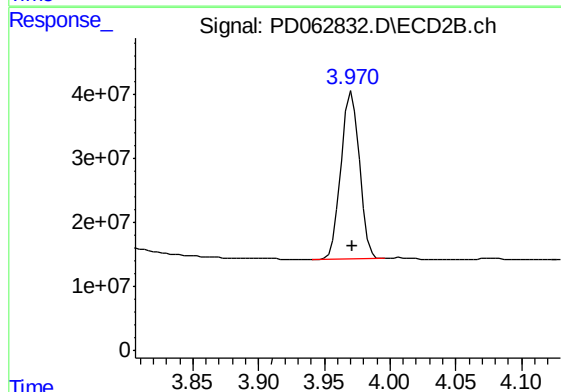


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 254423762
Conc: 21.98 ng/ml

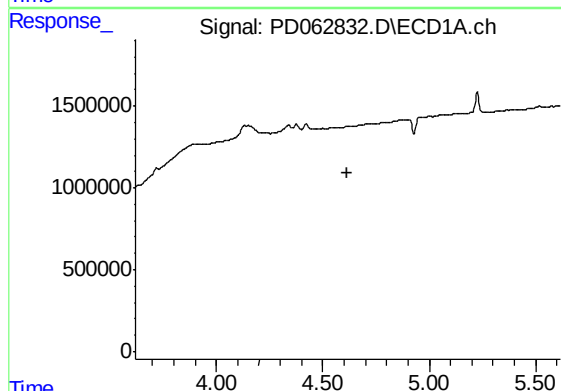


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

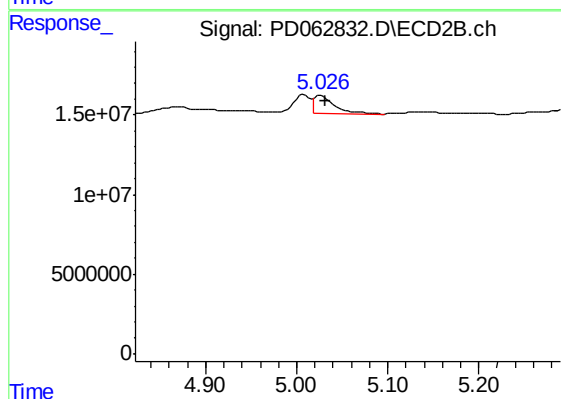

#7 delta-BHC


R.T.: 5.027 min
Delta R.T.: -0.005 min
Response: 17331392
Conc: 0.96 ng/ml

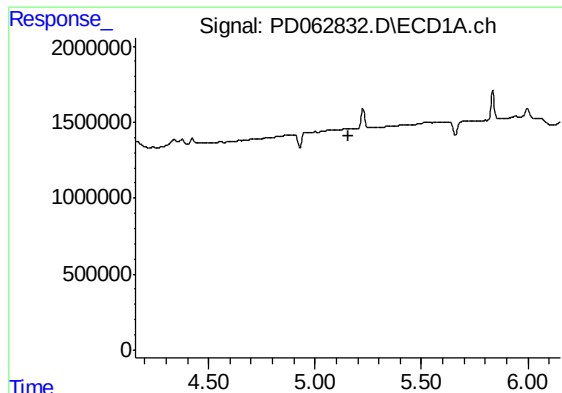

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

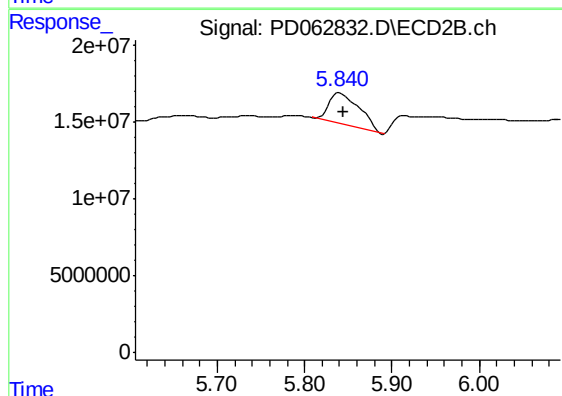


#8 Heptachlor epoxide

R.T.: 5.839 min
Delta R.T.: -0.005 min
Response: 50996686
Conc: 3.19 ng/ml

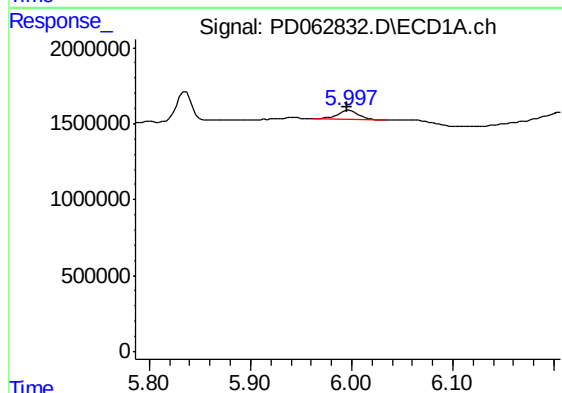


#14 Endrin

R.T.: 5.998 min
Delta R.T.: 0.002 min
Response: 813094
Conc: 0.73 ng/ml

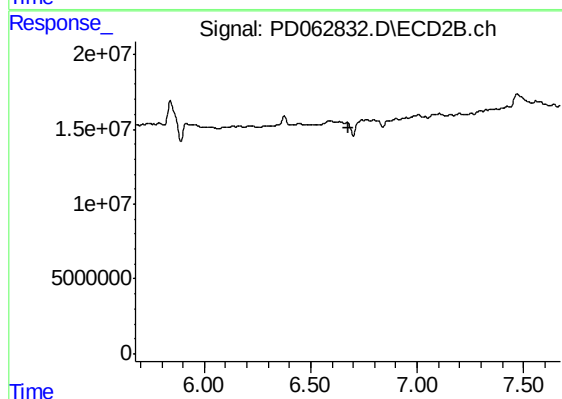

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.676 min
Response: 0
Conc: N.D.

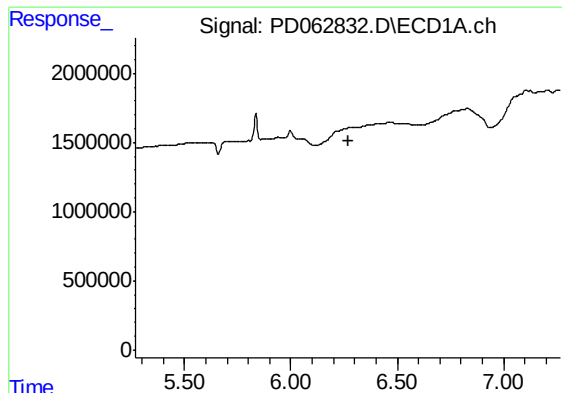

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

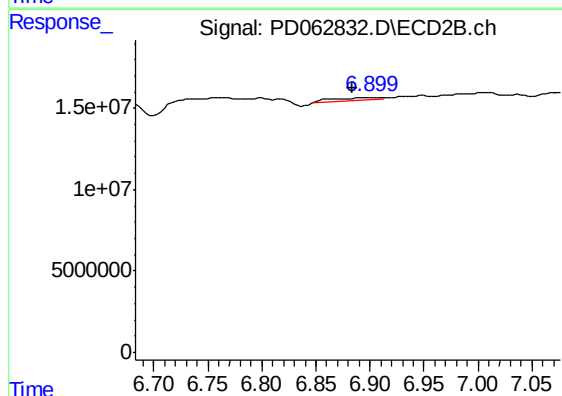


#15 Endosulfan II

R.T.: 6.900 min
Delta R.T.: 0.016 min
Response: 6588688
Conc: 0.49 ng/ml

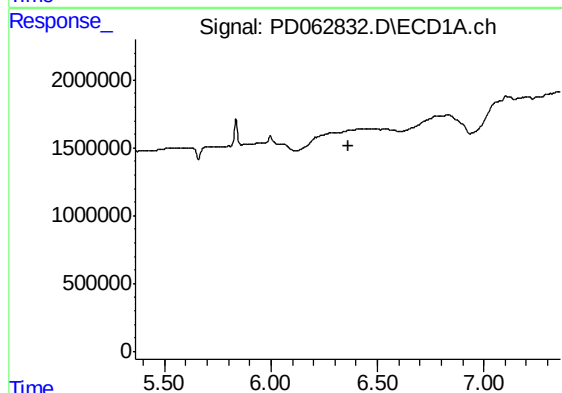


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

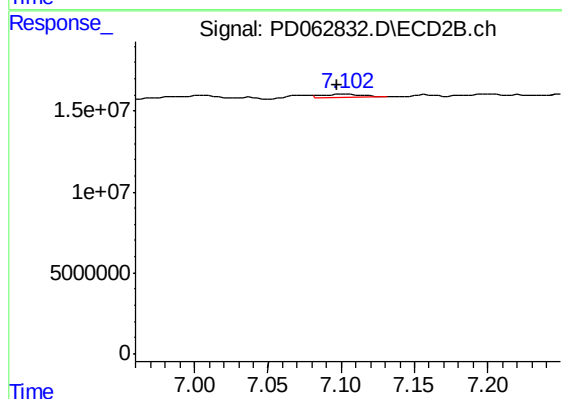

#17 4,4'-DDT


R.T.: 7.104 min
Delta R.T.: 0.007 min
Response: 4825607
Conc: 0.38 ng/ml

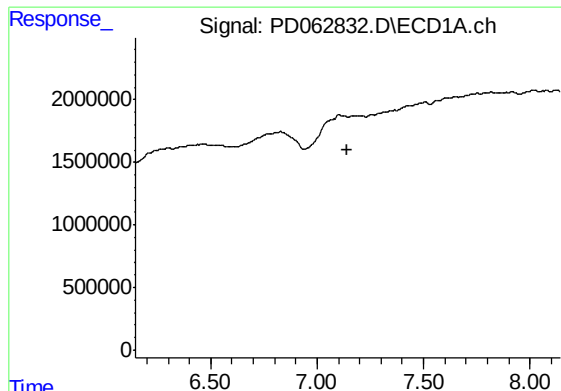

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

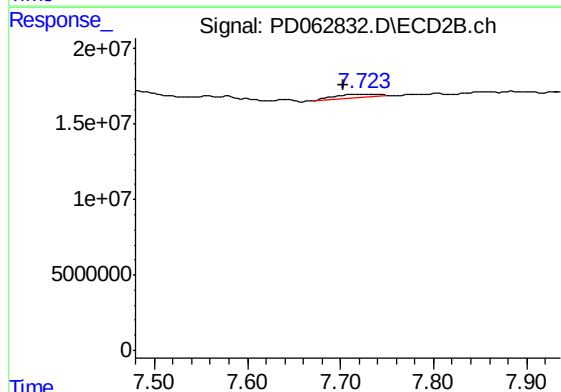


#21 Endrin ketone

R.T.: 7.726 min
Delta R.T.: 0.023 min
Response: 7276623
Conc: 0.54 ng/ml

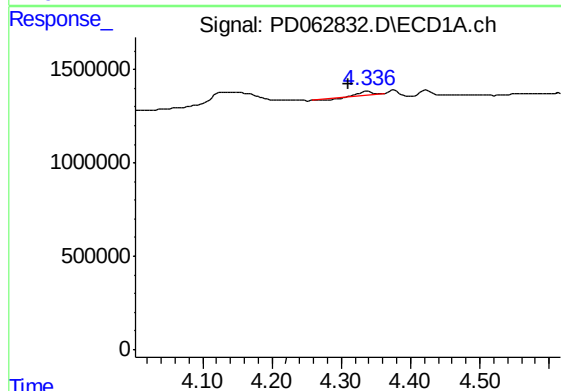


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.027 min
Response: 289478
Conc: 8.21 ng/ml

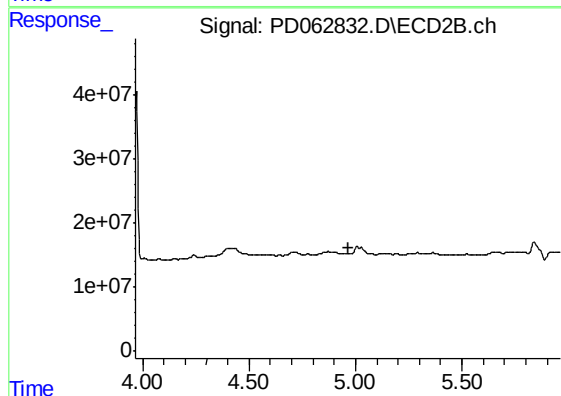

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

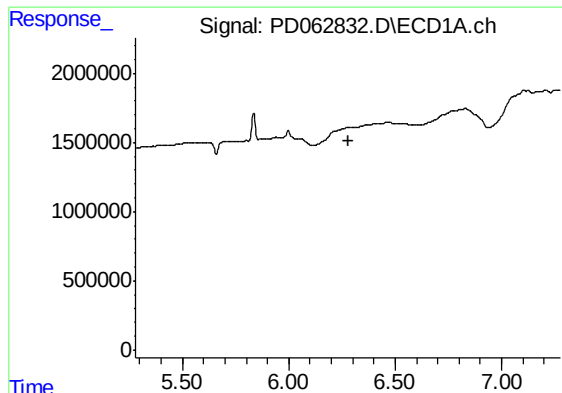

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

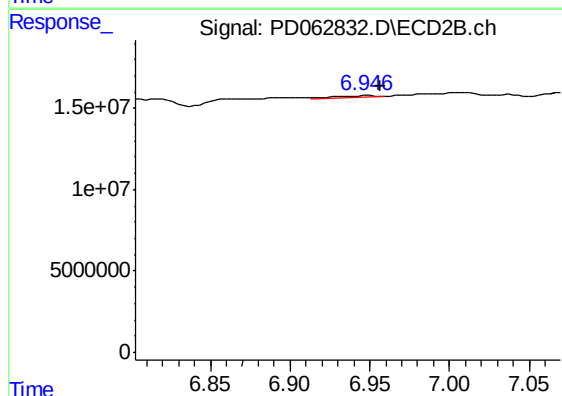


#27 Chlordane-5

R.T.: 6.949 min
Delta R.T.: -0.008 min
Response: 2049130
Conc: 4.17 ng/ml

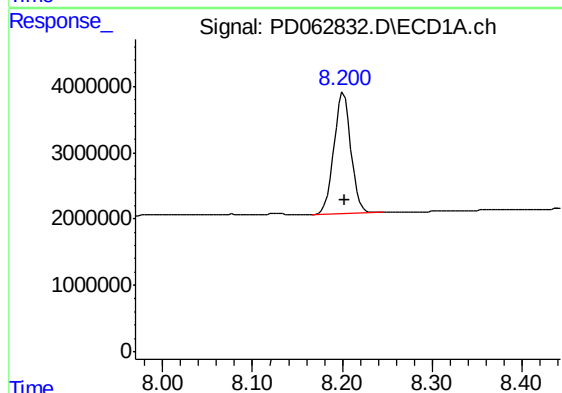

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.002 min
Response: 23898443
Conc: 22.57 ng/ml

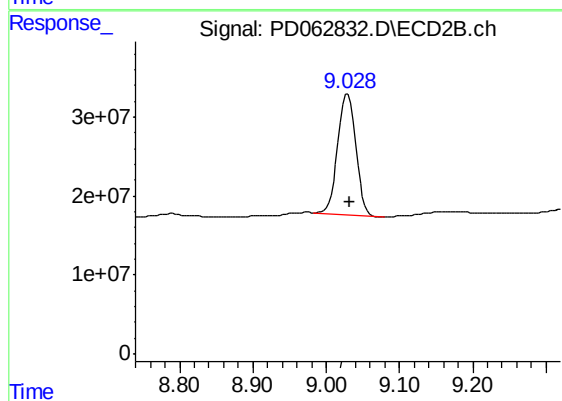

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.003 min
Response: 260720661
Conc: 22.59 ng/ml