

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 13:04
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 07:43:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 11:04:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	3.971	47585032	596.1E6	50.856	49.115
7) SA Decachlor...	8.203	9.031	56942872	622.8E6	50.861	52.591
Target Compounds						
2) Toxaphene-1	5.700	6.547	3733981	76711963	485.065	515.277
3) Toxaphene-2	6.183	7.054	4356388	64834820	523.827	520.821
4) Toxaphene-3	6.302	7.131	9599937	178.8E6	505.569	495.125
5) Toxaphene-4	6.548	7.216	10161871	112.6E6	519.508	503.526
6) Toxaphene-5	7.036	7.630	11196623	79607118	505.407	502.834

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 13:04
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 07:43:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 11:04:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

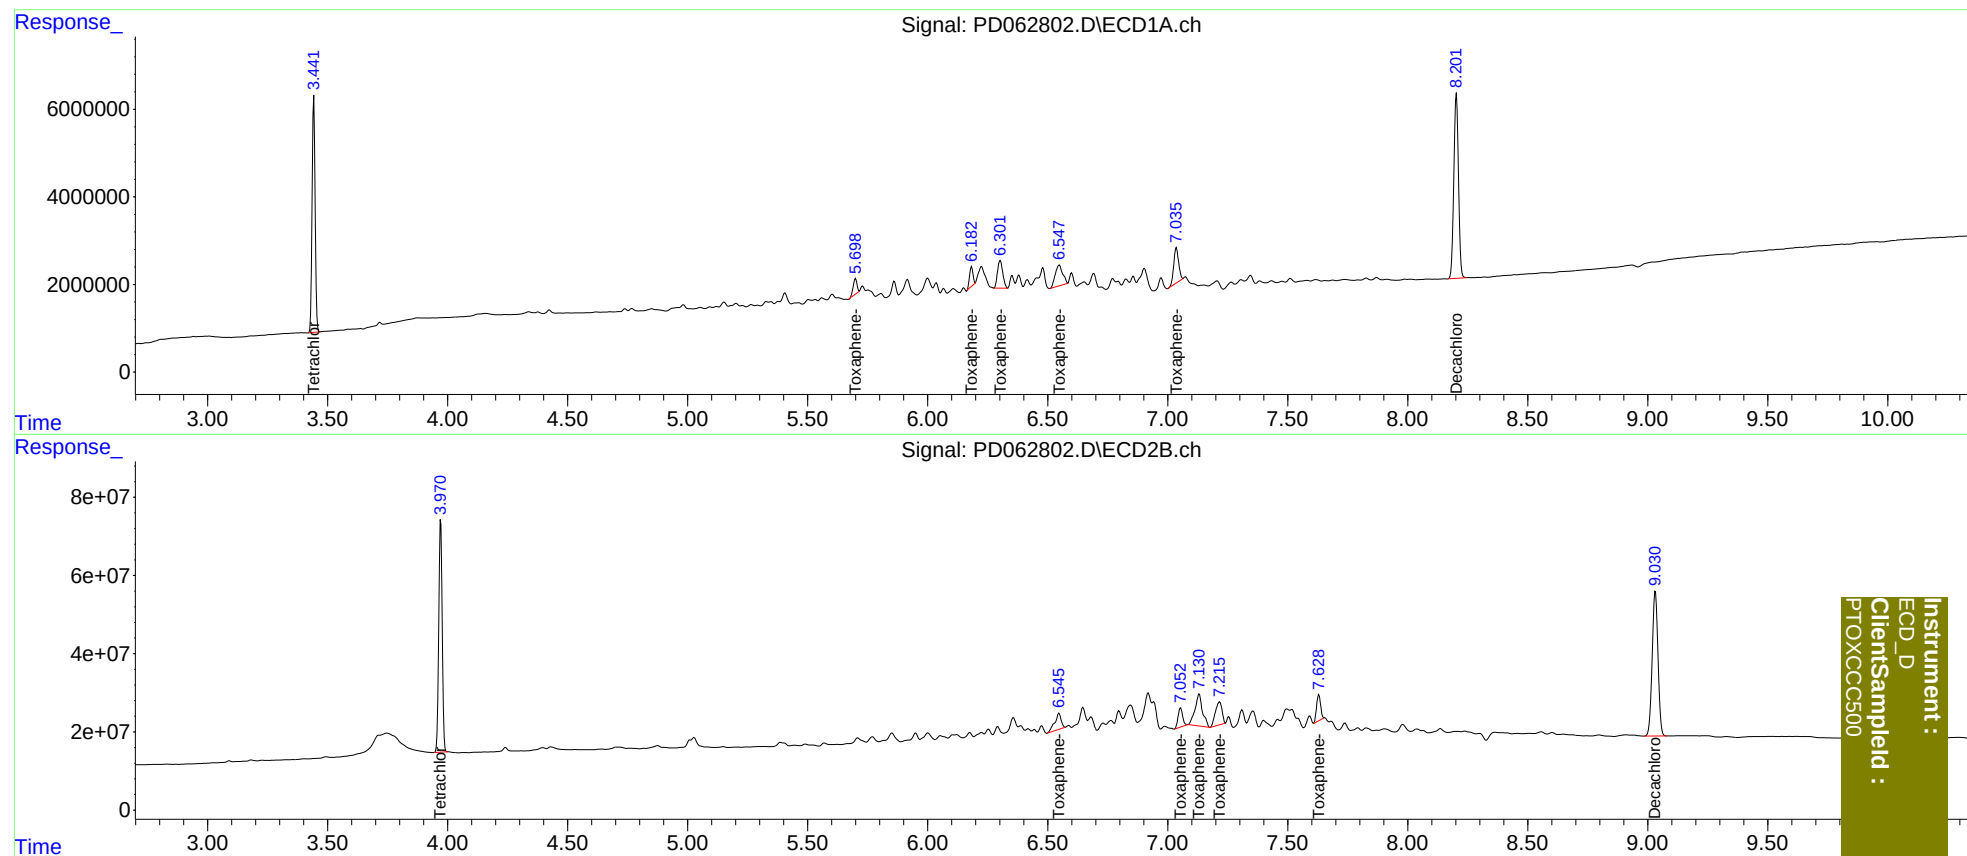

Instrument :
ECD_D
Client Sample :
PTOXC500