

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 12:50
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 07:22:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	3.971	52520220	558.0E6	59.064	48.198
28)	SA Decachlor...	8.207	9.033	54033873	573.1E6	51.037	49.662
Target Compounds							
23)	Chlordane-1	4.316	4.965	17607498	269.6E6	499.315	470.221
24)	Chlordane-2	4.818	5.433	20728923	256.2E6	508.960	479.801
25)	Chlordane-3	5.388	6.079	58704066	1070.3E6	495.413	478.883
26)	Chlordane-4	5.446	6.153	49252605	1228.5E6	507.890	476.311
27)	Chlordane-5	6.284	6.958	21781653	239.1E6	499.662	486.188



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 12:50
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 07:22:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

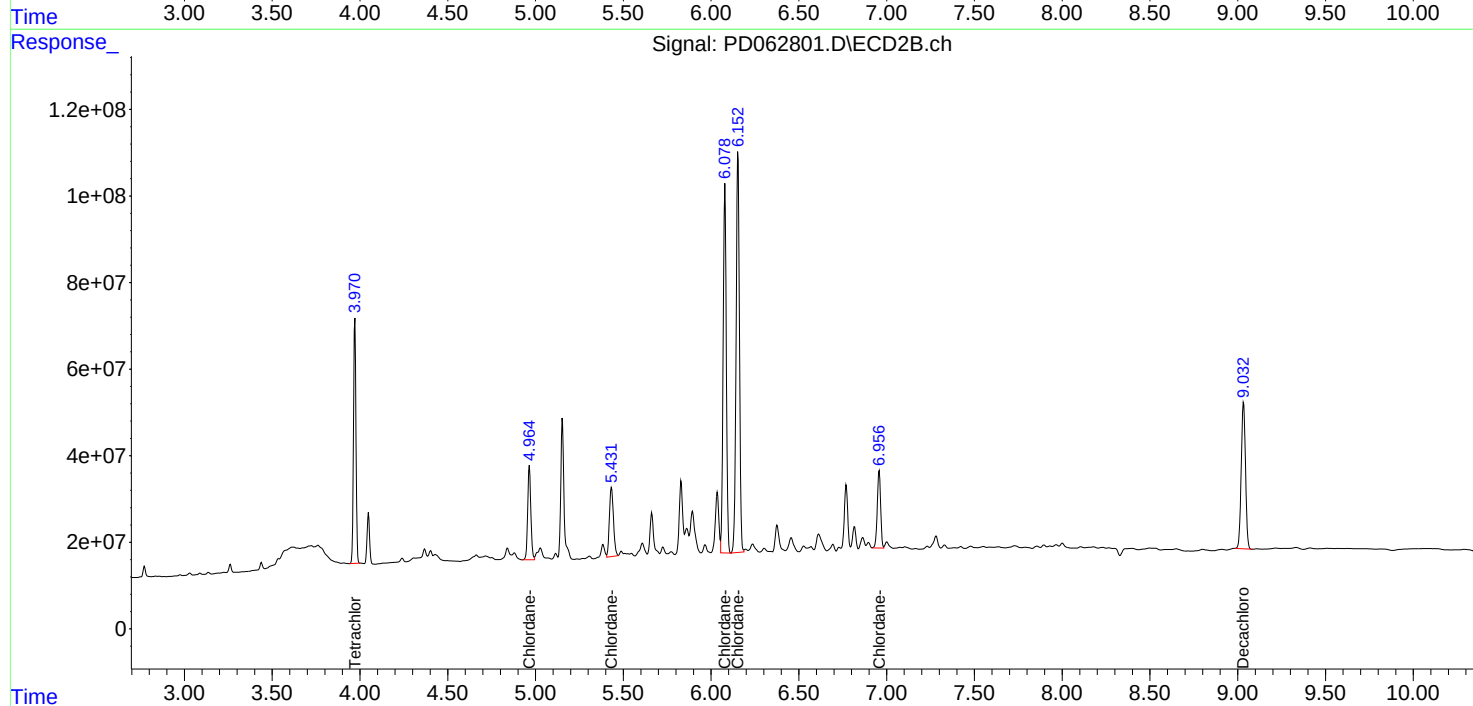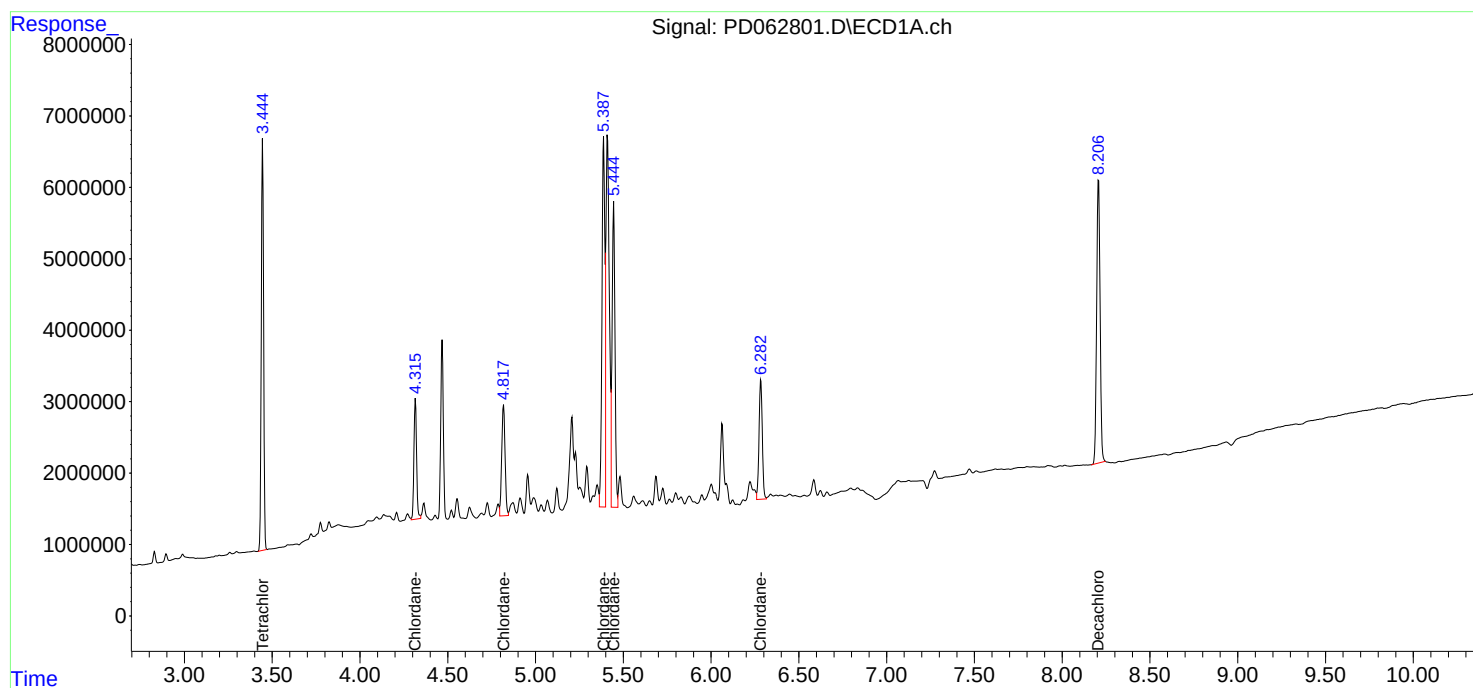


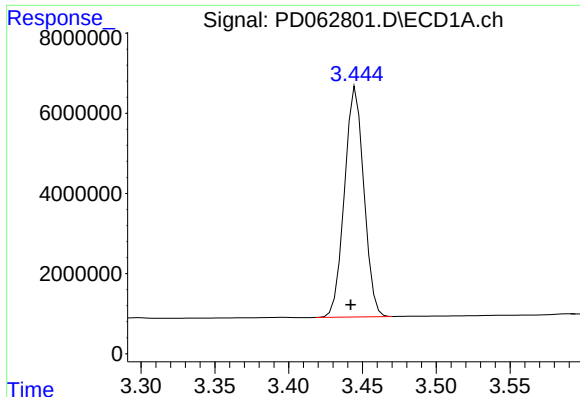

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: 0.004 min
Response: 52520220
Conc: 59.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

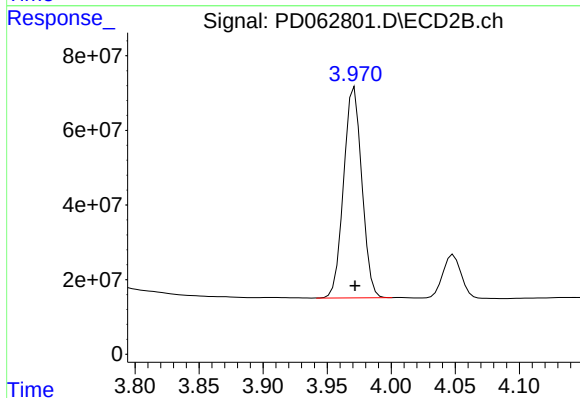


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 557991106
Conc: 48.20 ng/ml

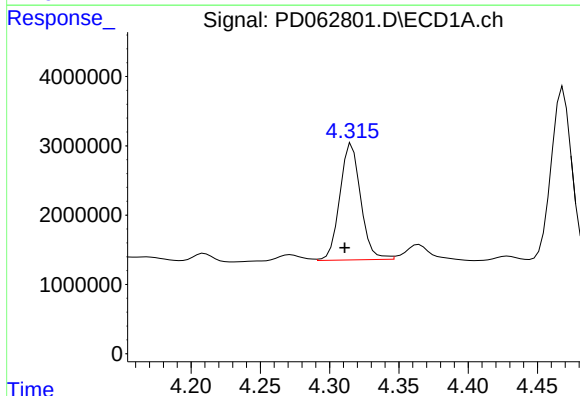


#23 Chlordane-1

R.T.: 4.316 min
Delta R.T.: 0.005 min
Response: 17607498
Conc: 499.32 ng/ml

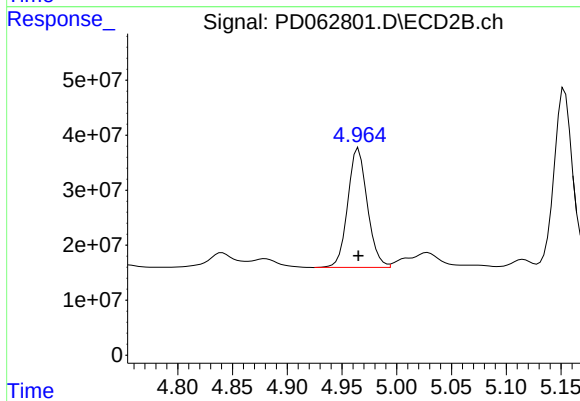

#23 Chlordane-1


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 269635866
Conc: 470.22 ng/ml

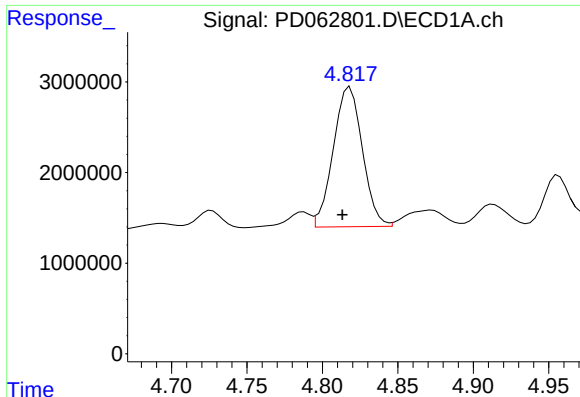

#24 Chlordane-2


R.T.: 4.818 min
Delta R.T.: 0.005 min
Response: 20728923
Conc: 508.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

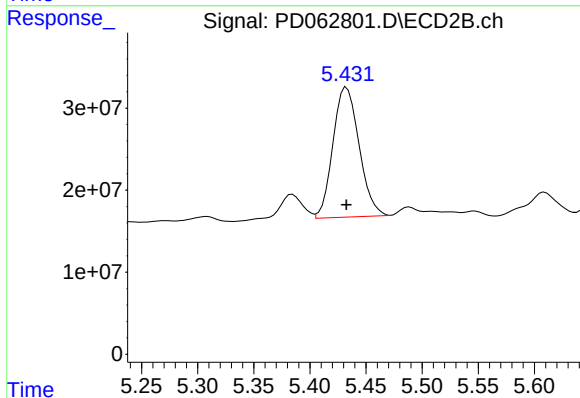


#24 Chlordane-2

R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 256151236
Conc: 479.80 ng/ml

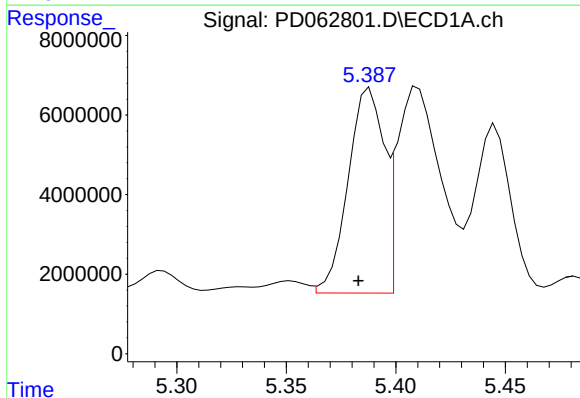


#25 Chlordane-3

R.T.: 5.388 min
Delta R.T.: 0.005 min
Response: 58704066
Conc: 495.41 ng/ml

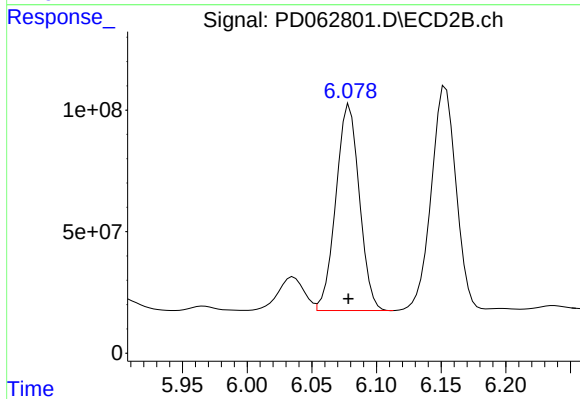

#25 Chlordane-3


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 1070260478
Conc: 478.88 ng/ml

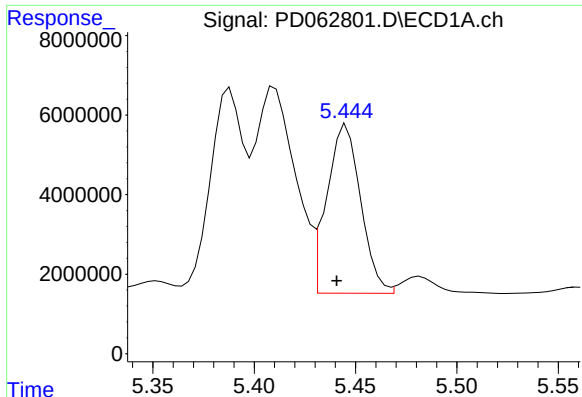

#26 Chlordane-4


R.T.: 5.446 min
Delta R.T.: 0.005 min
Response: 49252605
Conc: 507.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

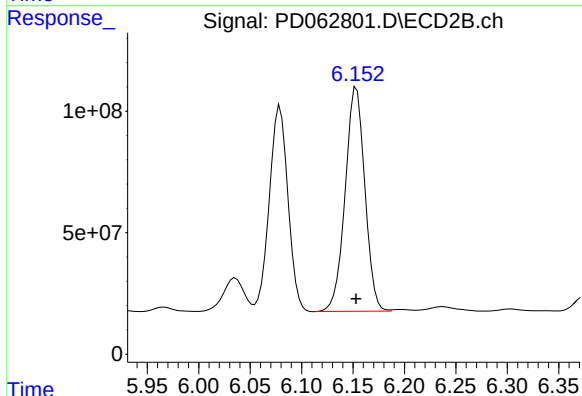


#26 Chlordane-4

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 1228547058
Conc: 476.31 ng/ml

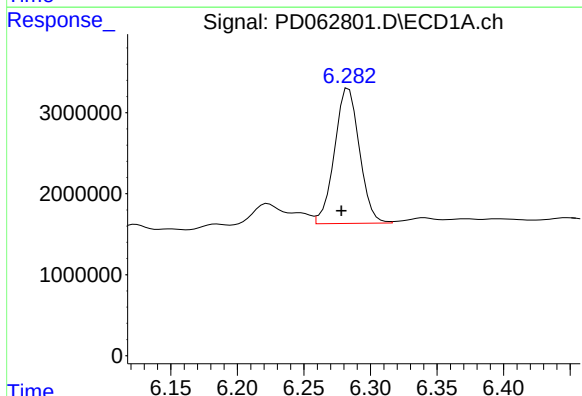


#27 Chlordane-5

R.T.: 6.284 min
Delta R.T.: 0.006 min
Response: 21781653
Conc: 499.66 ng/ml

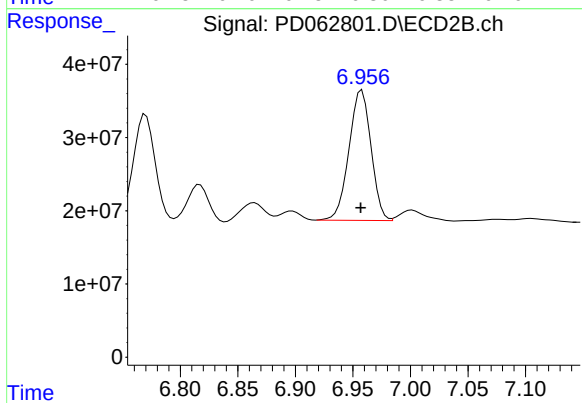

#27 Chlordane-5


R.T.: 6.958 min
Delta R.T.: 0.001 min
Response: 239128669
Conc: 486.19 ng/ml

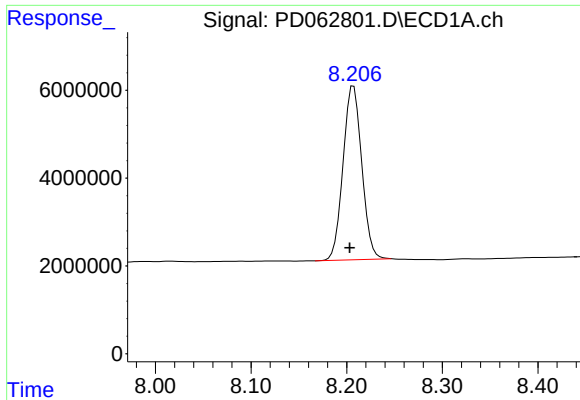

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.004 min
Response: 54033873
Conc: 51.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

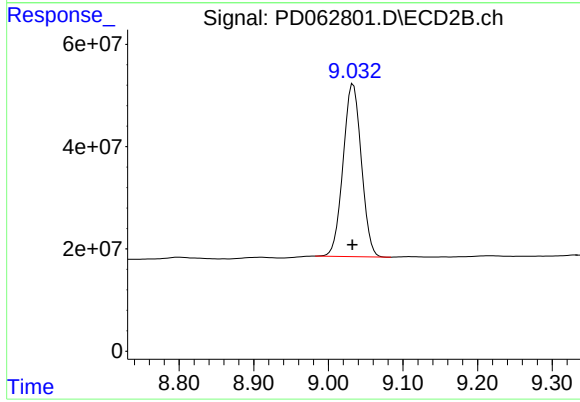

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.001 min
Response: 573054865
Conc: 49.66 ng/ml