

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 16:01
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 07:23:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	50011942	528.8E6	56.243	45.674
28)	SA Decachlor...	8.202	9.030	52484350	558.7E6	49.574	48.415
Target Compounds							
23)	Chlordane-1	4.311	4.964	16529036	258.9E6	468.732	451.439
24)	Chlordane-2	4.813	5.431	19944590	241.2E6	489.702	451.832
25)	Chlordane-3	5.382	6.077	56455441	1015.2E6	476.436	454.267
26)	Chlordane-4	5.440	6.151	46975927	1171.9E6	484.413	454.335
27)	Chlordane-5	6.278	6.955	21411669	225.5E6	491.175	458.506



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 16:01
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 07:23:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

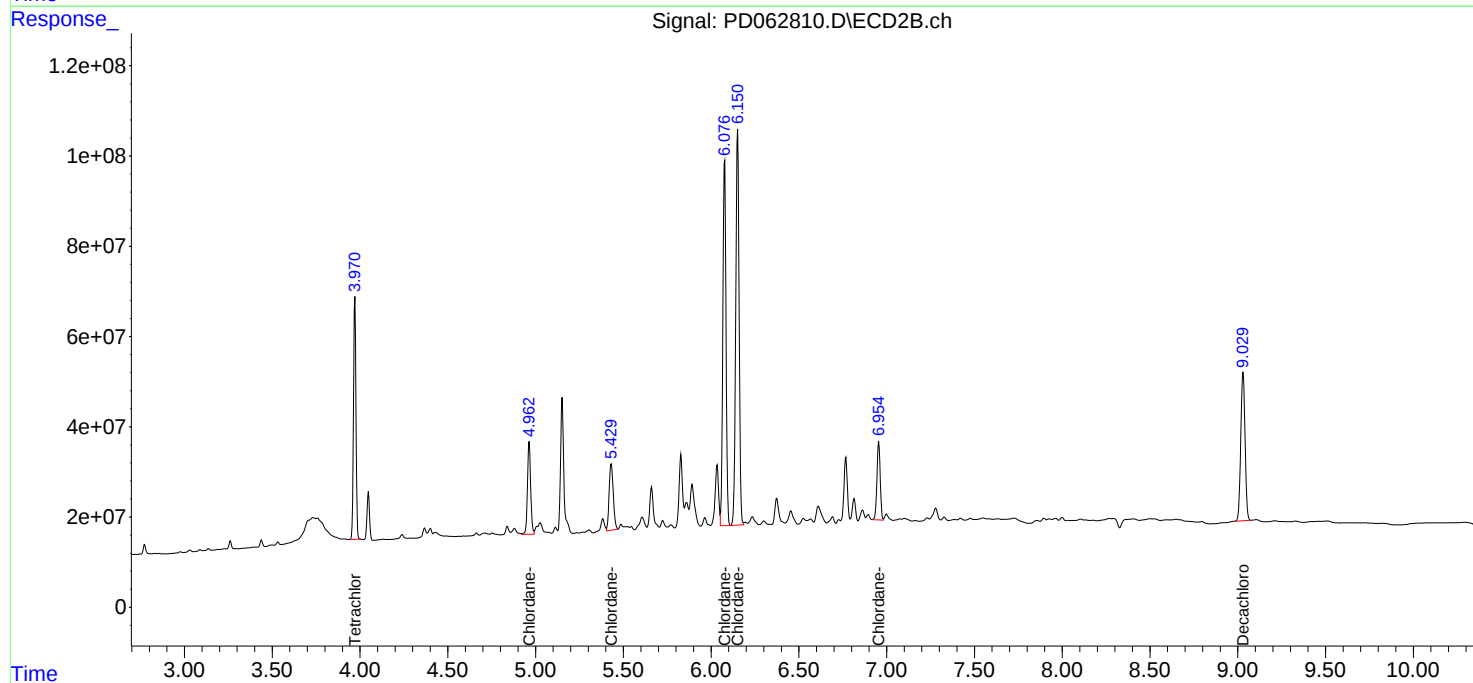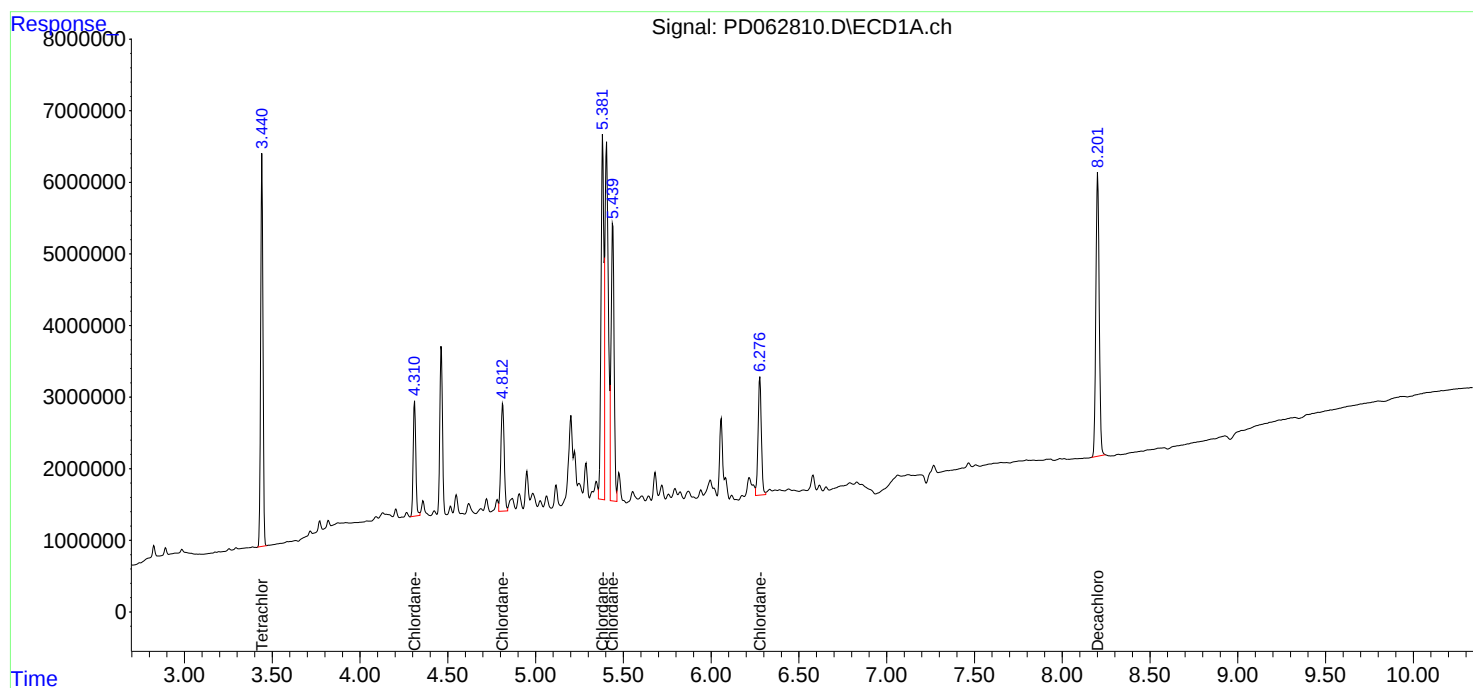


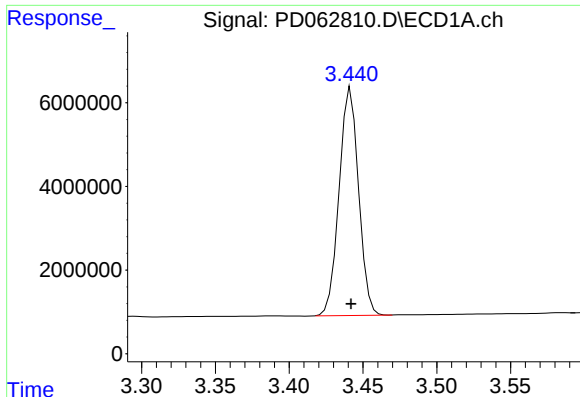

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 50011942
Conc: 56.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

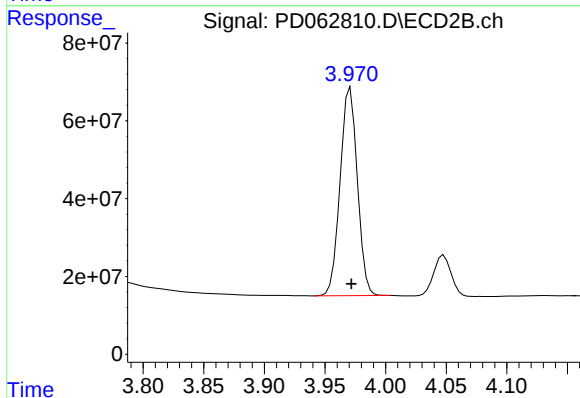


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 528765526
Conc: 45.67 ng/ml

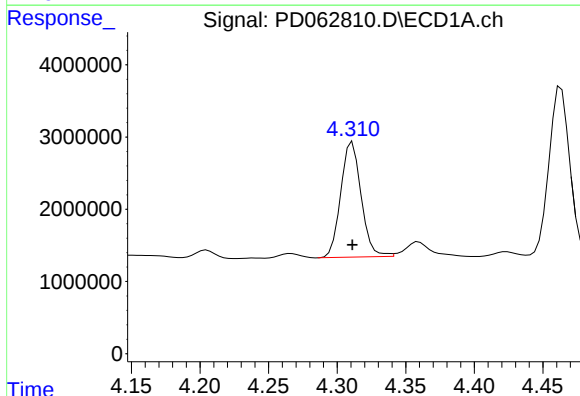


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 16529036
Conc: 468.73 ng/ml

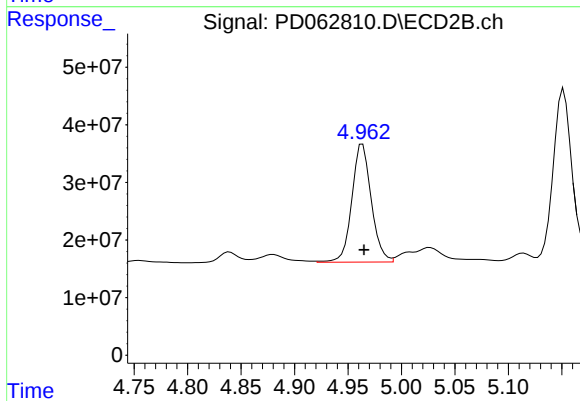

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 258865841
Conc: 451.44 ng/ml

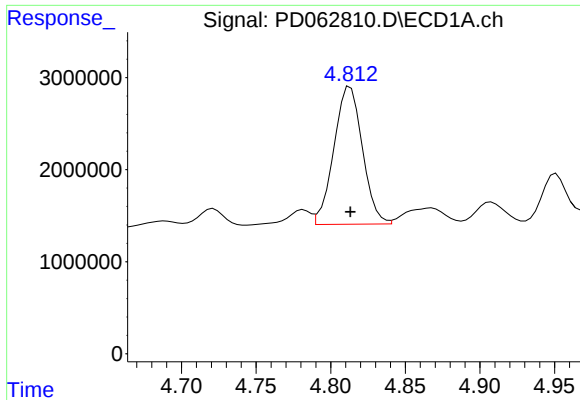

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 19944590
Conc: 489.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

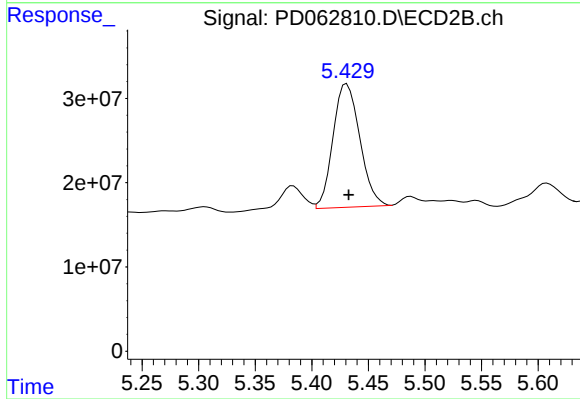


#24 Chlordane-2

R.T.: 5.431 min
Delta R.T.: -0.002 min
Response: 241219115
Conc: 451.83 ng/ml

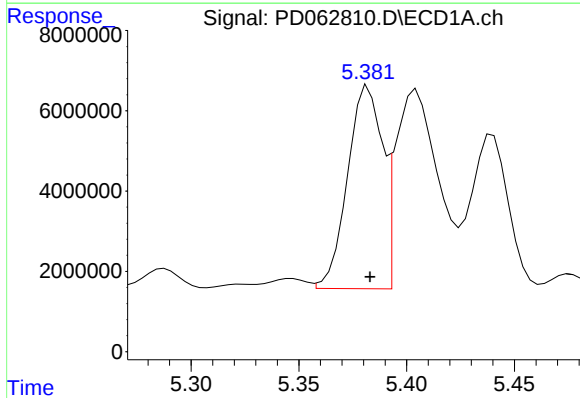


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 56455441
Conc: 476.44 ng/ml

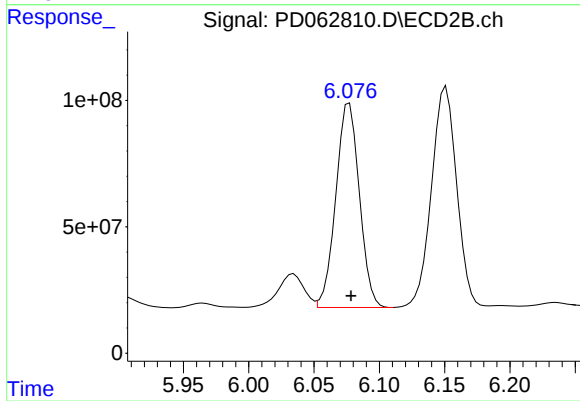

#25 Chlordane-3


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 1015246118
Conc: 454.27 ng/ml

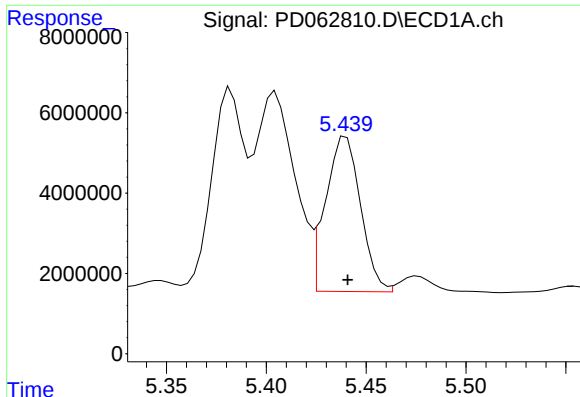

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 46975927
Conc: 484.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

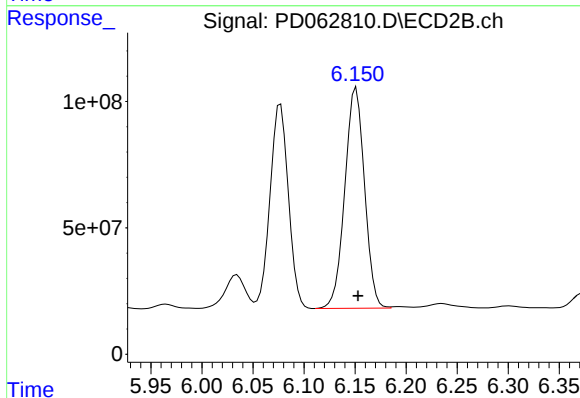


#26 Chlordane-4

R.T.: 6.151 min
Delta R.T.: -0.002 min
Response: 1171864526
Conc: 454.34 ng/ml

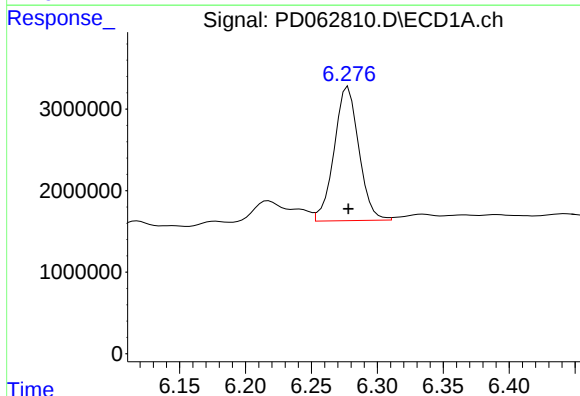


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 21411669
Conc: 491.17 ng/ml

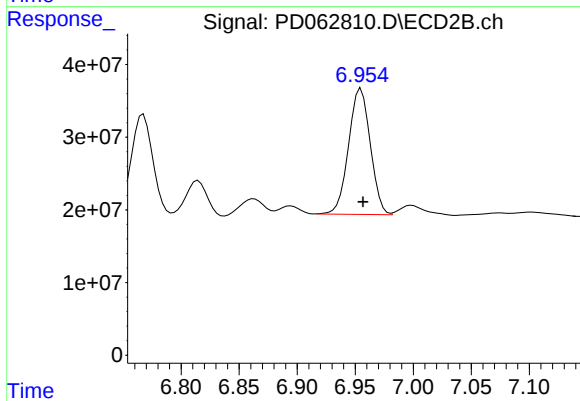

#27 Chlordane-5


R.T.: 6.955 min
Delta R.T.: -0.002 min
Response: 225513470
Conc: 458.51 ng/ml

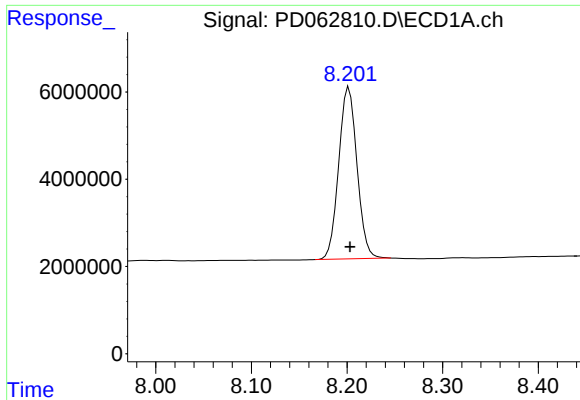

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.001 min
Response: 52484350
Conc: 49.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

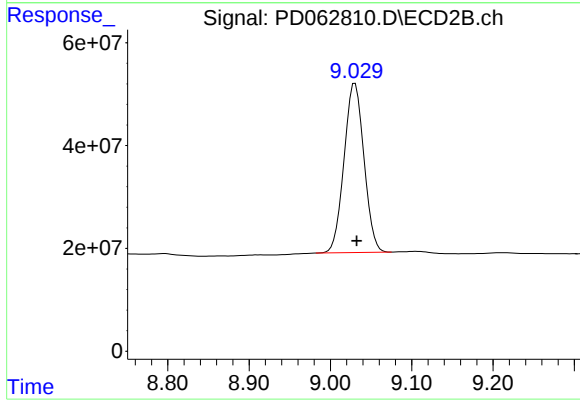

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 558655907
Conc: 48.41 ng/ml