

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 21:05
 Operator : AR\AJ
 Sample : M2310-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BS-SP1

Manual Integrations
 APPROVED

Ankita
 5/10/2021 2:03:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 08:05:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	20646855	255.0E6	23.219	22.028
28)	SA Decachlor...	8.201	9.030	24079692	263.0E6	22.744	22.788
Target Compounds							
16)	A 4,4'-DDD	6.120	6.795	881166	15380747	0.925m	1.190m#
17)	MA 4,4'-DDT	6.361	7.096	1248371	22894699	1.300	1.797 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 21:05
Operator : AR\AJ
Sample : M2310-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BS-SP1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:03:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 08:05:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

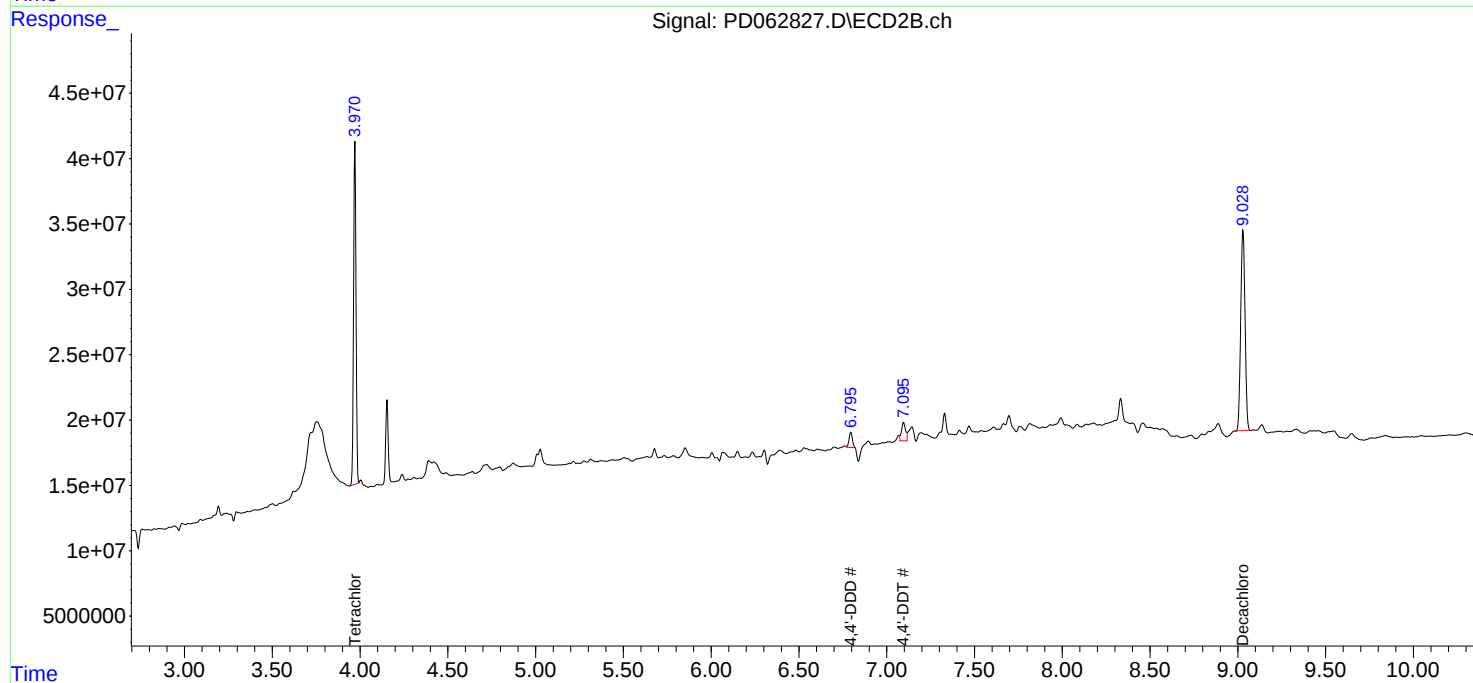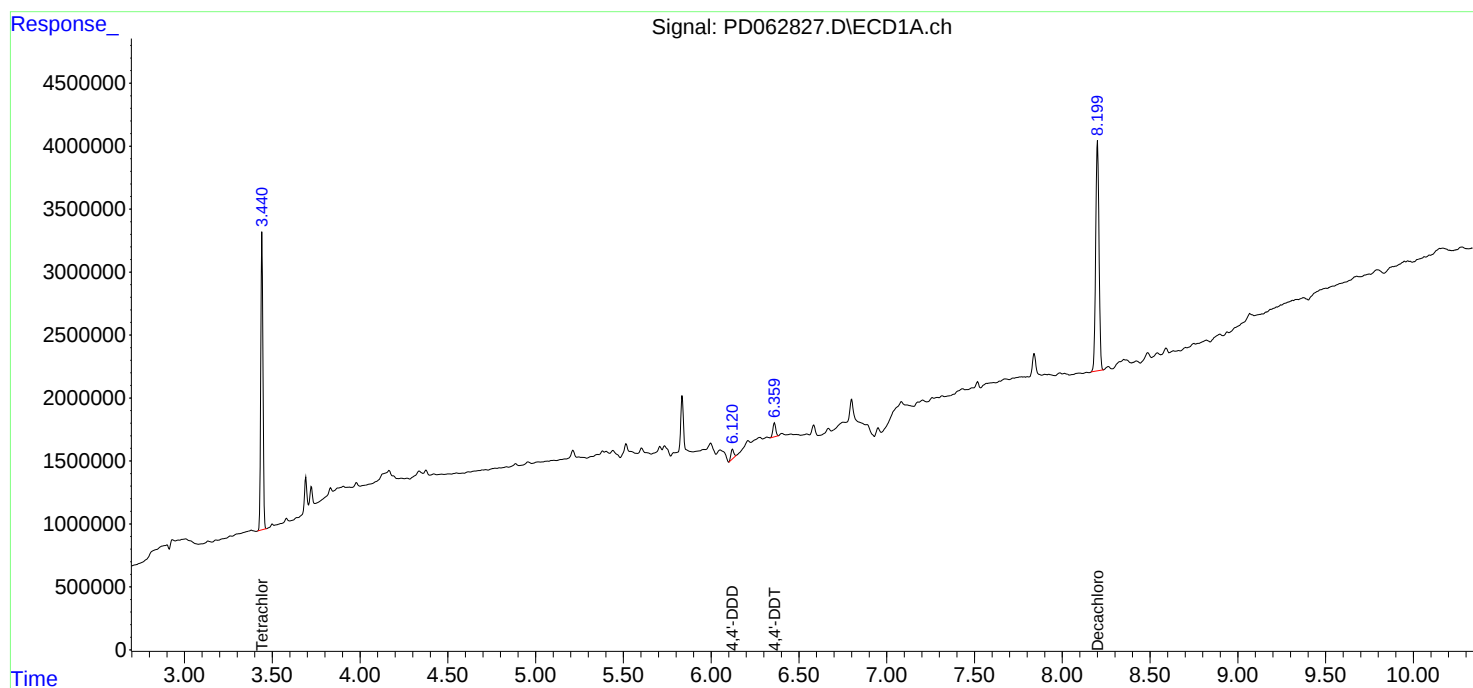

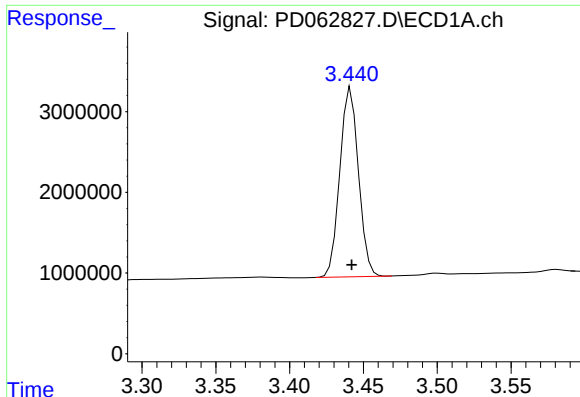


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 20646855
Conc: 23.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
BS-SP1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:03:24 PM

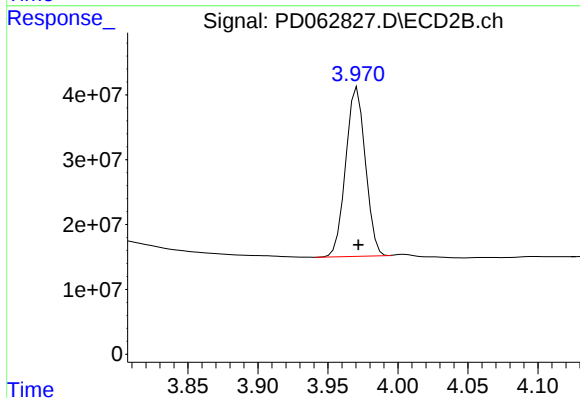


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 255023483
Conc: 22.03 ng/ml

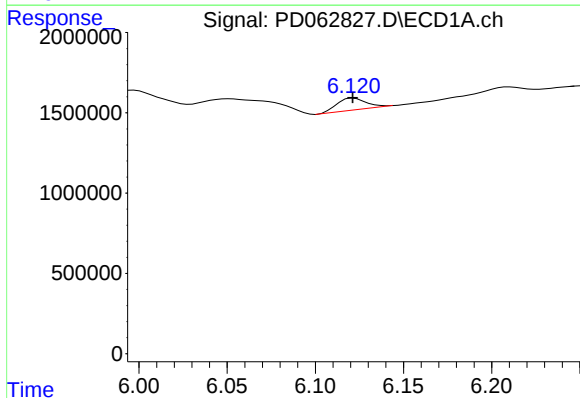


#16 4,4'-DDD

R.T.: 6.120 min
Delta R.T.: -0.001 min
Response: 881166
Conc: 0.93 ng/ml m

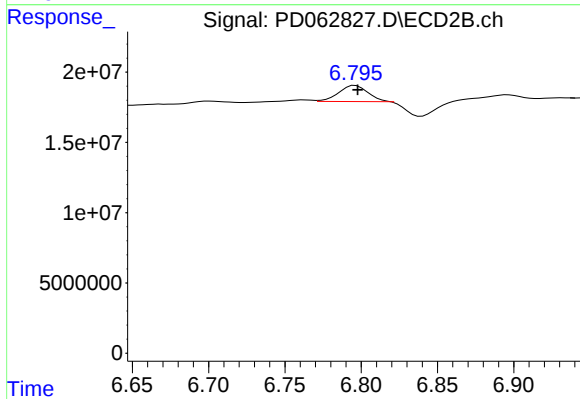

#16 4,4'-DDD

R.T.: 6.795 min
Delta R.T.: -0.003 min
Response: 15380747
Conc: 1.19 ng/ml m

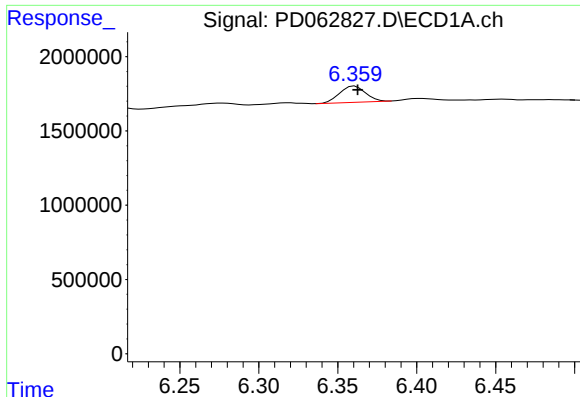


#17 4,4'-DDT

R.T.: 6.361 min
Delta R.T.: -0.002 min
Response: 1248371
Conc: 1.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
BS-SP1


Manual Integrations
APPROVED

Ankita
5/10/2021 2:03:24 PM

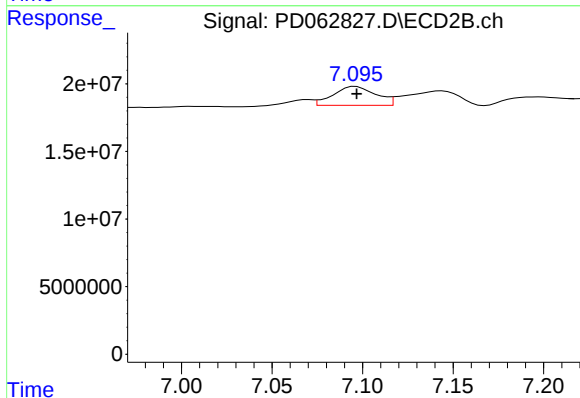


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 22894699
Conc: 1.80 ng/ml

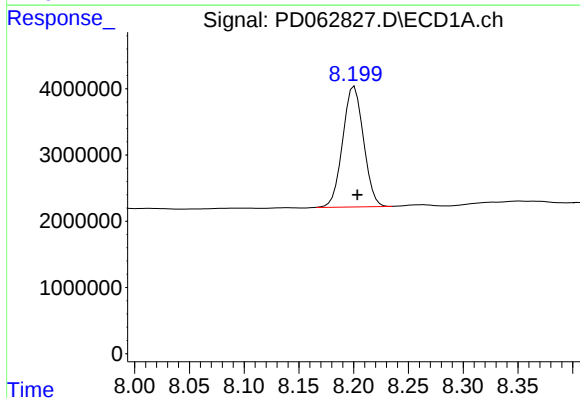

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.003 min
Response: 24079692
Conc: 22.74 ng/ml

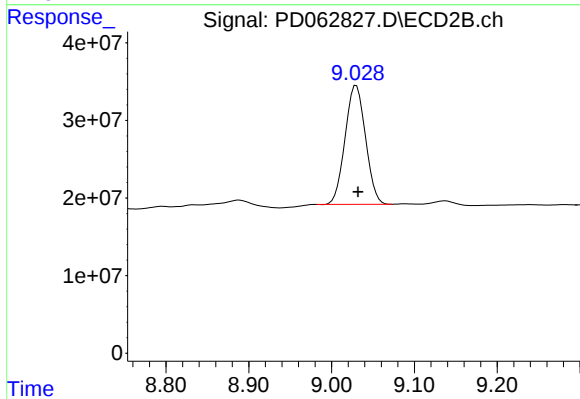

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 262950806
Conc: 22.79 ng/ml