

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050923\
 Data File : PD075362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2023 10:14
 Operator : AR\AJ
 Sample : 02419-24
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW921

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/10/2023
 Supervised By : Ankita Jodhani 05/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 21:08:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.770	46615676	15289805	20.438	14.496 #
2)	SA Decachlor...	9.095	7.915	117.2E6	91425779	47.356	96.810 #
Target Compounds							
3)	MA gamma-BHC...	4.348	3.581	382.5E6	105.3E6	106.403m	71.655m#
14)	MA Endrin	6.595	5.607	4127.5E6	1569.4E6	1427.318	1290.302m
17)	MA 4,4'-DDT	7.019	6.032	4313.0E6	1659.0E6	1699.222m	1646.049m
19)	B Endosulfa...	7.161	6.332	247.5E6	148.5E6	89.959m	127.697m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050923\
Data File : PD075362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2023 10:14
Operator : AR\AJ
Sample : 02419-24
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 21:08:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

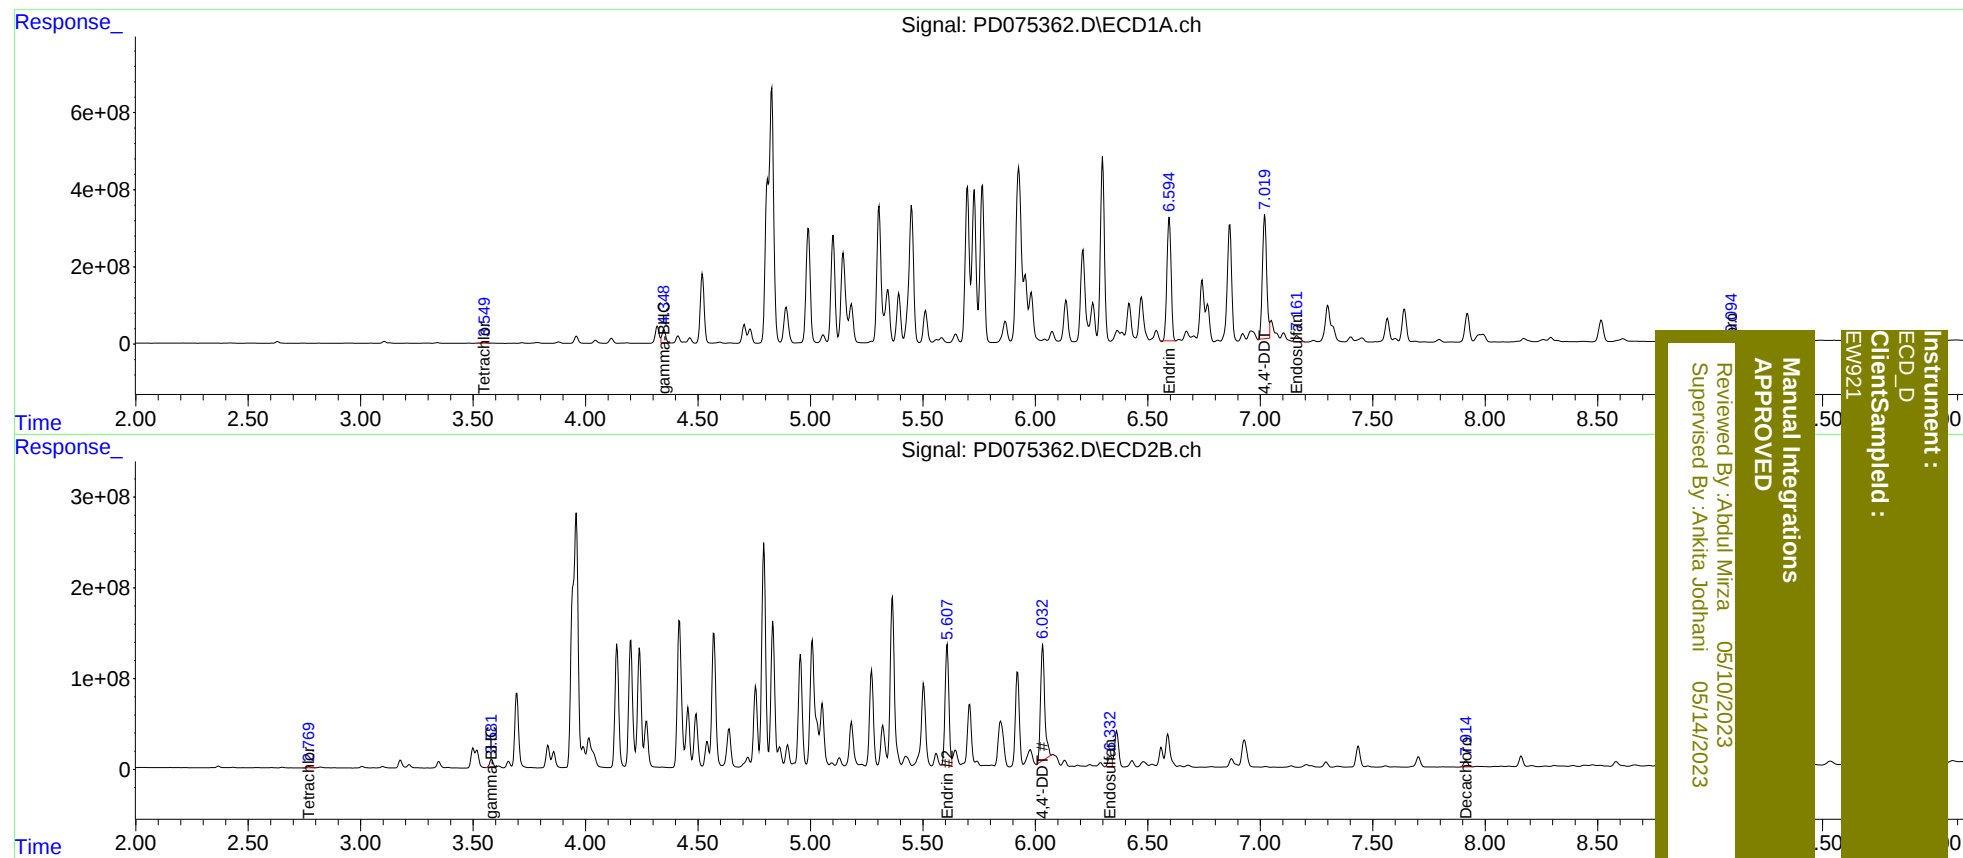

Reviewed By: Abdul Mirza 05/10/2023
Supervised By: Ankita Jodhani 05/14/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW921