

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050924\
 Data File : PD082743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2024 21:03
 Operator : AR\AJ
 Sample : P2374-06MSD 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0Y34MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 03:44:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat May 11 02:23:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.777	33542666	86986242	24.523	23.738
2)	SA Decachlor...	9.123	7.907	44251329	84560756	23.736	23.487
Target Compounds							
2)	A alpha-BHC	4.023	3.277	157.5E6	348.3E6	66.884	61.615
3)	MA gamma-BHC...	4.357	3.605	141.5E6	306.2E6	62.489	59.250
4)	MA Heptachlor	4.949	3.944	139.6E6	297.9E6	63.736	57.787
5)	MB Aldrin	5.293	4.224	138.0E6	294.9E6	63.835	59.581
6)	B beta-BHC	4.553	3.901	58332307	127.4E6	61.370	57.279
7)	B delta-BHC	4.802	4.131	139.9E6	315.5E6	67.201	59.054
8)	B Heptachlo...	5.720	4.725	126.3E6	272.4E6	63.853	59.861
9)	A Endosulfan I	6.108	5.094	121.6E6	252.4E6	63.061	59.931
10)	B trans-Chl...	5.978	4.974	123.8E6	270.9E6	63.157	60.349
11)	B cis-Chlor...	6.058	5.038	125.2E6	270.2E6	62.040	59.398
12)	B 4,4'-DDE	6.229	5.227	248.3E6	525.8E6	123.938	121.092
13)	MA Dieldrin	6.384	5.358	258.2E6	557.8E6	123.978	119.480
14)	MA Endrin	6.616	5.634	221.1E6	486.0E6	127.508	118.721
15)	B Endosulfa...	6.835	5.927	218.5E6	460.8E6	122.878	120.303
16)	A 4,4'-DDD	6.748	5.780	188.4E6	417.9E6	125.959	119.454
17)	MA 4,4'-DDT	7.064	6.031	204.0E6	442.2E6	130.522	122.988
18)	B Endrin al...	6.965	6.106	156.3E6	335.4E6	123.125	118.335
19)	B Endosulfa...	7.201	6.329	204.1E6	438.9E6	127.027	122.018
20)	A Methoxychlor	7.541	6.606	506.8E6	985.0E6	608.764	565.342
21)	B Endrin ke...	7.688	6.834	217.8E6	485.1E6	125.265	121.533

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050924\
Data File : PD082743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2024 21:03
Operator : AR\AJ
Sample : P2374-06MSD 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 03:44:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat May 11 02:23:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

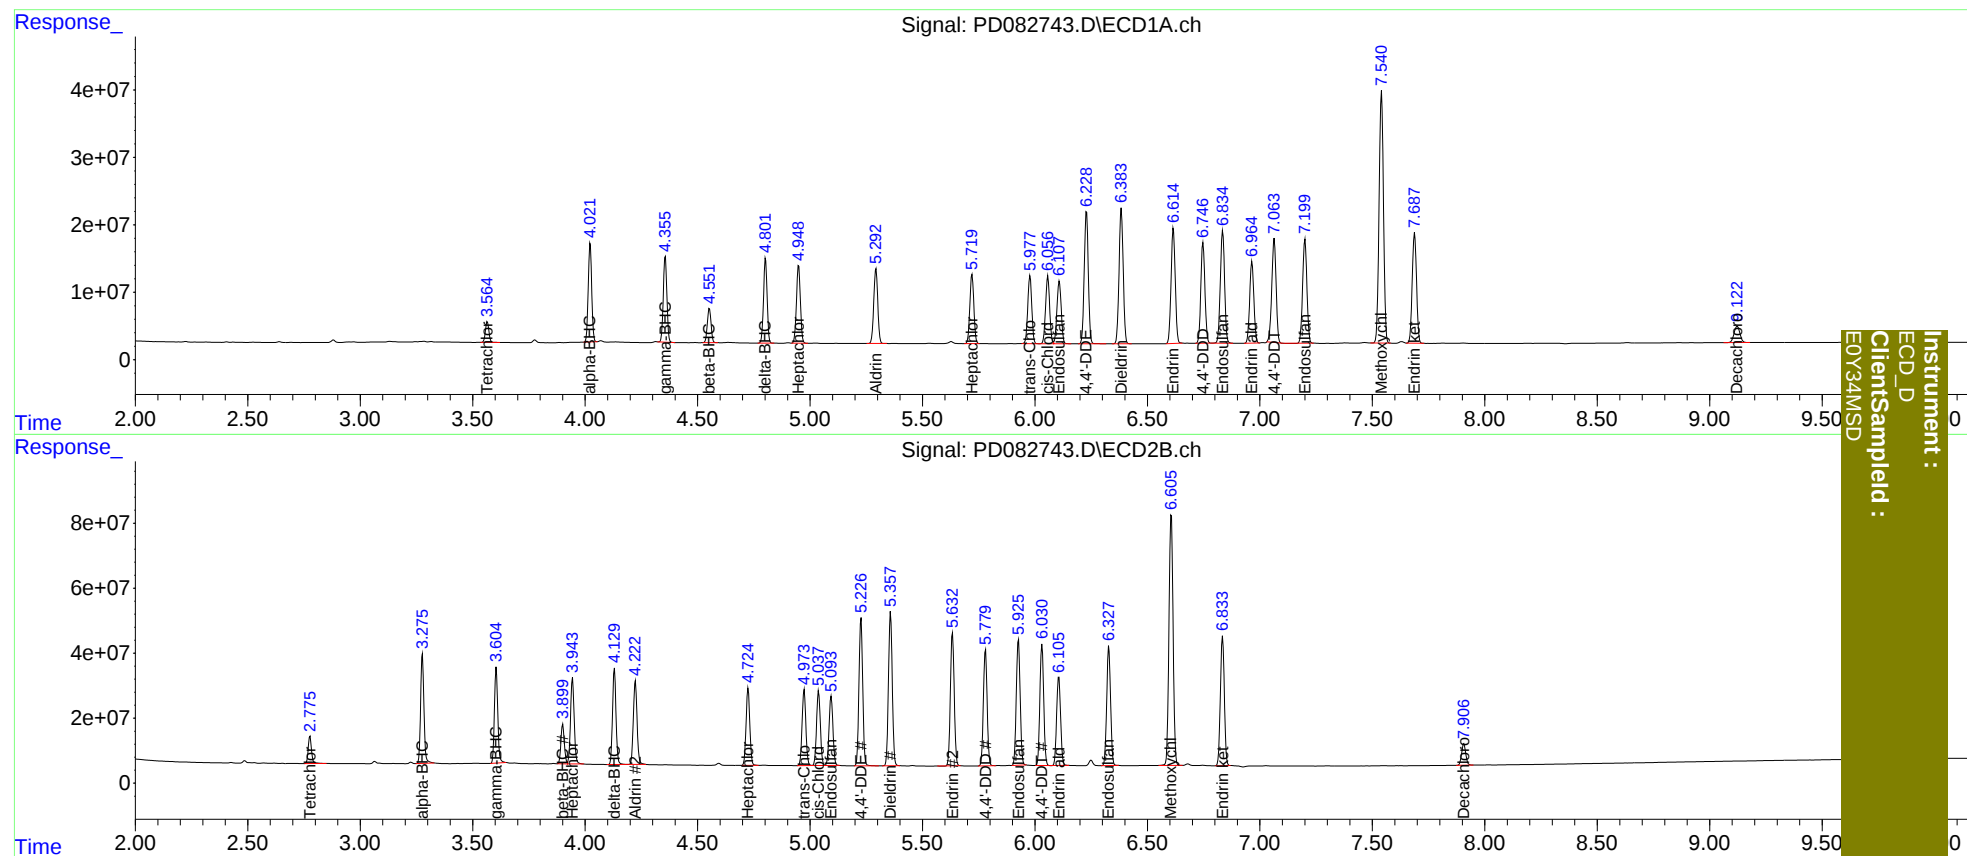

Instrument :
ECD_D
ClientSampled :
E0Y34MSD