

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
 Data File : PD062835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 09:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 13:39:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	21009076	239.3E6	23.627	20.673
28)	SA Decachlor...	8.200	9.029	23714494	260.2E6	22.399	22.550
Target Compounds							
5)	MB Aldrin	0.000	5.472	0	1625484	N.D.	0.097 #
7)	B delta-BHC	0.000	5.006f	0	24808175	N.D.	1.374 #
8)	B Heptachlo...	0.000	5.852	0	7514453	N.D.	0.470 #
9)	A Endosulfan I	0.000	6.199	0	4246509	N.D.	0.288 #
14)	MA Endrin	0.000	6.666	0	5402914	N.D.	0.384 #
15)	B Endosulfa...	0.000	6.903f	0	12992349	N.D.	0.973 #
17)	MA 4,4'-DDT	0.000	7.087	0	4439024	N.D.	0.348 #
22)	Mirex	0.000	8.157	0	20295859	N.D.	2.216 #
23)	Chlordane-1	4.337f	0.000	446657	0	12.666	N.D. #
27)	Chlordane-5	0.000	6.948	0	903040	N.D.	1.836 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
Data File : PD062835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 09:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 13:39:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

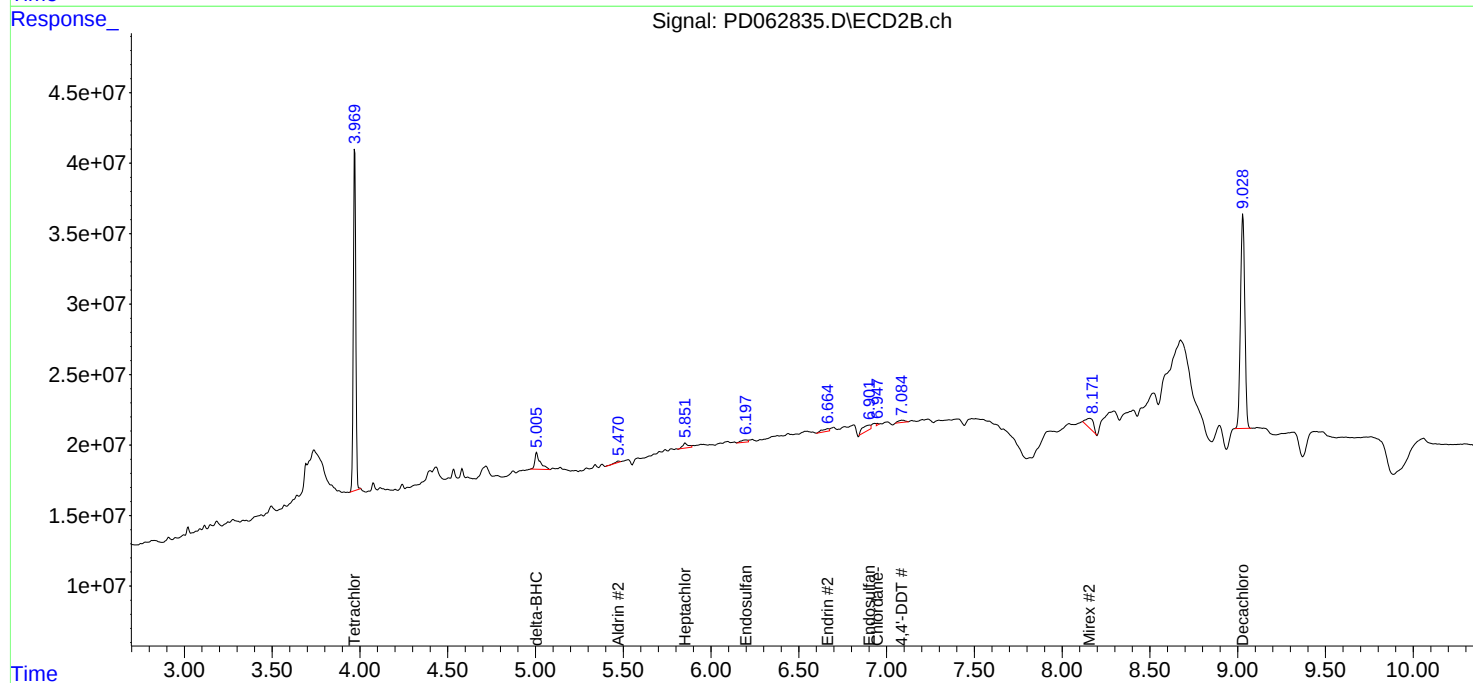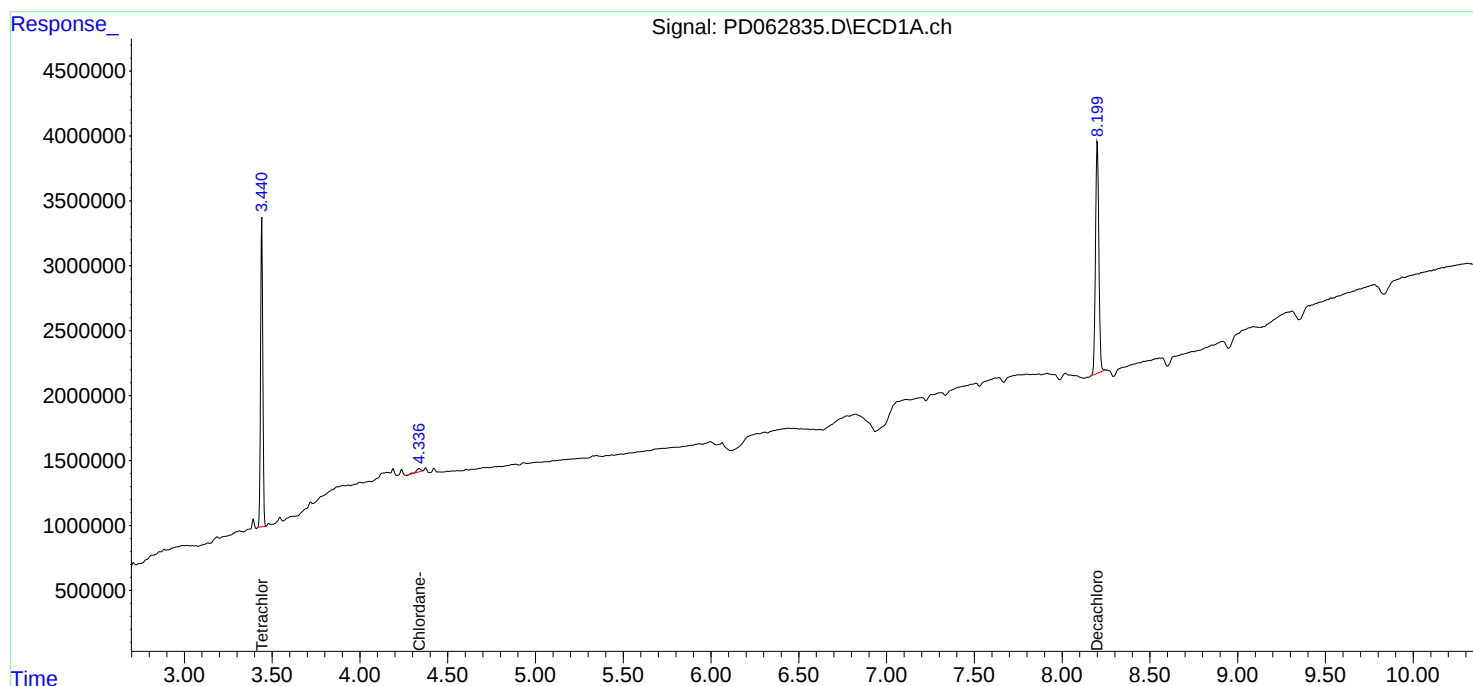


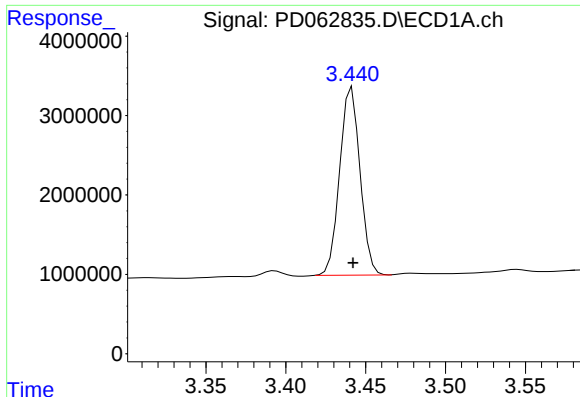

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 21009076
Conc: 23.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

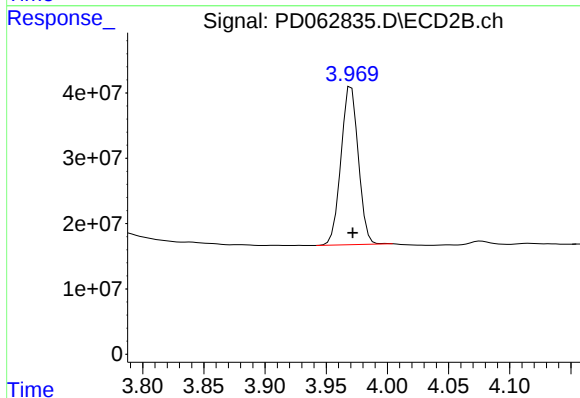


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.001 min
Response: 239326927
Conc: 20.67 ng/ml

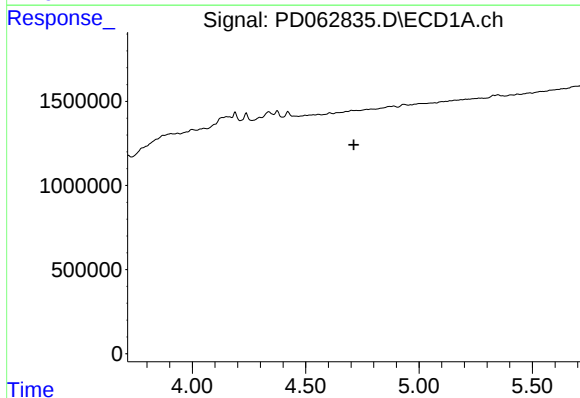


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

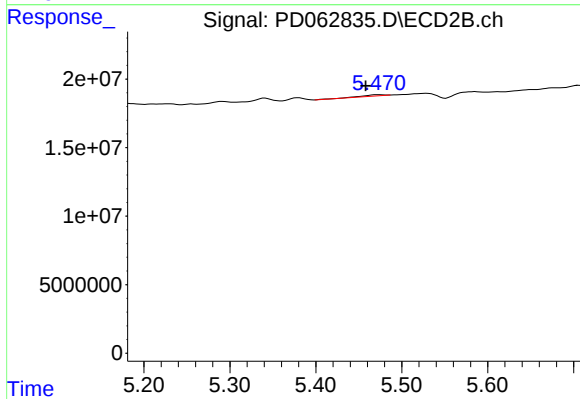

#5 Aldrin


R.T.: 5.472 min
Delta R.T.: 0.014 min
Response: 1625484
Conc: 0.10 ng/ml

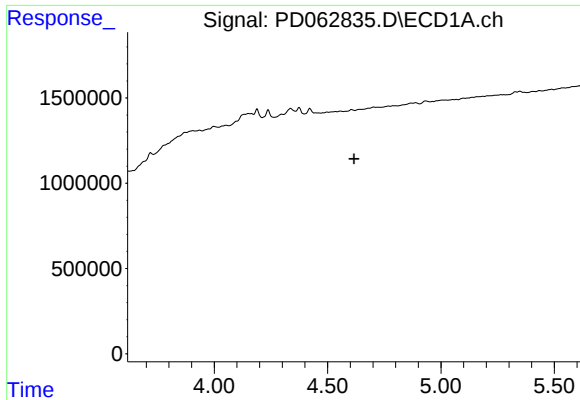

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

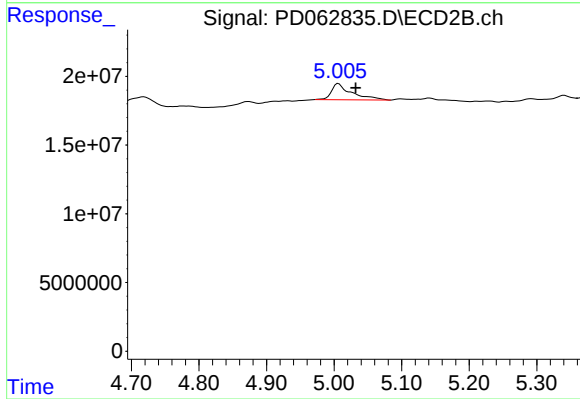


#7 delta-BHC

R.T.: 5.006 min
Delta R.T.: -0.025 min
Response: 24808175
Conc: 1.37 ng/ml

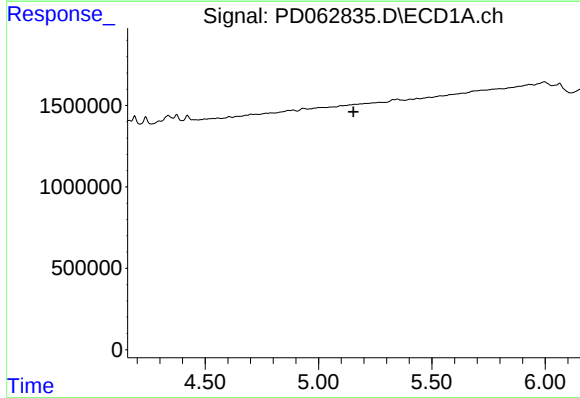


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

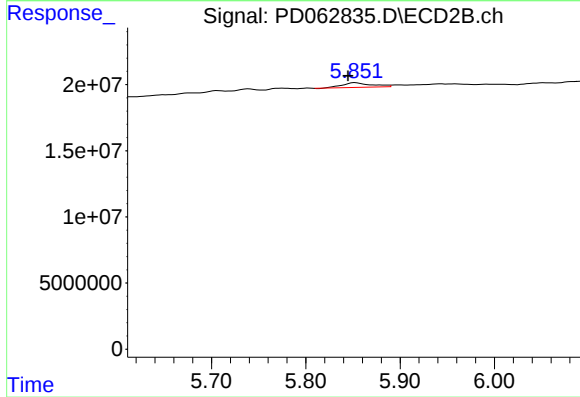

#8 Heptachlor epoxide


R.T.: 5.852 min
Delta R.T.: 0.007 min
Response: 7514453
Conc: 0.47 ng/ml

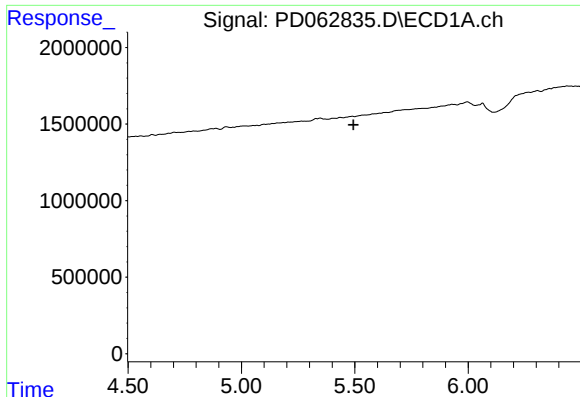

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

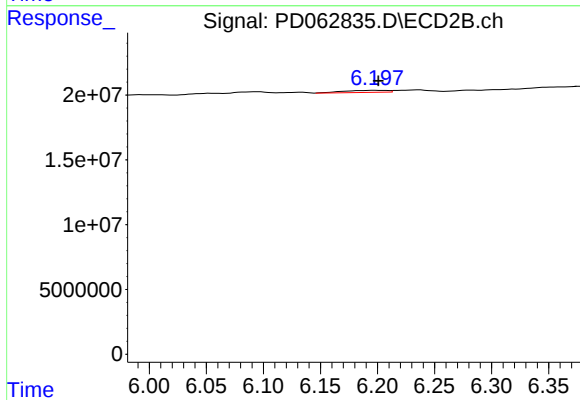


#9 Endosulfan I

R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 4246509
Conc: 0.29 ng/ml

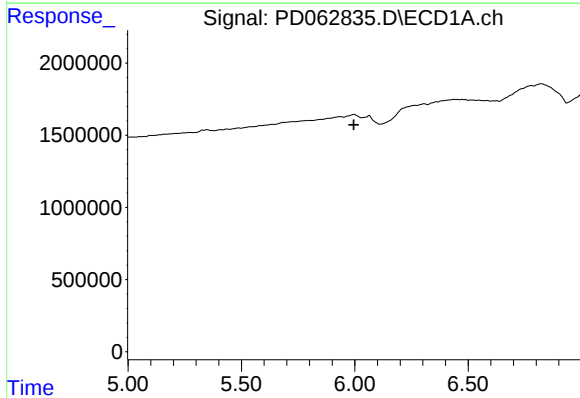


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

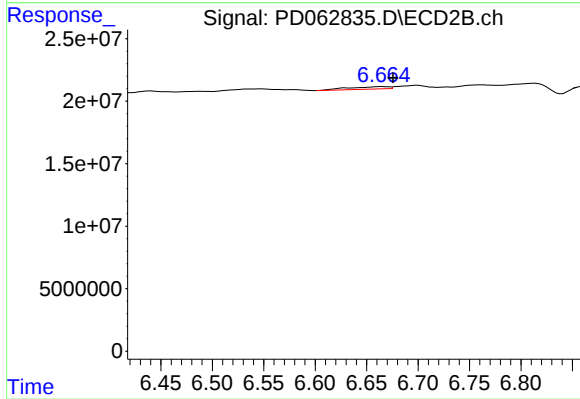

#14 Endrin


R.T.: 6.666 min
Delta R.T.: -0.010 min
Response: 5402914
Conc: 0.38 ng/ml

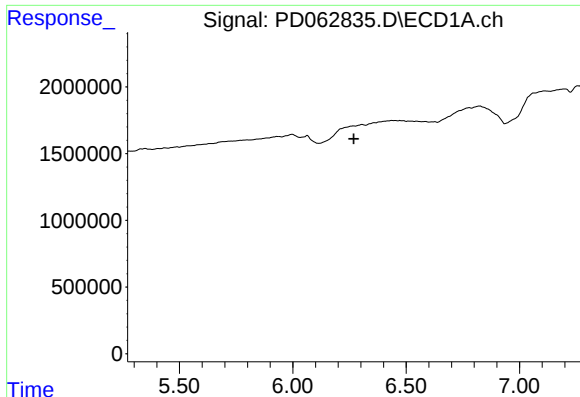

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

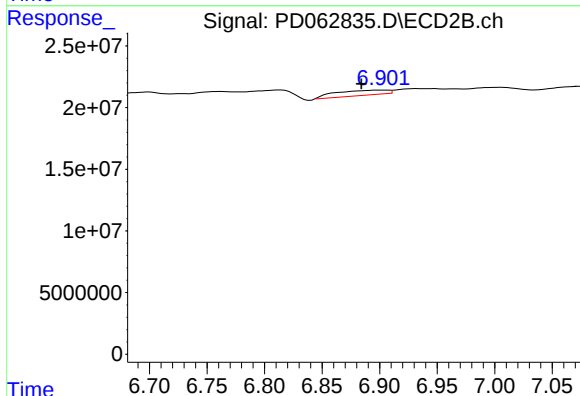


#15 Endosulfan II

R.T.: 6.903 min
Delta R.T.: 0.019 min
Response: 12992349
Conc: 0.97 ng/ml

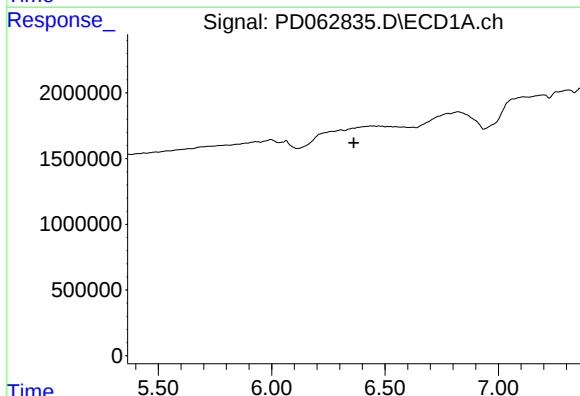


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

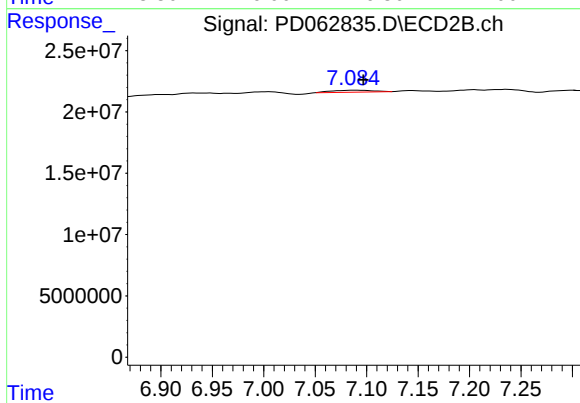

#17 4,4'-DDT


R.T.: 7.087 min
Delta R.T.: -0.009 min
Response: 4439024
Conc: 0.35 ng/ml

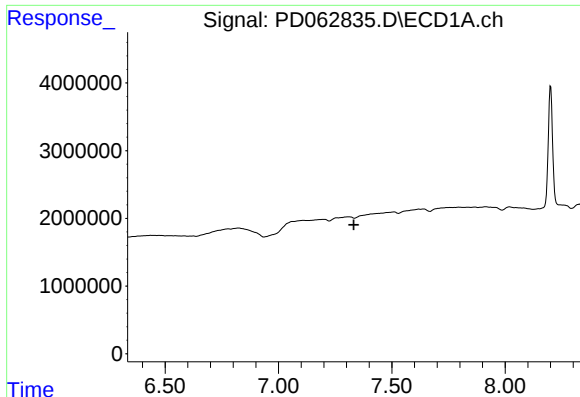

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

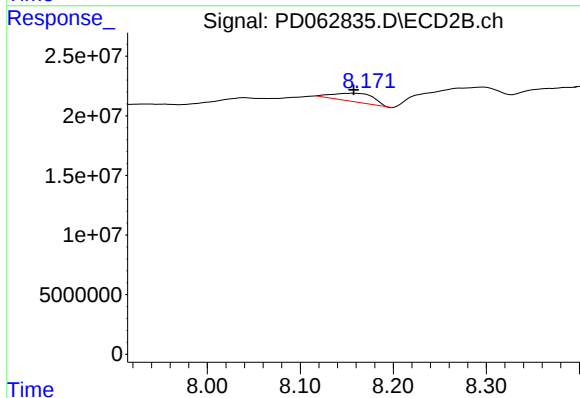


#22 Mirex

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 20295859
Conc: 2.22 ng/ml

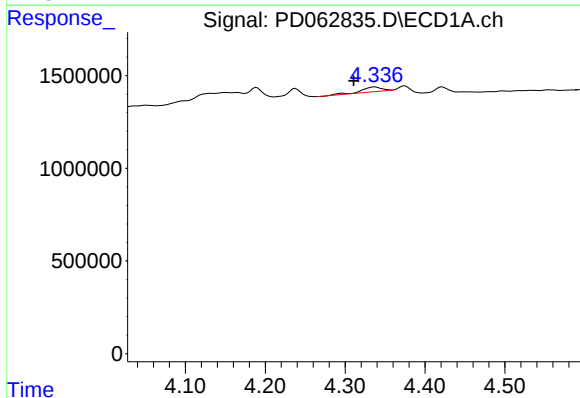


#23 Chlordane-1

R.T.: 4.337 min
Delta R.T.: 0.026 min
Response: 446657
Conc: 12.67 ng/ml

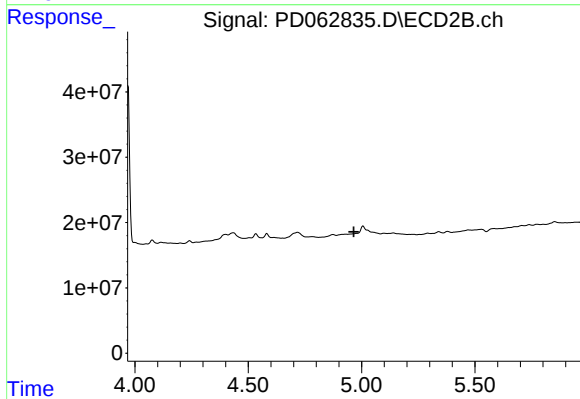

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.965 min
Response: 0
Conc: N.D.

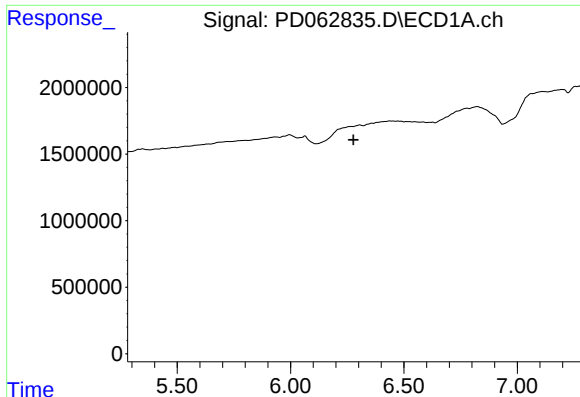

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

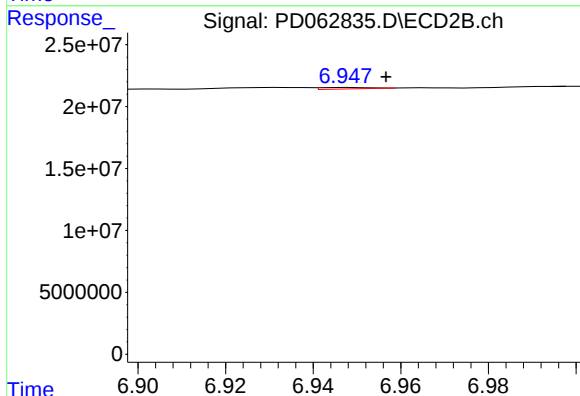


#27 Chlordane-5

R.T.: 6.948 min
Delta R.T.: -0.009 min
Response: 903040
Conc: 1.84 ng/ml

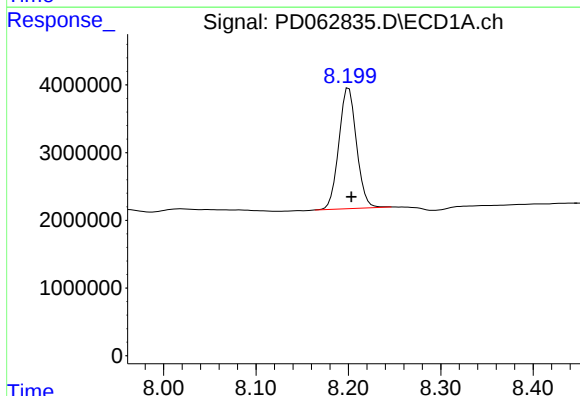

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.003 min
Response: 23714494
Conc: 22.40 ng/ml

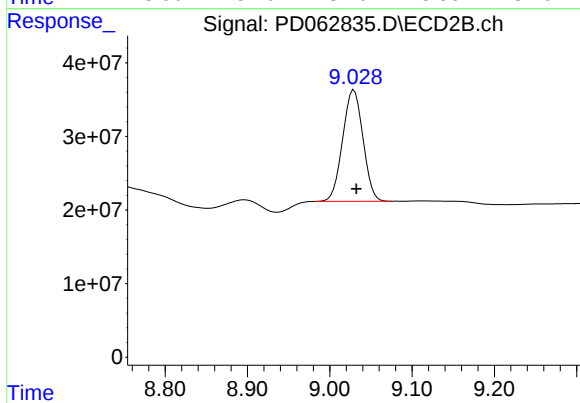

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: -0.003 min
Response: 260200124
Conc: 22.55 ng/ml