

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
 Data File : PD062840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 11:02
 Operator : AR\AJ
 Sample : PB136252BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 13:45:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	3.971	24145497	296.3E6	27.154	25.595
28)	SA Decachlor...	8.204	9.030	28075448	308.7E6	26.519	26.752
Target Compounds							
2)	A alpha-BHC	0.000	4.368	0	6265016	N.D.	0.325 #
7)	B delta-BHC	0.000	5.026	0	7307937	N.D.	0.405 #
8)	B Heptachlo...	0.000	5.854	0	8814663	N.D.	0.552 #
9)	A Endosulfan I	0.000	6.182f	0	3097176	N.D.	0.210 #
11)	B alpha-Chl...	0.000	6.132f	0	3664644	N.D.	0.240 #
14)	MA Endrin	0.000	6.684	0	5266097	N.D.	0.375 #
15)	B Endosulfa...	0.000	6.897	0	6525248	N.D.	0.488 #
26)	Chlordane-4	0.000	6.132f	0	3664644	N.D.	1.421 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
Data File : PD062840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 11:02
Operator : AR\AJ
Sample : PB136252BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 13:45:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

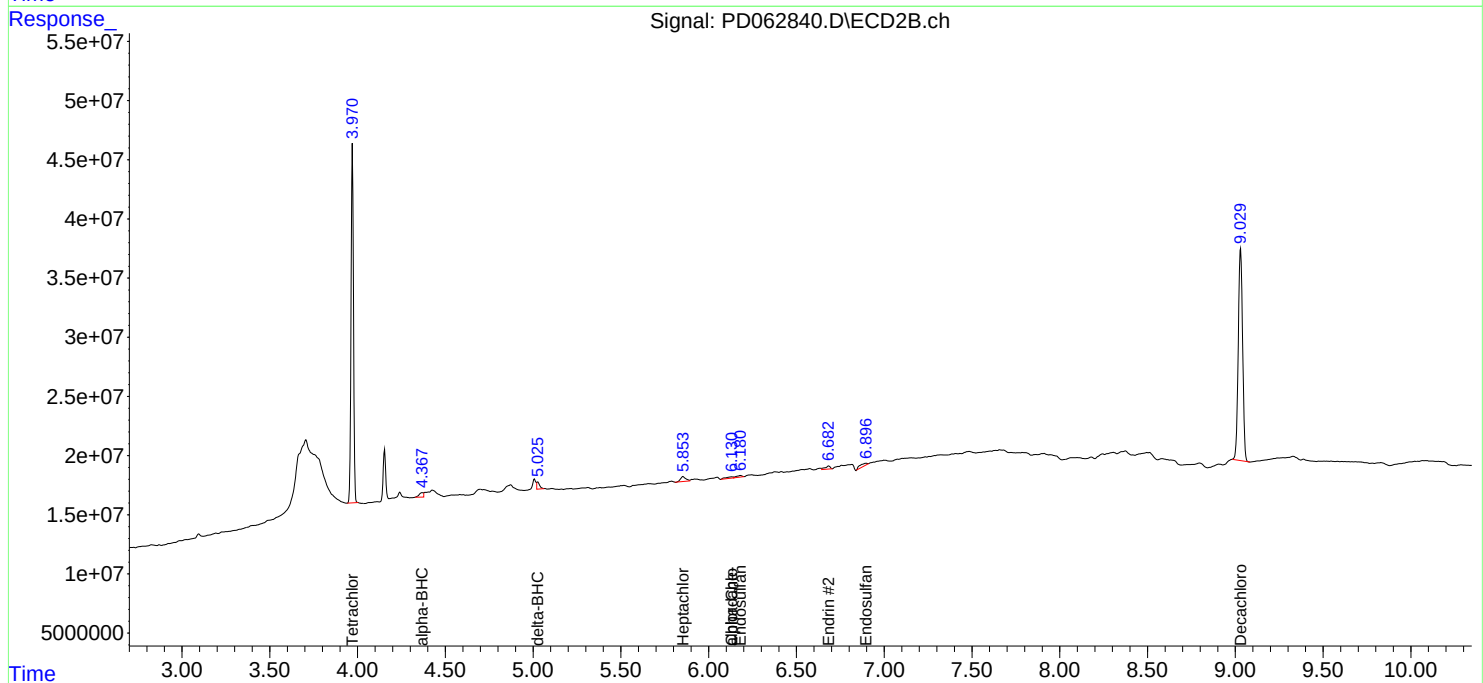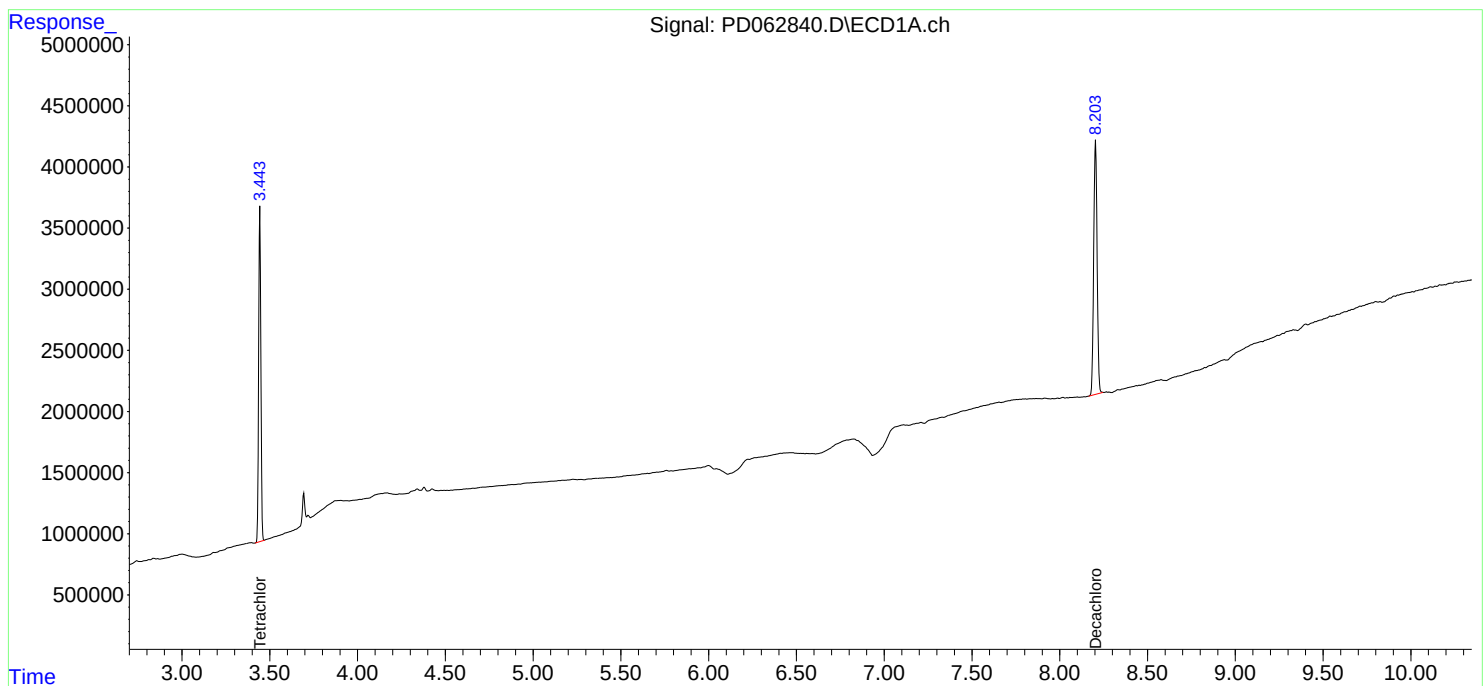


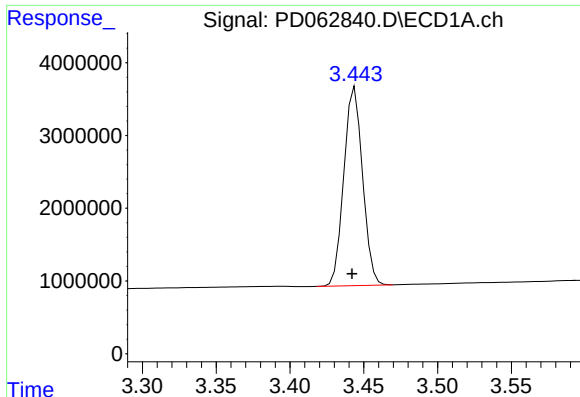

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.002 min
Response: 24145497
Conc: 27.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

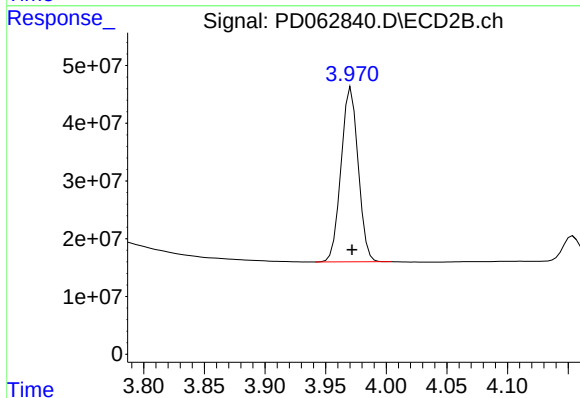


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 296315354
Conc: 25.60 ng/ml

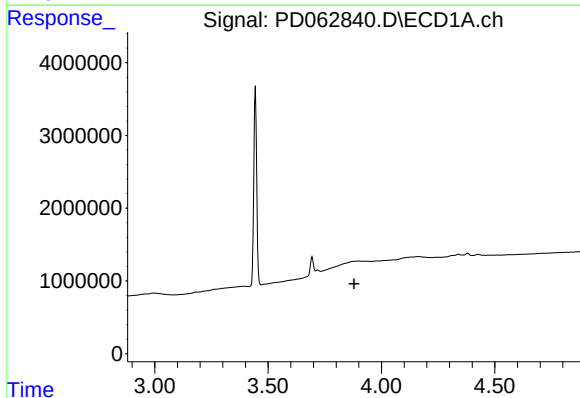


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.879 min
Response: 0
Conc: N.D.

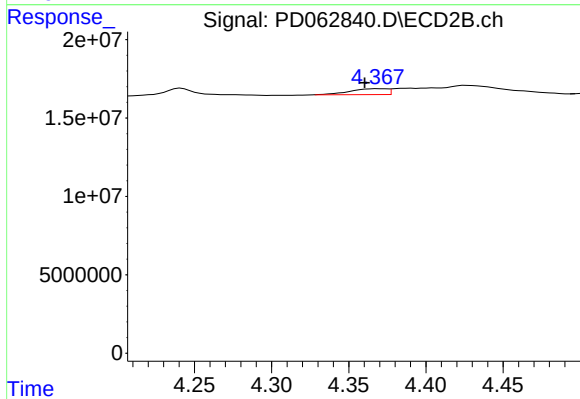

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: 0.008 min
Response: 6265016
Conc: 0.33 ng/ml

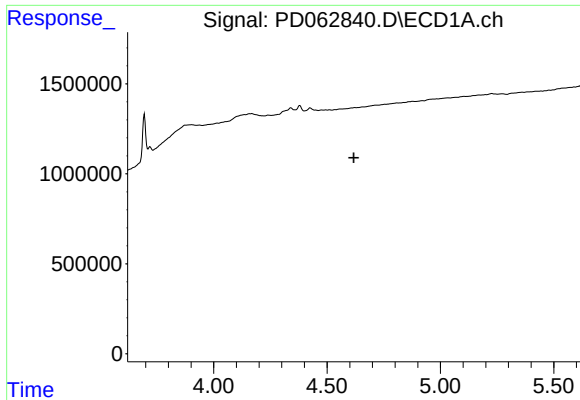

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

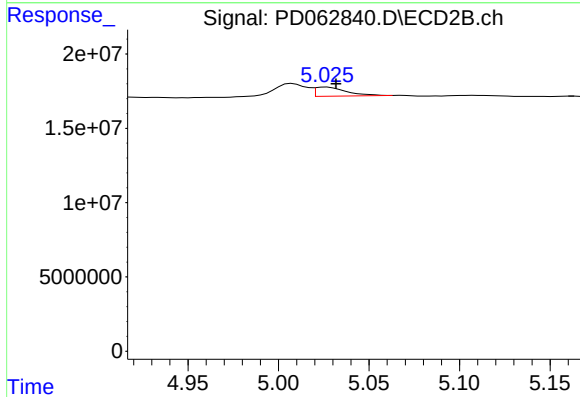


#7 delta-BHC

R.T.: 5.026 min
Delta R.T.: -0.005 min
Response: 7307937
Conc: 0.40 ng/ml

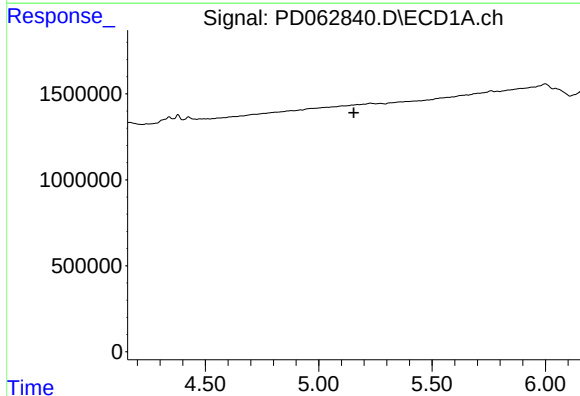


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.155 min
Response: 0
Conc: N.D.

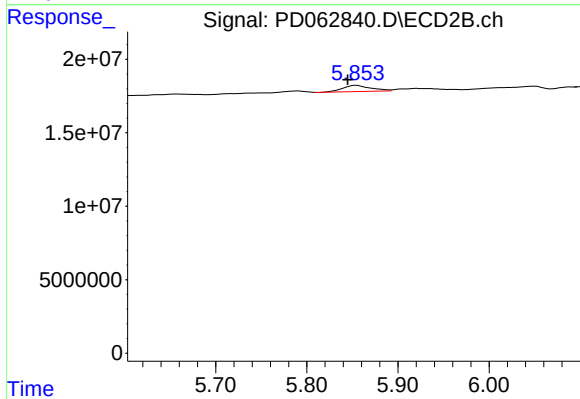

#8 Heptachlor epoxide


R.T.: 5.854 min
Delta R.T.: 0.009 min
Response: 8814663
Conc: 0.55 ng/ml

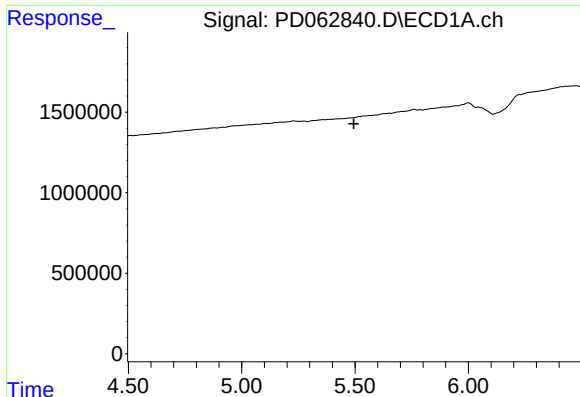

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

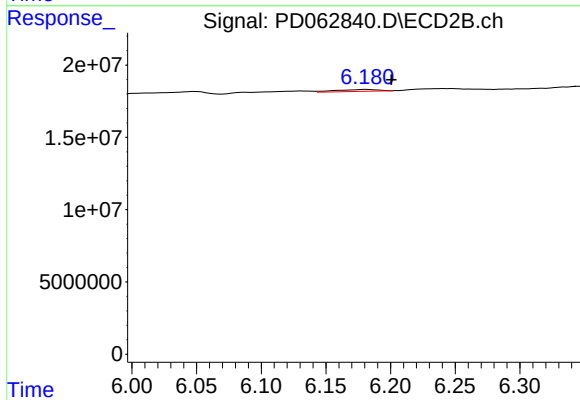


#9 Endosulfan I

R.T.: 6.182 min
Delta R.T.: -0.019 min
Response: 3097176
Conc: 0.21 ng/ml

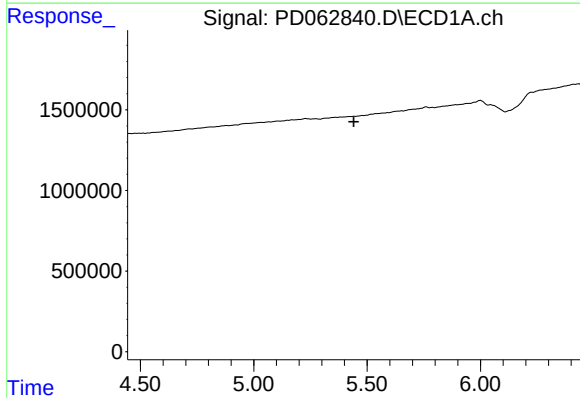


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

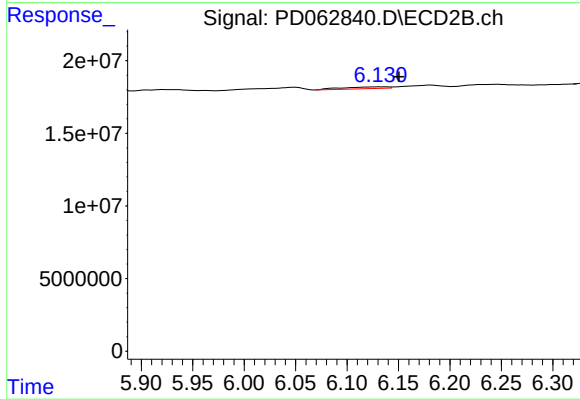

#11 alpha-Chlordane


R.T.: 6.132 min
Delta R.T.: -0.019 min
Response: 3664644
Conc: 0.24 ng/ml

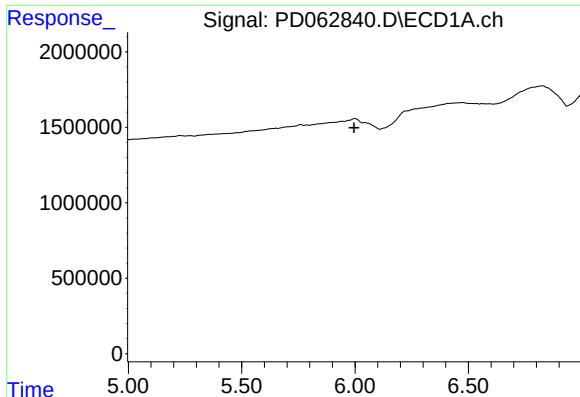

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

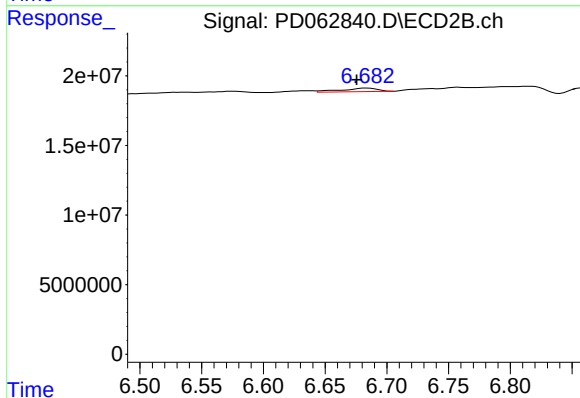


#14 Endrin

R.T.: 6.684 min
Delta R.T.: 0.008 min
Response: 5266097
Conc: 0.37 ng/ml

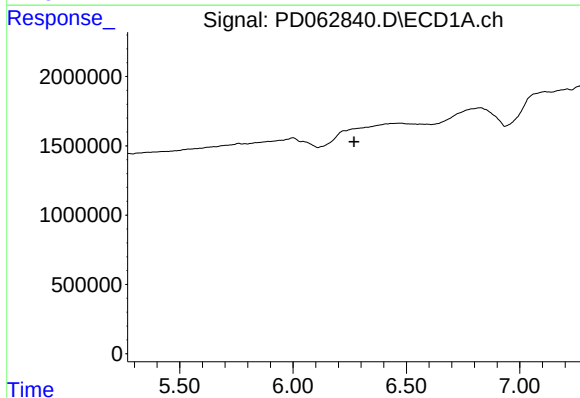


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.269 min
Response: 0
Conc: N.D.

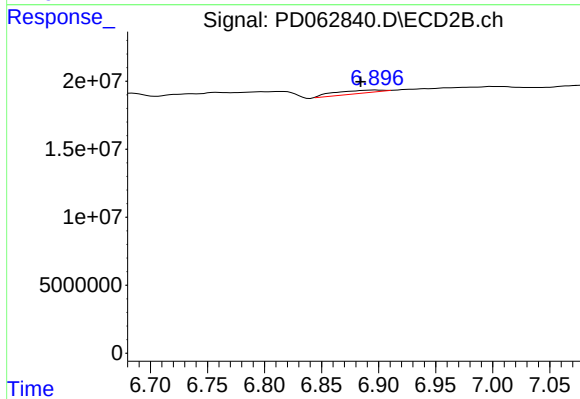

#15 Endosulfan II


R.T.: 6.897 min
Delta R.T.: 0.013 min
Response: 6525248
Conc: 0.49 ng/ml

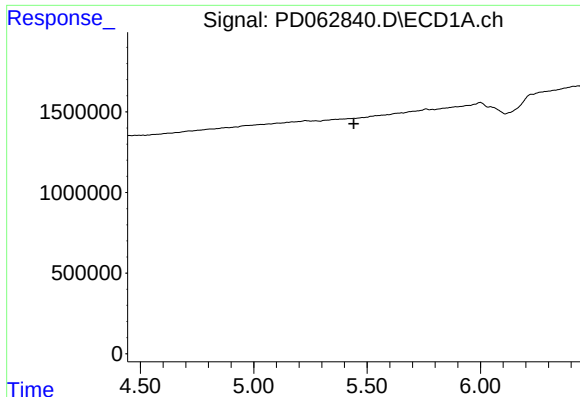

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

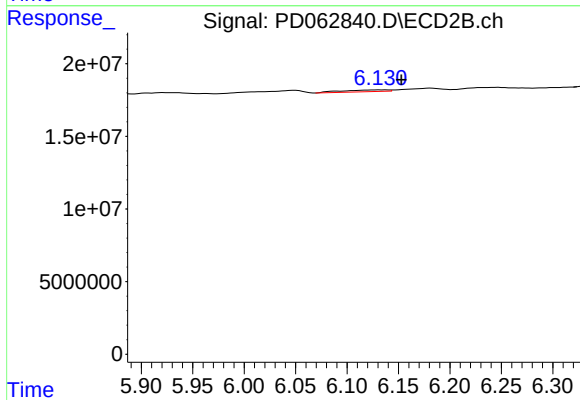


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: -0.021 min
Response: 3664644
Conc: 1.42 ng/ml

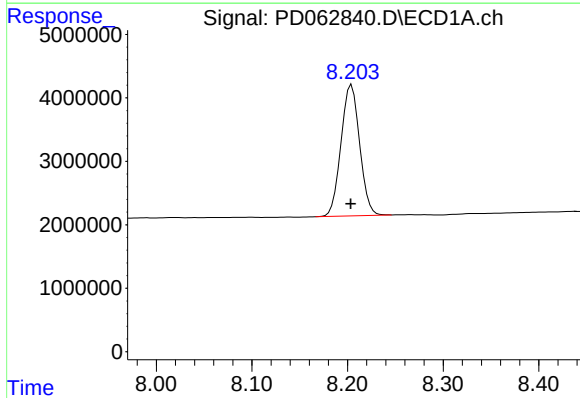

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 28075448
Conc: 26.52 ng/ml

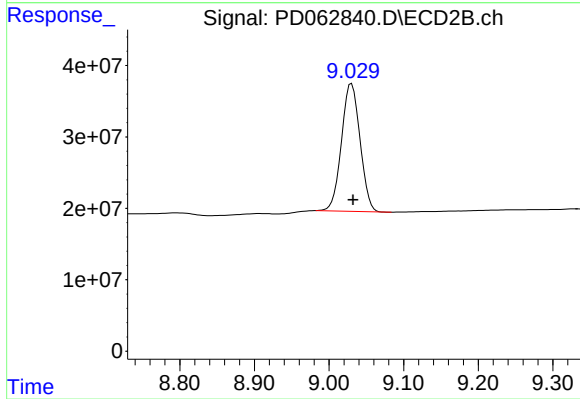

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 308685599
Conc: 26.75 ng/ml