

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
 Data File : PD062843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 11:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 13:40:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	3.971	20468145	247.7E6	23.018	21.395
28)	SA Decachlor...	8.205	9.031	24696601	263.7E6	23.327	22.849
Target Compounds							
6)	B beta-BHC	4.380f	0.000	166116	0	0.277	N.D. #
7)	B delta-BHC	0.000	5.008f	0	22127468	N.D.	1.226 #
8)	B Heptachlo...	0.000	5.854	0	9725387	N.D.	0.609 #
9)	A Endosulfan I	0.000	6.223f	0	1763761	N.D.	0.119 #
14)	MA Endrin	0.000	6.688	0	4888220	N.D.	0.348 #
15)	B Endosulfa...	0.000	6.881	0	12731133	N.D.	0.953 #
18)	B Endrin al...	6.463f	0.000	1755089	0	1.881	N.D. #
22)	Mirex	0.000	8.175f	0	12366862	N.D.	1.350 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051021\
Data File : PD062843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 11:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 13:40:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

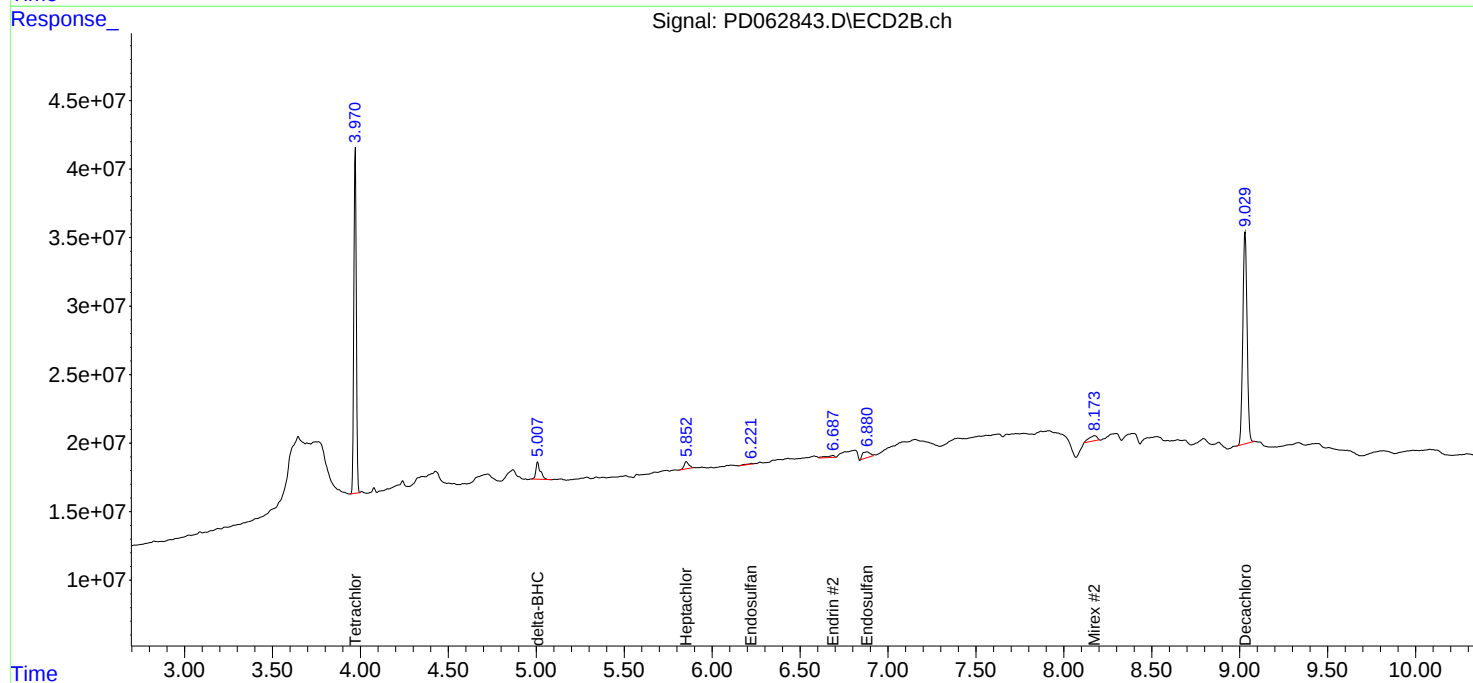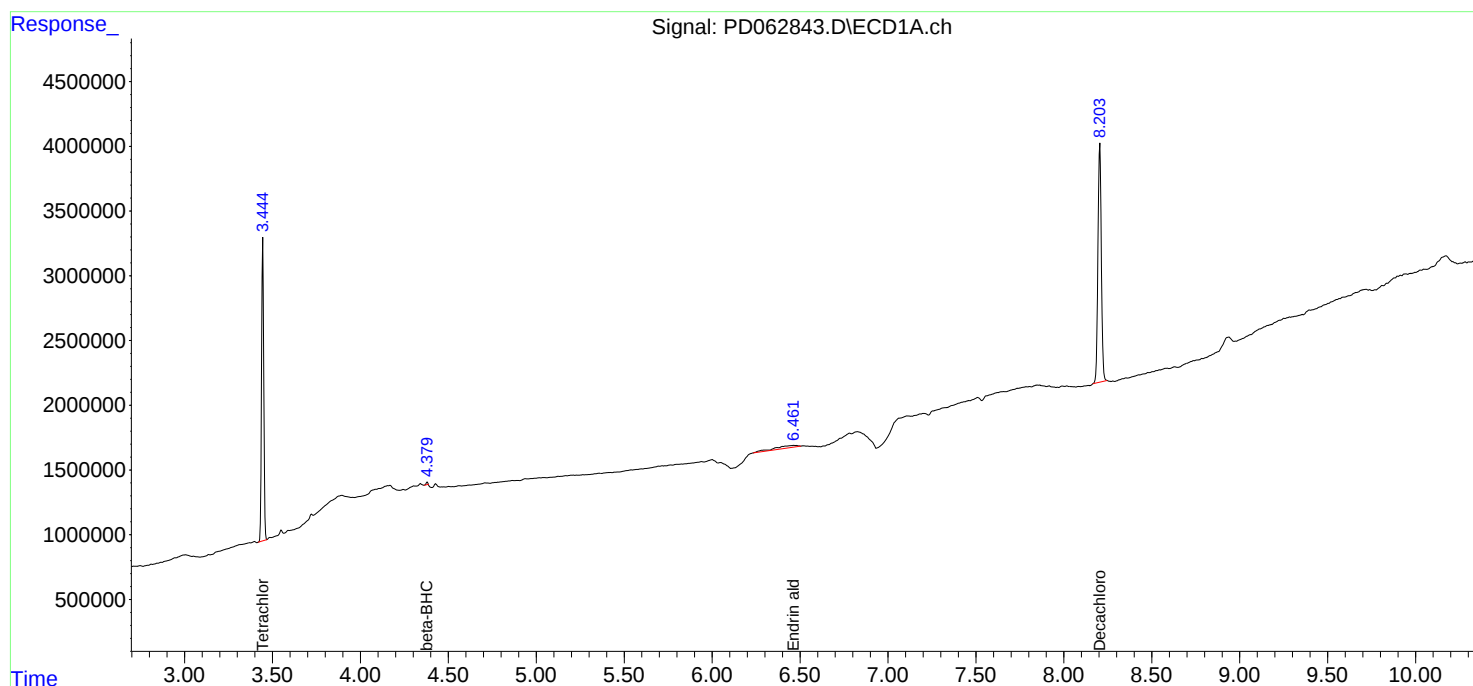


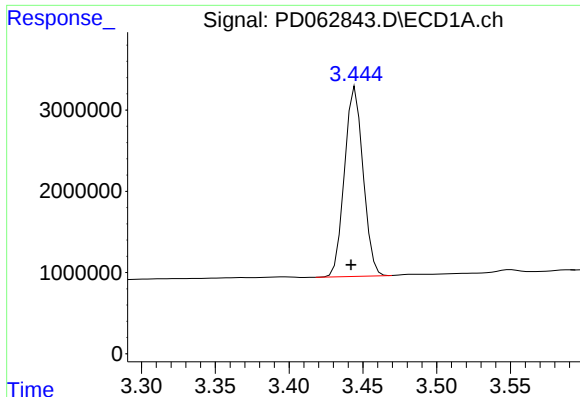

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.003 min
Response: 20468145
Conc: 23.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

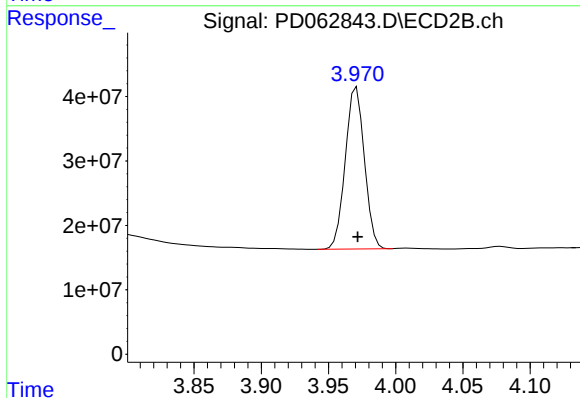


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 247686237
Conc: 21.39 ng/ml

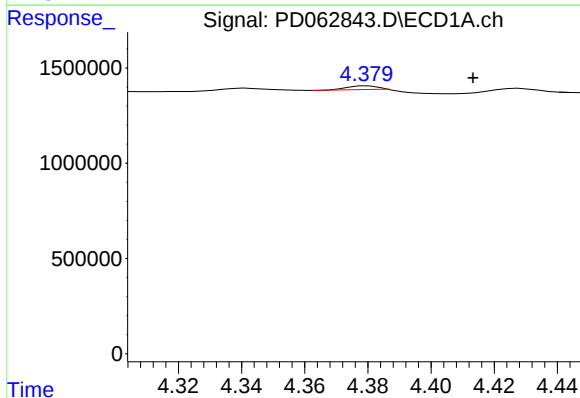


#6 beta-BHC

R.T.: 4.380 min
Delta R.T.: -0.033 min
Response: 166116
Conc: 0.28 ng/ml

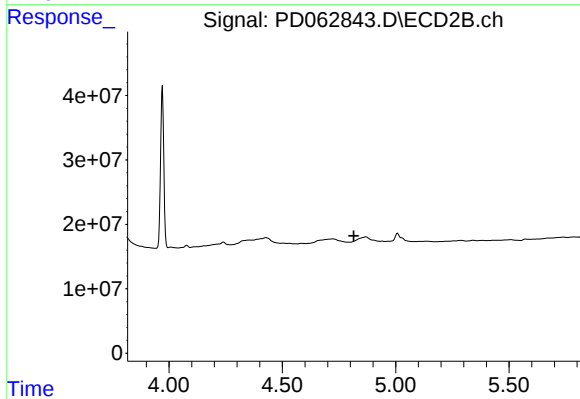

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.816 min
Response: 0
Conc: N.D.

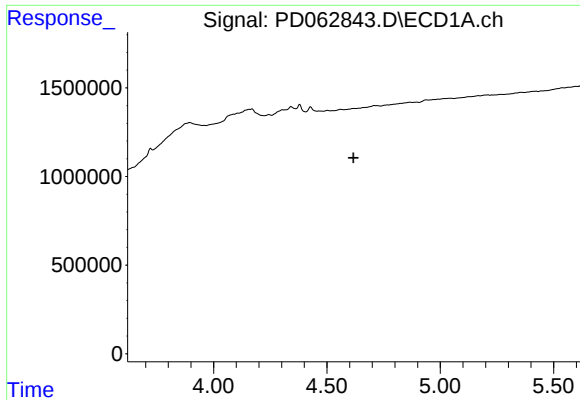

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

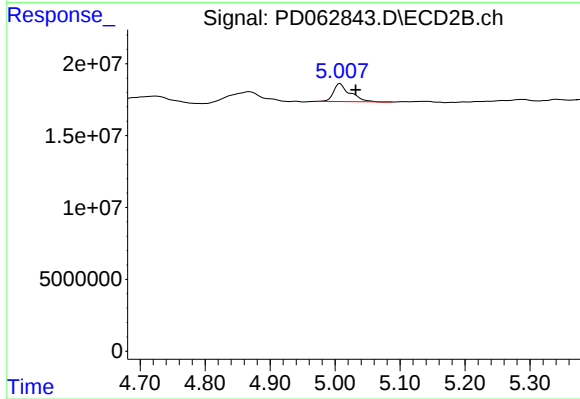


#7 delta-BHC

R.T.: 5.008 min
Delta R.T.: -0.024 min
Response: 22127468
Conc: 1.23 ng/ml

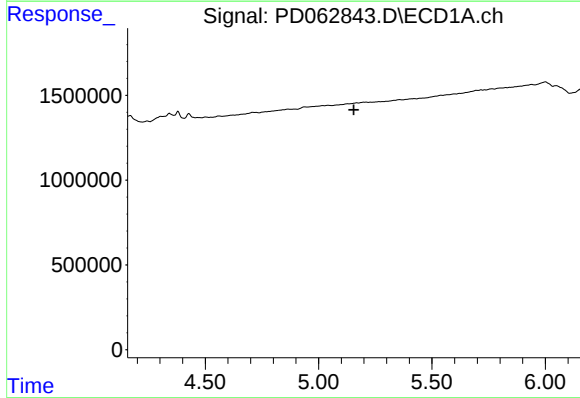


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

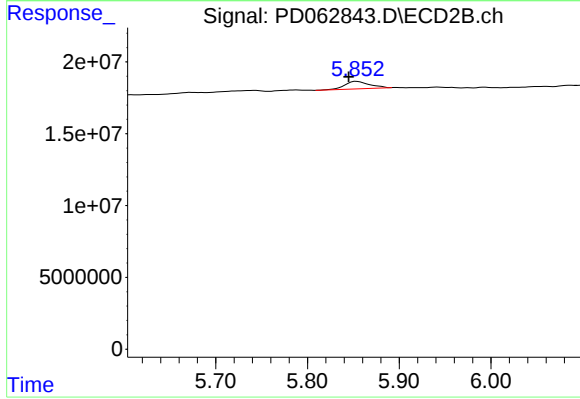

#8 Heptachlor epoxide


R.T.: 5.854 min
Delta R.T.: 0.009 min
Response: 9725387
Conc: 0.61 ng/ml

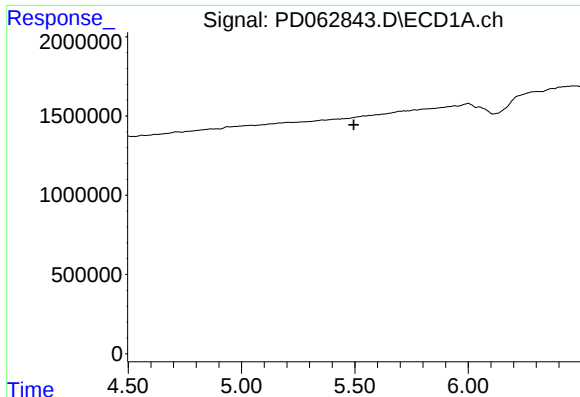

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

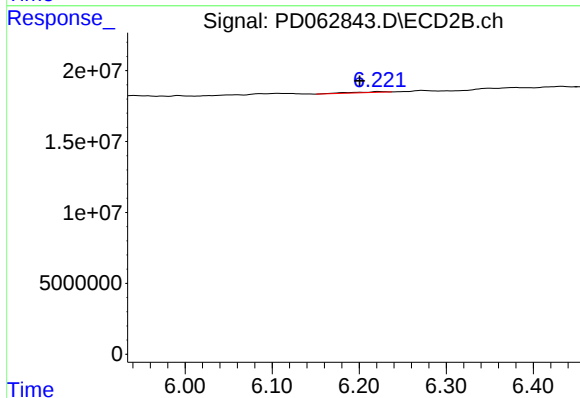


#9 Endosulfan I

R.T.: 6.223 min
Delta R.T.: 0.022 min
Response: 1763761
Conc: 0.12 ng/ml

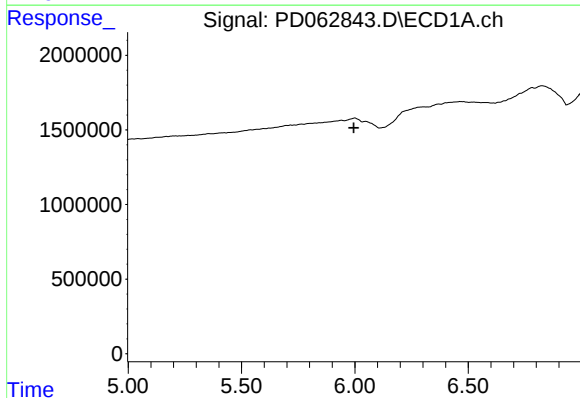


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

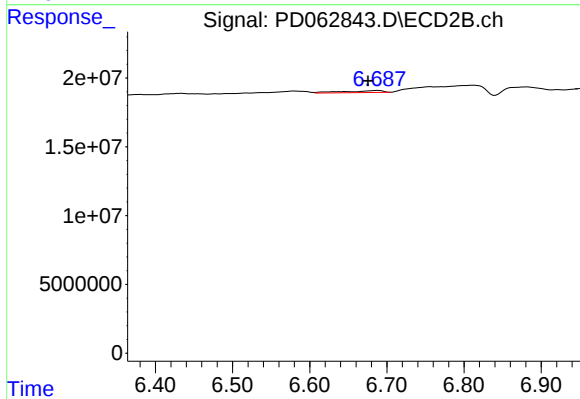

#14 Endrin


R.T.: 6.688 min
Delta R.T.: 0.013 min
Response: 4888220
Conc: 0.35 ng/ml

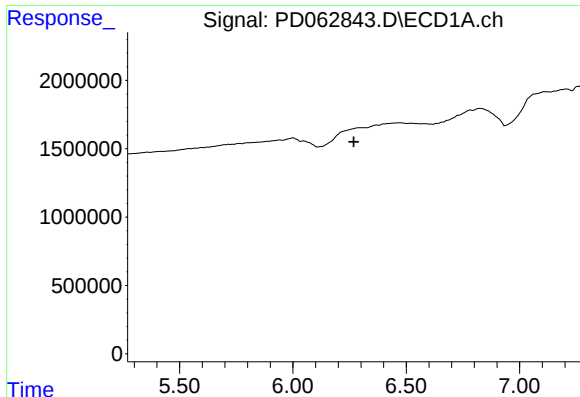

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

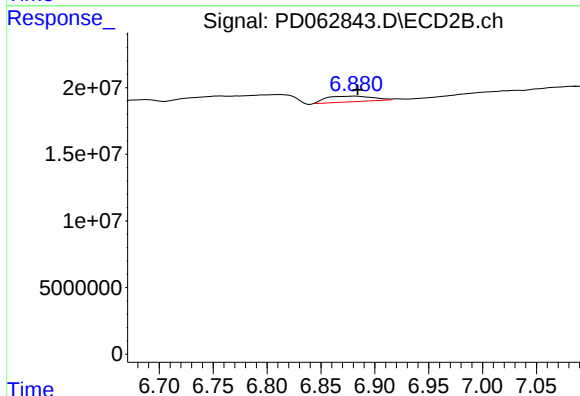


#15 Endosulfan II

R.T.: 6.881 min
Delta R.T.: -0.003 min
Response: 12731133
Conc: 0.95 ng/ml

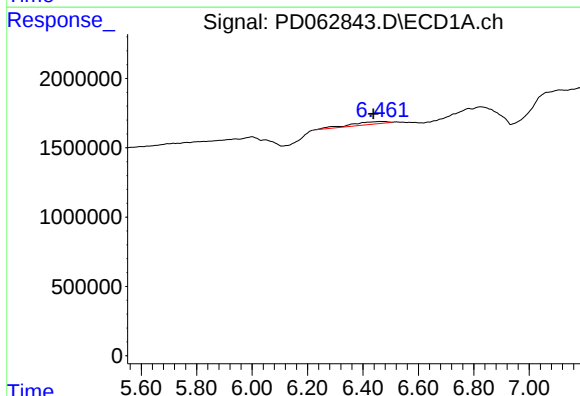


#18 Endrin aldehyde

R.T.: 6.463 min
Delta R.T.: 0.025 min
Response: 1755089
Conc: 1.88 ng/ml

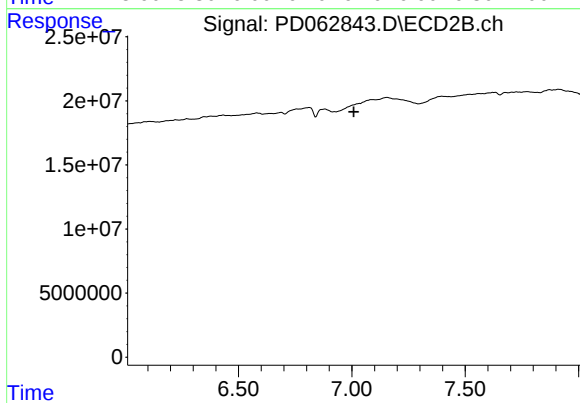

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.009 min
Response: 0
Conc: N.D.

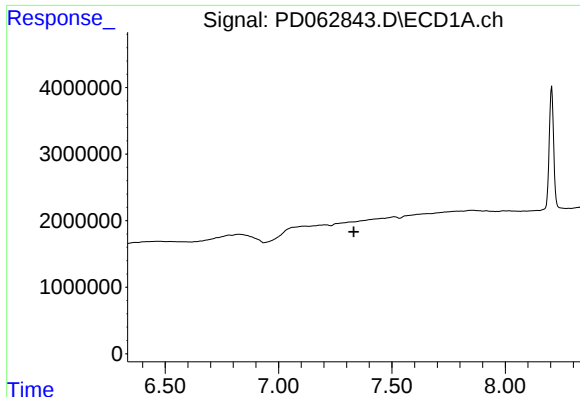

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

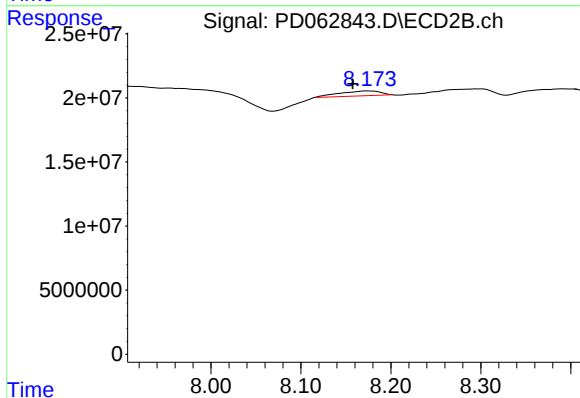


#22 Mirex

R.T.: 8.175 min
Delta R.T.: 0.017 min
Response: 12366862
Conc: 1.35 ng/ml

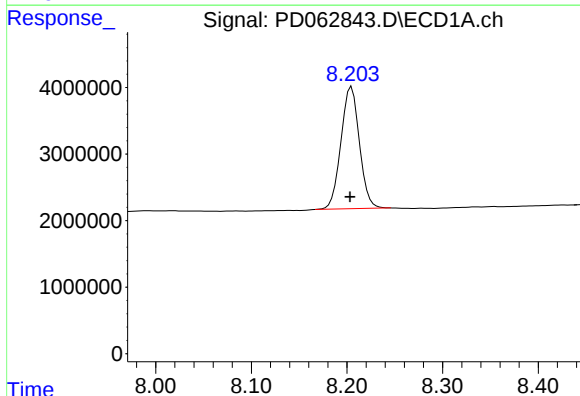

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.001 min
Response: 24696601
Conc: 23.33 ng/ml

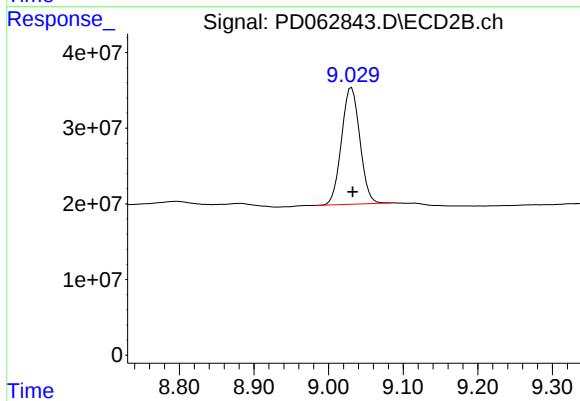

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.001 min
Response: 263655444
Conc: 22.85 ng/ml