

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051023\
 Data File : PD075429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 02:59
 Operator : AR\AJ
 Sample : 02694-16
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JREP6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/11/2023
 Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 05:16:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.771	23638370	12472899	10.364	11.826
2) SA Decachlor...	9.091	7.916	32257155	12426007	13.035	13.158
Target Compounds						
4) MA Heptachlor	4.917	3.939	4033150	1500727	1.082	1.027
17) MA 4,4'-DDT	7.078	6.054	15617463	7332159	6.153m	7.275m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051023\
Data File : PD075429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 02:59
Operator : AR\AJ
Sample : 02694-16
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 05:16:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

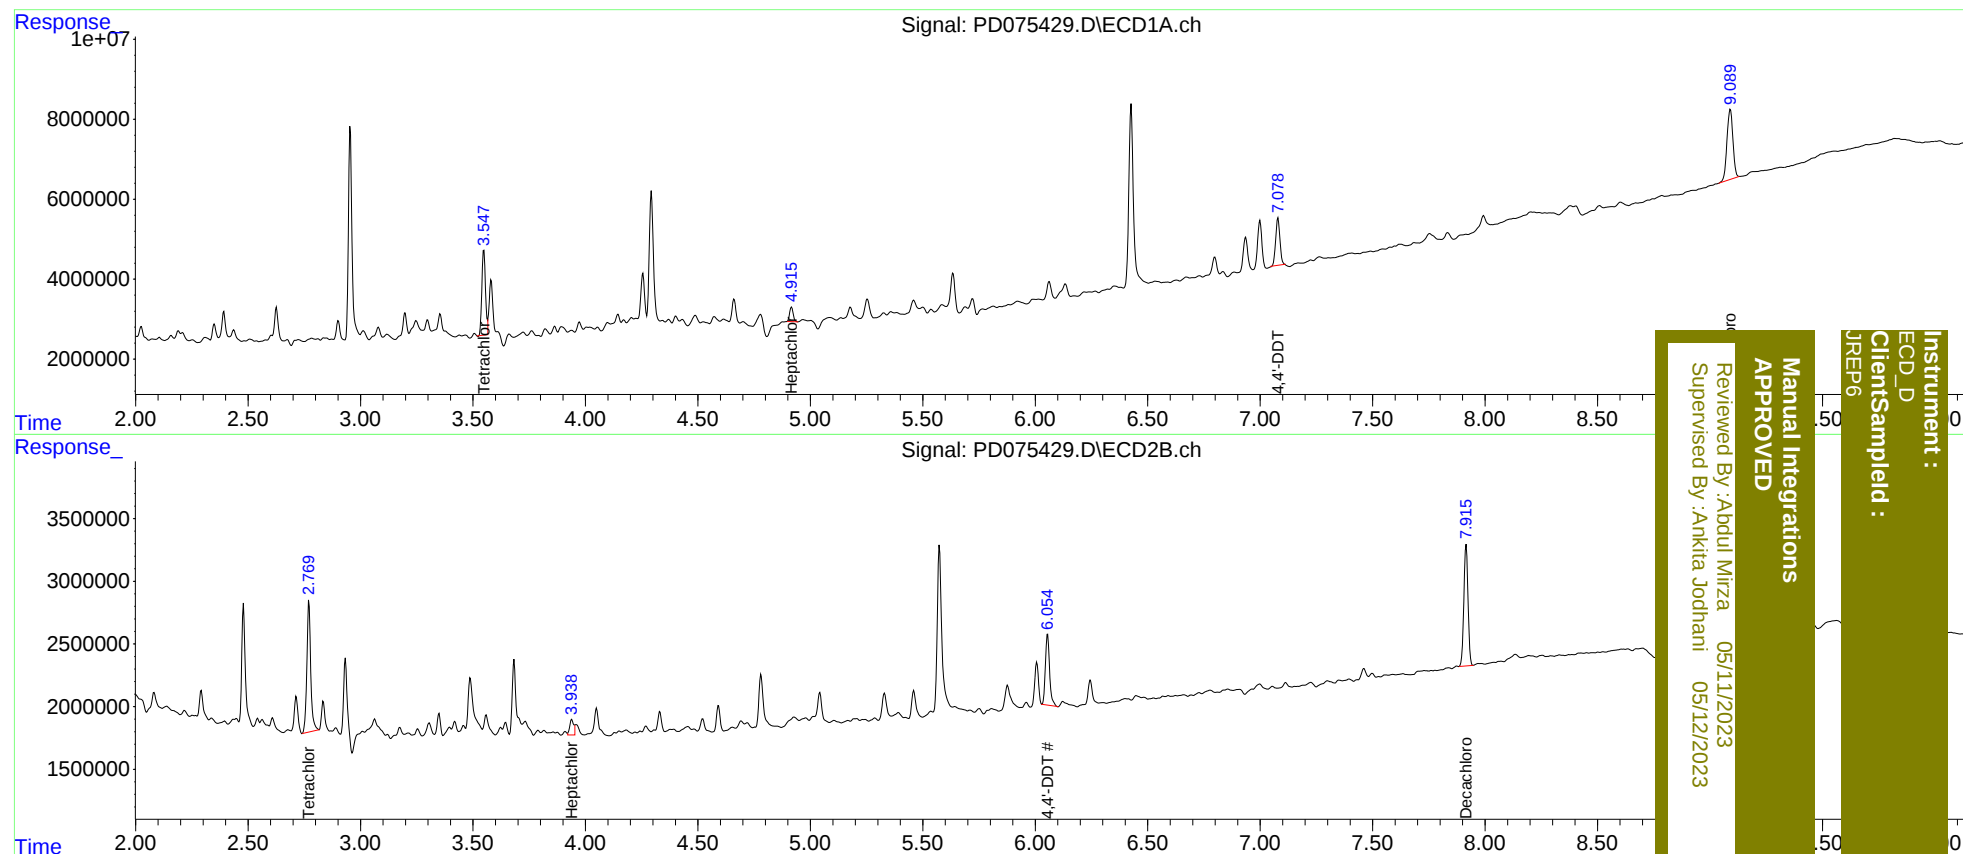

Reviewed By: Abdul Mirza 05/11/2023
Supervised By: Ankita Jodhani 05/12/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
JREP6