

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051121\
 Data File : PD062853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 15:58
 Operator : AR\AJ
 Sample : M2336-02MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG6K9MS

Manual Integrations
 APPROVED

Ankita
 5/11/2021 9:39:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 23:13:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	16750429	212.3E6	17.496m	17.483m
27)	SA Decachlor...	8.200	9.029	25505465	272.7E6	23.762	24.986
Target Compounds							
2)	A alpha-BHC	3.877	4.360	37605283	462.8E6	26.859	24.473
3)	MA gamma-BHC...	4.159	4.643	38979320	277.7E6	29.180m	16.078 #
4)	MA Heptachlor	4.462	5.152	34355450	393.9E6	26.756	22.630
5)	MB Aldrin	4.710	5.457	36628309	442.5E6	28.120	25.584
6)	B beta-BHC	4.411	4.814	17496226	193.8E6	28.181	25.386
7)	B delta-BHC	4.616	5.030	15860689	206.6E6	11.656	11.137m
8)	B Heptachlo...	5.153	5.843	31159257	412.2E6	25.426	25.702
9)	A Endosulfan I	5.491	6.198	30954909	396.5E6	27.683m	27.033m
10)	B trans-Chl...	5.381	6.077	33017110	408.5E6	26.337	24.942
11)	B cis-Chlor...	5.439	6.148	38666200	392.9E6	31.489	25.312m
12)	B 4,4'-DDE	5.603	6.307	62107217	746.6E6	50.185	47.649
13)	MA Dieldrin	5.737	6.456	76005444	819.8E6	60.297	52.870
14)	MA Endrin	5.994	6.674	62009650	744.4E6	58.605	59.691
15)	B Endosulfa...	6.266	6.882	65099783	719.8E6	62.770m	57.515m
16)	A 4,4'-DDD	6.120	6.795	54871265	666.8E6	55.104	53.654m
17)	MA 4,4'-DDT	6.361	7.093	54079449	612.4E6	57.738	51.579m
18)	B Endrin al...	6.436	7.005	58650058	566.4E6	65.733	51.914m
19)	B Endosulfa...	6.650	7.229	52072871	678.0E6	52.093	53.131m
20)	A Methoxychlor	6.907	7.554	154.6E6	1519.3E6	289.755m	268.039
21)	B Endrin ke...	7.142	7.700	85158038	783.5E6	72.666	63.663

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051121\
Data File : PD062853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 15:58
Operator : AR\AJ
Sample : M2336-02MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 23:13:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

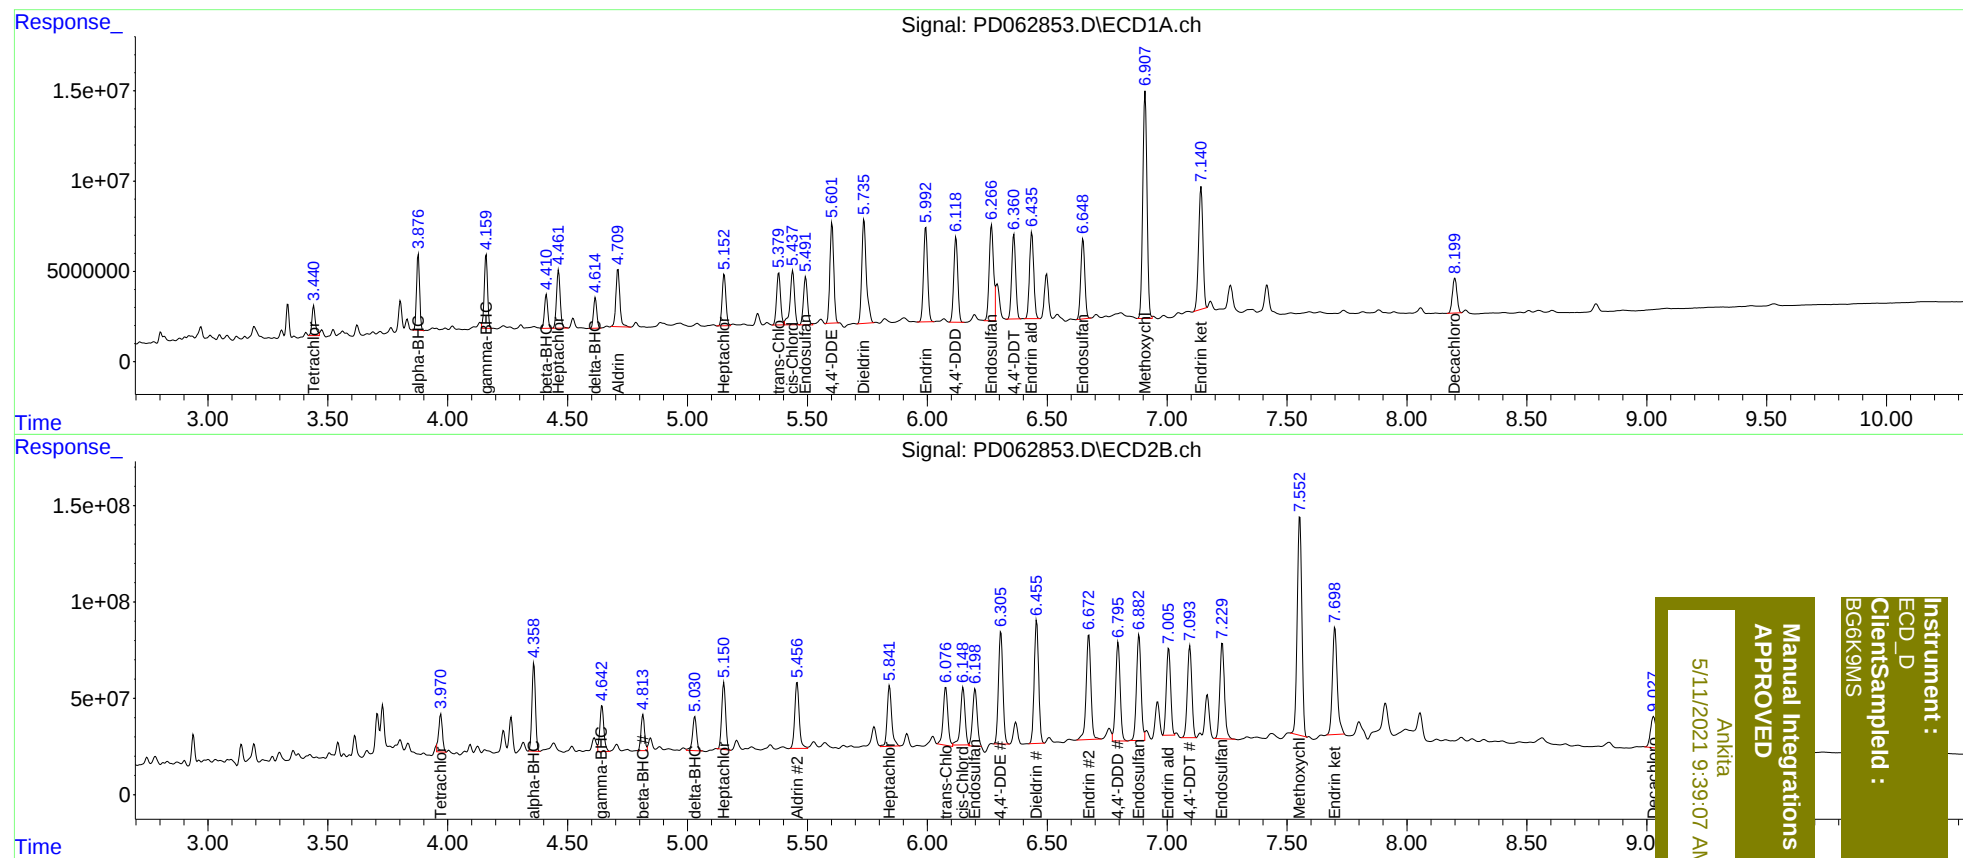

Manual Integrations
APPROVED

5/11/2021 9:39:07 AM
Ankita

Instrument :
ECD_D
ClientSampled :
BG6K9MS