

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051121\
 Data File : PD062854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2021 16:12
 Operator : AR\AJ
 Sample : M2336-03MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG6K9MSD

Manual Integrations
 APPROVED

Ankita
 5/11/2021 9:39:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 23:13:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	15790657	211.6E6	16.493m	17.425m
27)	SA Decachlor...	8.201	9.030	25209888	267.1E6	23.486	24.469
Target Compounds							
2)	A alpha-BHC	3.878	4.360	37458605	456.8E6	26.754	24.153
3)	MA gamma-BHC...	4.160	4.643	39070109	274.8E6	29.248m	15.905 #
4)	MA Heptachlor	4.463	5.152	34786741	389.4E6	27.092	22.371
5)	MB Aldrin	4.711	5.457	36739569	438.4E6	28.205	25.343
6)	B beta-BHC	4.412	4.814	17499284	192.0E6	28.186	25.157
7)	B delta-BHC	4.616	5.030	15818189	197.1E6	11.625	10.625m
8)	B Heptachlo...	5.154	5.843	31040256	409.8E6	25.329	25.552
9)	A Endosulfan I	5.493	6.198	29159164	383.0E6	26.077	26.111m
10)	B trans-Chl...	5.381	6.077	32417830	403.8E6	25.859	24.657
11)	B cis-Chlor...	5.439	6.148	37602700	368.7E6	30.622	23.752m
12)	B 4,4'-DDE	5.602	6.306	63302984	732.2E6	51.151m	46.730
13)	MA Dieldrin	5.737	6.456	75306688	808.3E6	59.742	52.124
14)	MA Endrin	5.994	6.674	61892433	732.5E6	58.495	58.730
15)	B Endosulfa...	6.267	6.882	70835468	724.4E6	68.301m	57.885m
16)	A 4,4'-DDD	6.120	6.795	54472984	650.1E6	54.704	52.304m
17)	MA 4,4'-DDT	6.361	7.094	53458068	607.9E6	57.074	51.199m
18)	B Endrin al...	6.436	7.006	58155724	567.6E6	65.179	52.024m
19)	B Endosulfa...	6.650	7.229	51412467	665.0E6	51.432	52.109m
20)	A Methoxychlor	6.909	7.554	152.0E6	1449.9E6	284.839	255.796
21)	B Endrin ke...	7.142	7.701	84474318	744.2E6	72.083	60.470

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051121\
Data File : PD062854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2021 16:12
Operator : AR\AJ
Sample : M2336-03MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 23:13:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

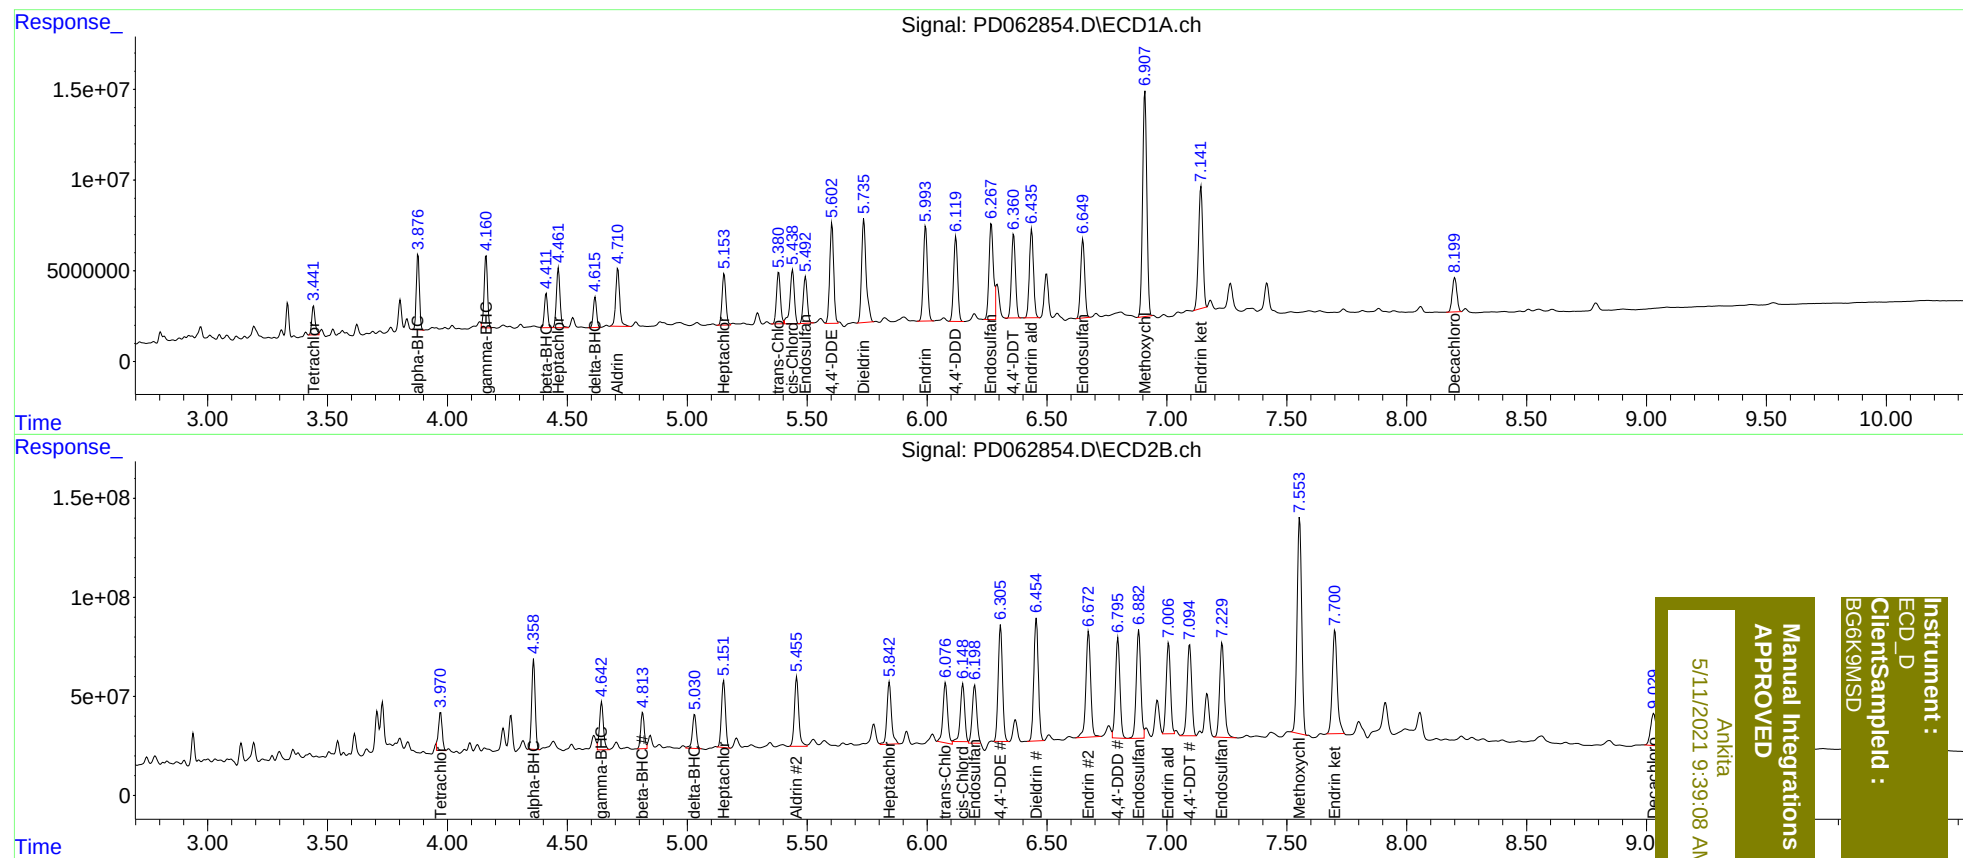

Manual Integrations
APPROVED

5/11/2021 9:39:08 AM
Ankita

Instrument :
ECD_D
ClientSampled :
BG6K9MSD