

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051122\
 Data File : PD069527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2022 16:35
 Operator : AR\AJ
 Sample : N2680-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B4-5-7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/11/2022
 Supervised By : mohammad ahmed 05/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 03:15:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.171	19954602	238.8E6	17.976	22.273
28) SA Decachlor...	8.195	9.362	16537127	89338959	13.244	13.652m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051122\
Data File : PD069527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2022 16:35
Operator : AR\AJ
Sample : N2680-08
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B4-5-7


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/11/2022
Supervised By : mohammad ahmed 05/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 03:15:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

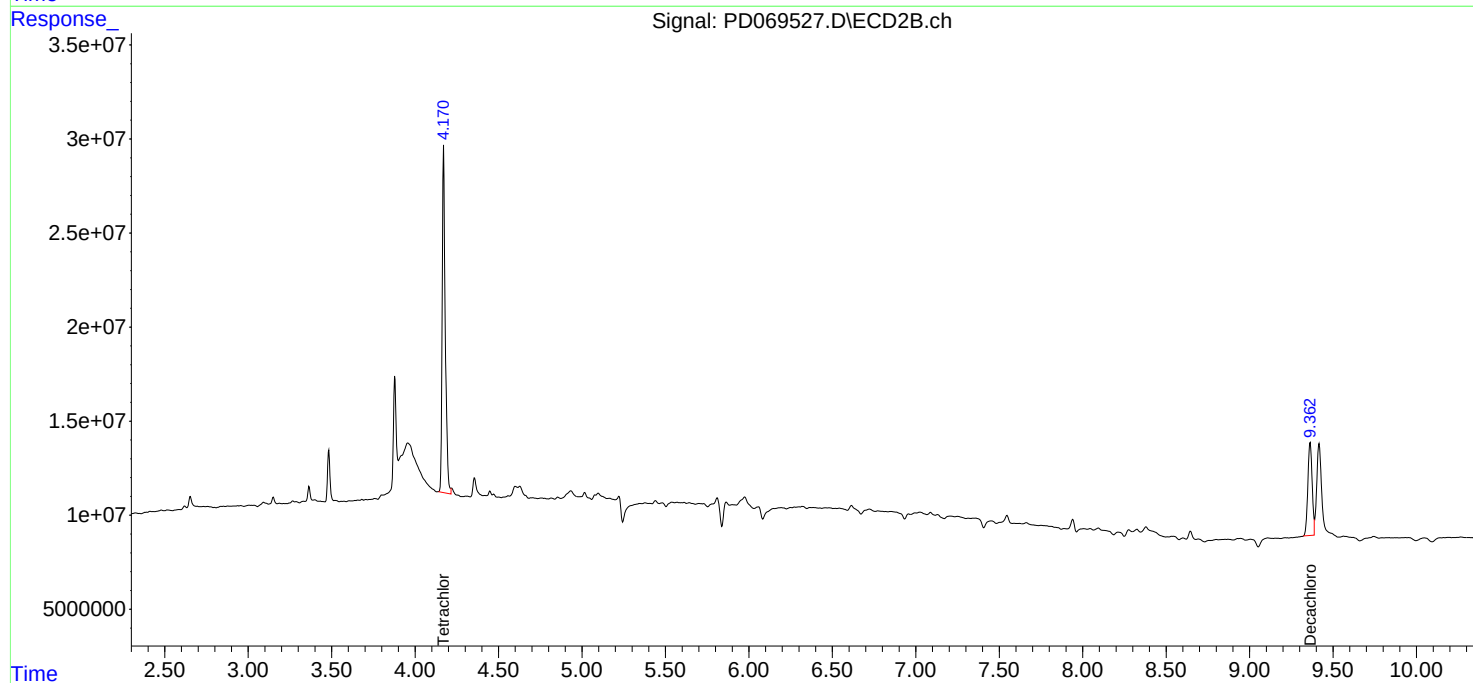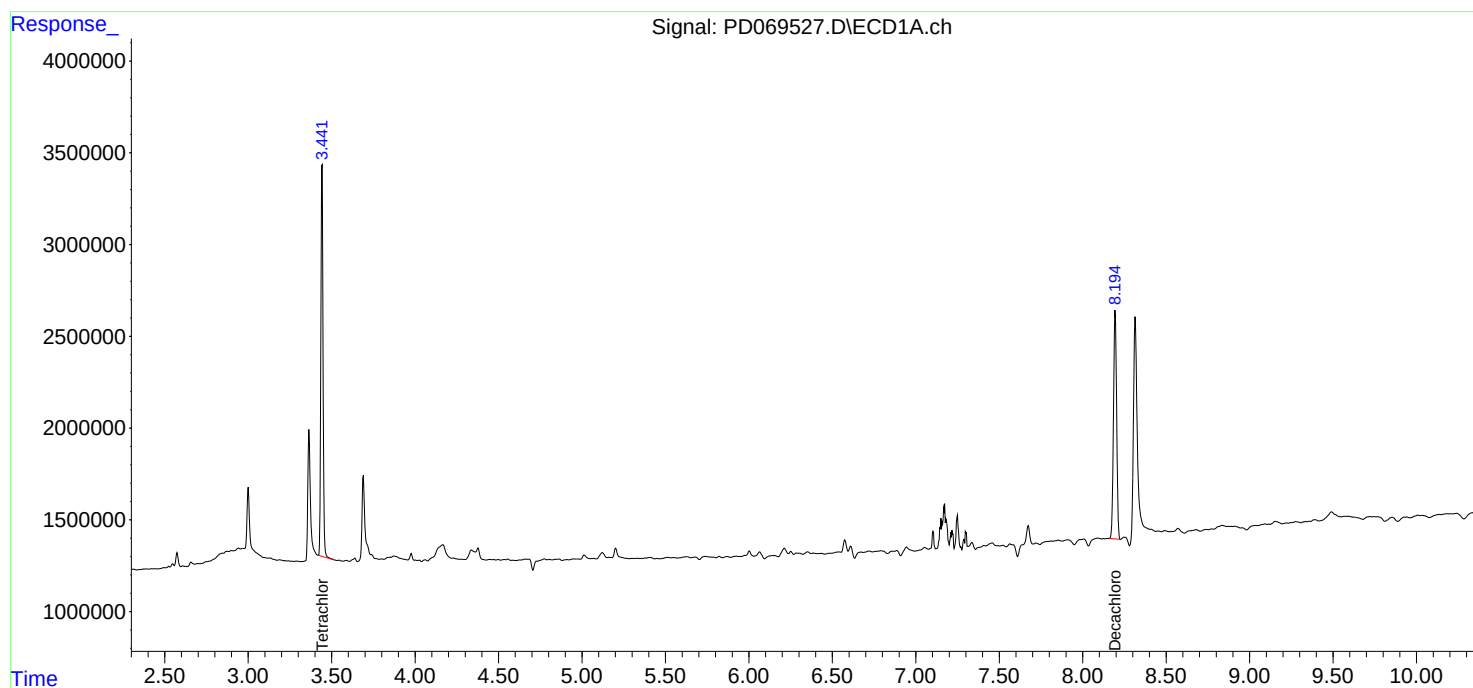

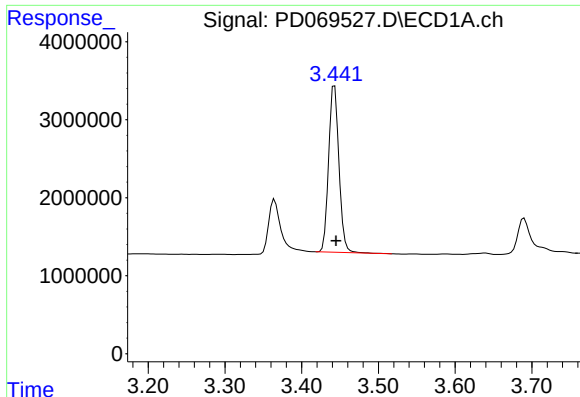


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 19954602
Conc: 17.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
B4-5-7


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/11/2022
Supervised By :mohammad ahmed 05/11/2022

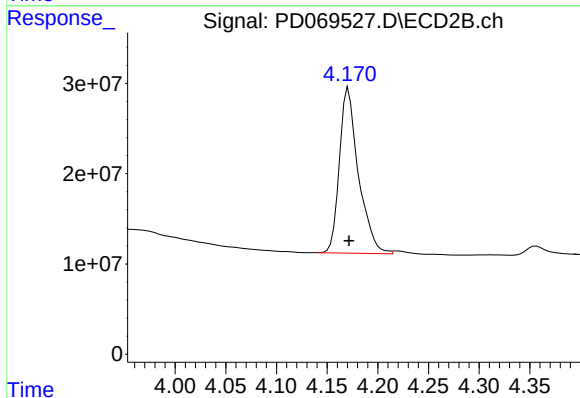


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 238803325
Conc: 22.27 ng/ml

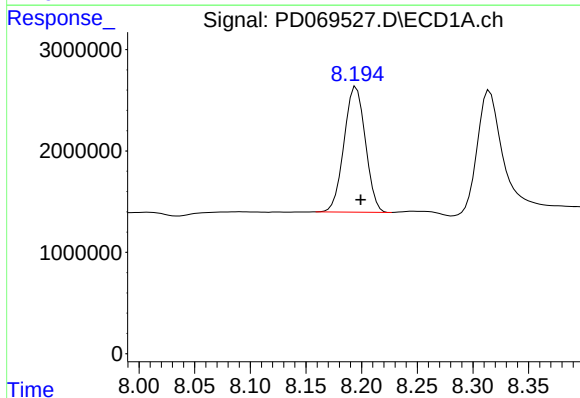

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: -0.004 min
Response: 16537127
Conc: 13.24 ng/ml

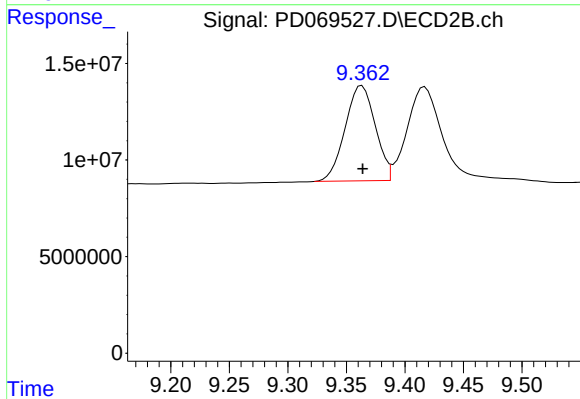

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.002 min
Response: 89338959
Conc: 13.65 ng/ml m