

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
 Data File : PD057870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 08:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 12:04:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.895	18514852	25378401	21.370	21.574
28)	SA Decachlor...	7.872	8.900	19817063	25913548	21.995	22.741
Target Compounds							
3)	MA gamma-BHC...	3.939f	0.000	3292149	0	2.383	N.D. #
23)	Chlordane-1	4.048	0.000	19462	0	0.691	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
Data File : PD057870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 08:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 12:04:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

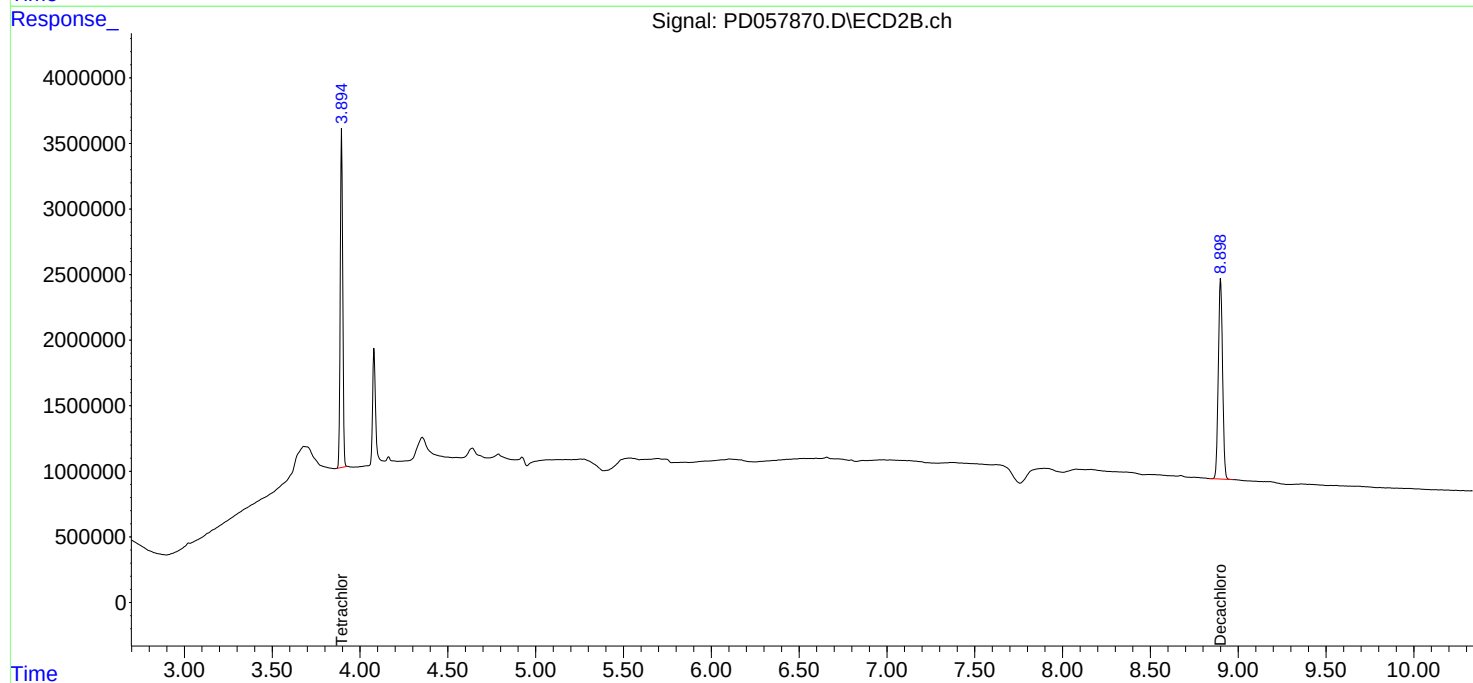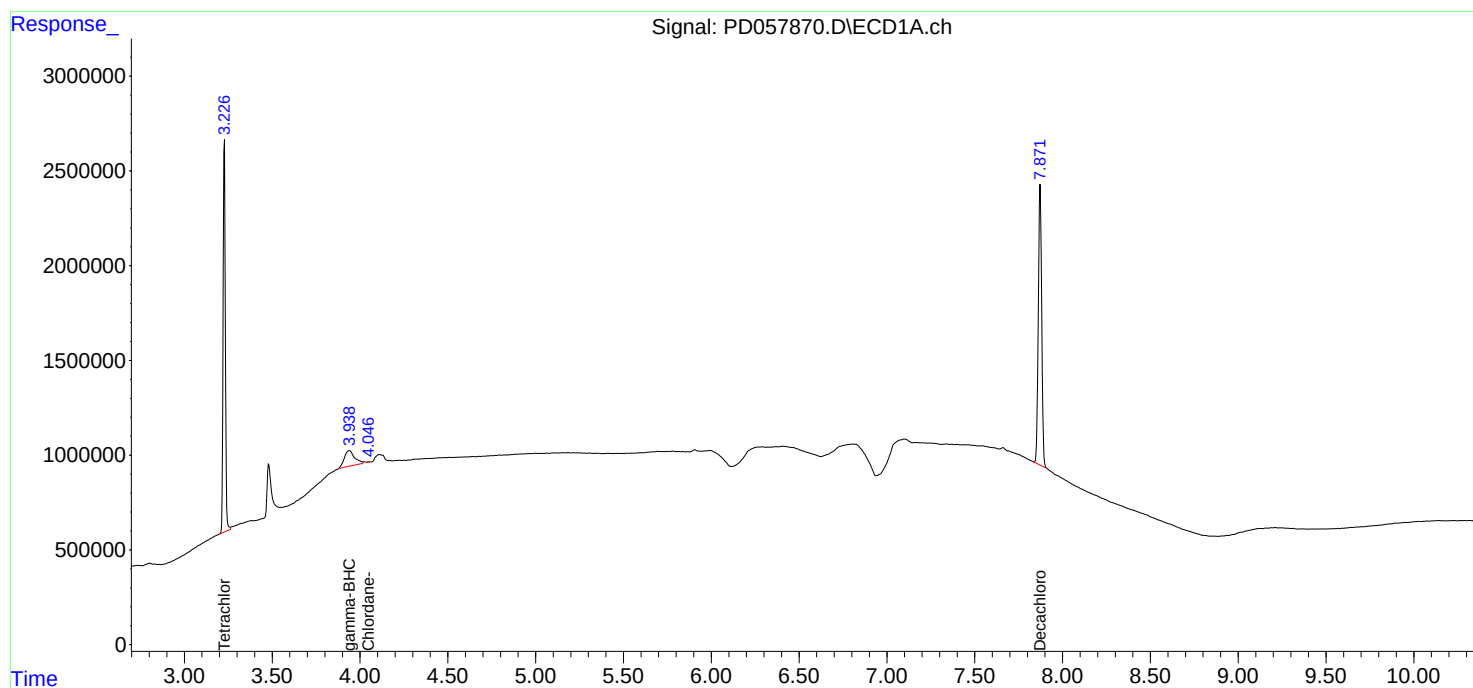


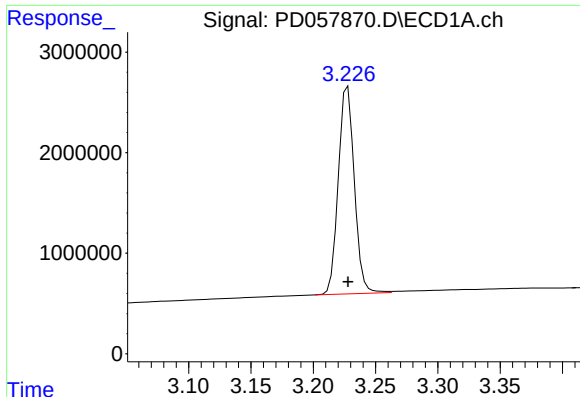

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 18514852
Conc: 21.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

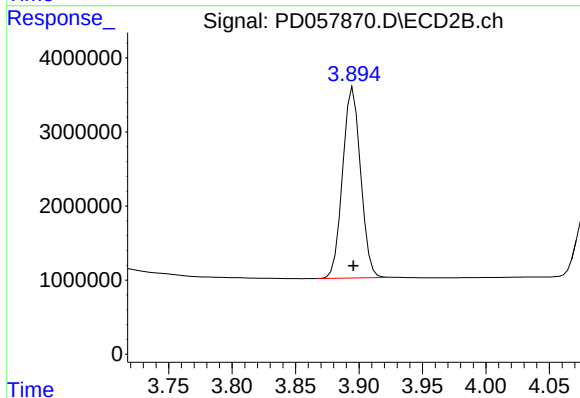


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 25378401
Conc: 21.57 ng/ml

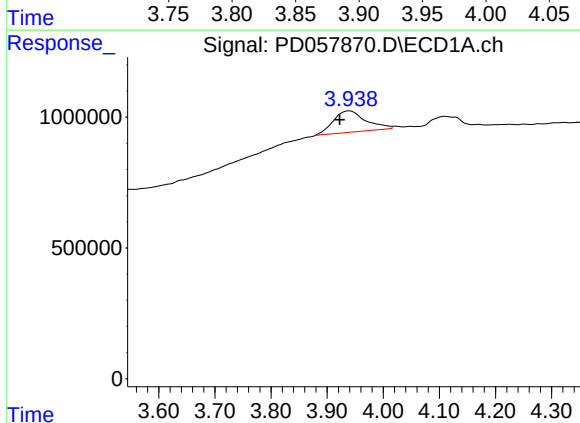


#3 gamma-BHC (Lindane)

R.T.: 3.939 min
Delta R.T.: 0.016 min
Response: 3292149
Conc: 2.38 ng/ml

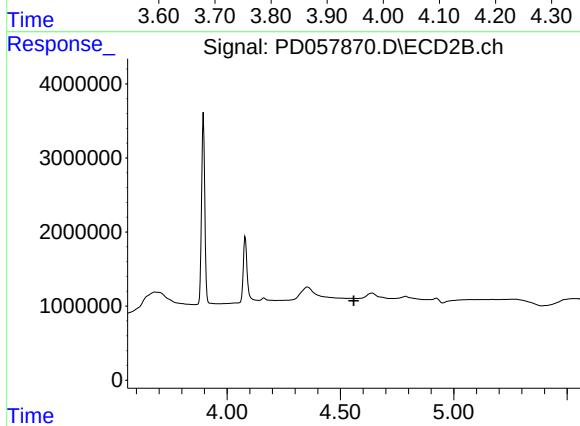

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

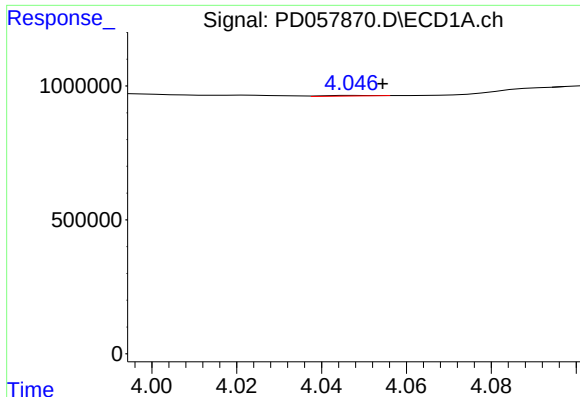

#23 Chlordane-1


R.T.: 4.048 min
Delta R.T.: -0.006 min
Response: 19462
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

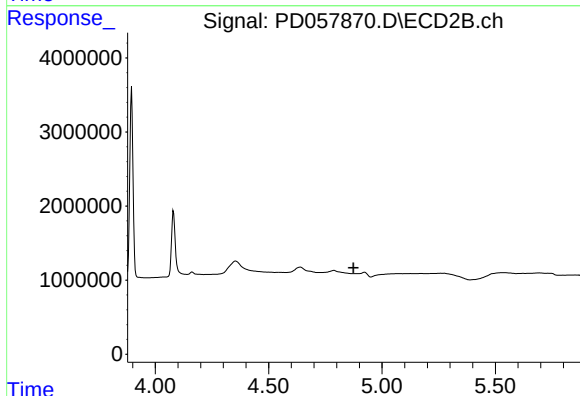


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

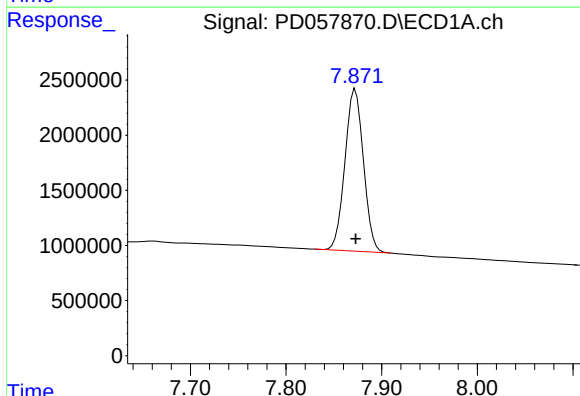

#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.000 min
Response: 19817063
Conc: 21.99 ng/ml

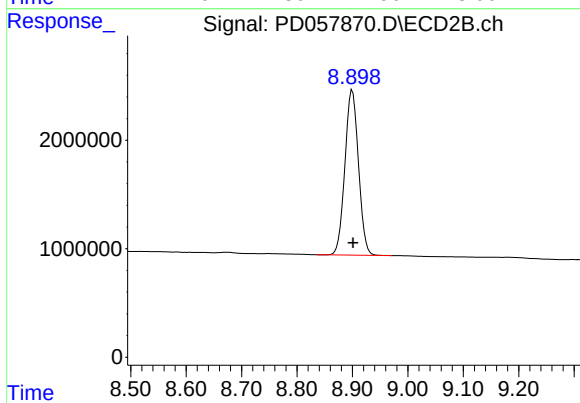

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.001 min
Response: 25913548
Conc: 22.74 ng/ml