

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
 Data File : PD057910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 19:09
 Operator : AJ\MA
 Sample : L2571-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:04:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.896	12283313	16905820	14.178	14.372
28)	SA Decachlor...	7.873	8.901	10040741	12412359	11.144	10.893
Target Compounds							
2)	A alpha-BHC	3.628f	0.000	90313	0	0.067	N.D. #
3)	MA gamma-BHC...	3.927	0.000	1504200	0	1.089	N.D. #
8)	B Heptachlo...	4.901f	0.000	564905	0	0.517	N.D. #
9)	A Endosulfan I	0.000	6.084	0	781252	N.D.	0.557 #
10)	B gamma-Chl...	5.090	5.966	419178	7417772	0.375	4.834 #
11)	B alpha-Chl...	5.157	0.000	624887	0	0.560	N.D. #
14)	MA Endrin	5.703	0.000	572969	0	0.589	N.D. #
25)	Chlordane-3	5.090	5.966	419178	7417772	4.140	39.115 #
26)	Chlordane-4	5.157	0.000	624887	0	6.743	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
Data File : PD057910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 19:09
Operator : AJ\MA
Sample : L2571-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:04:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

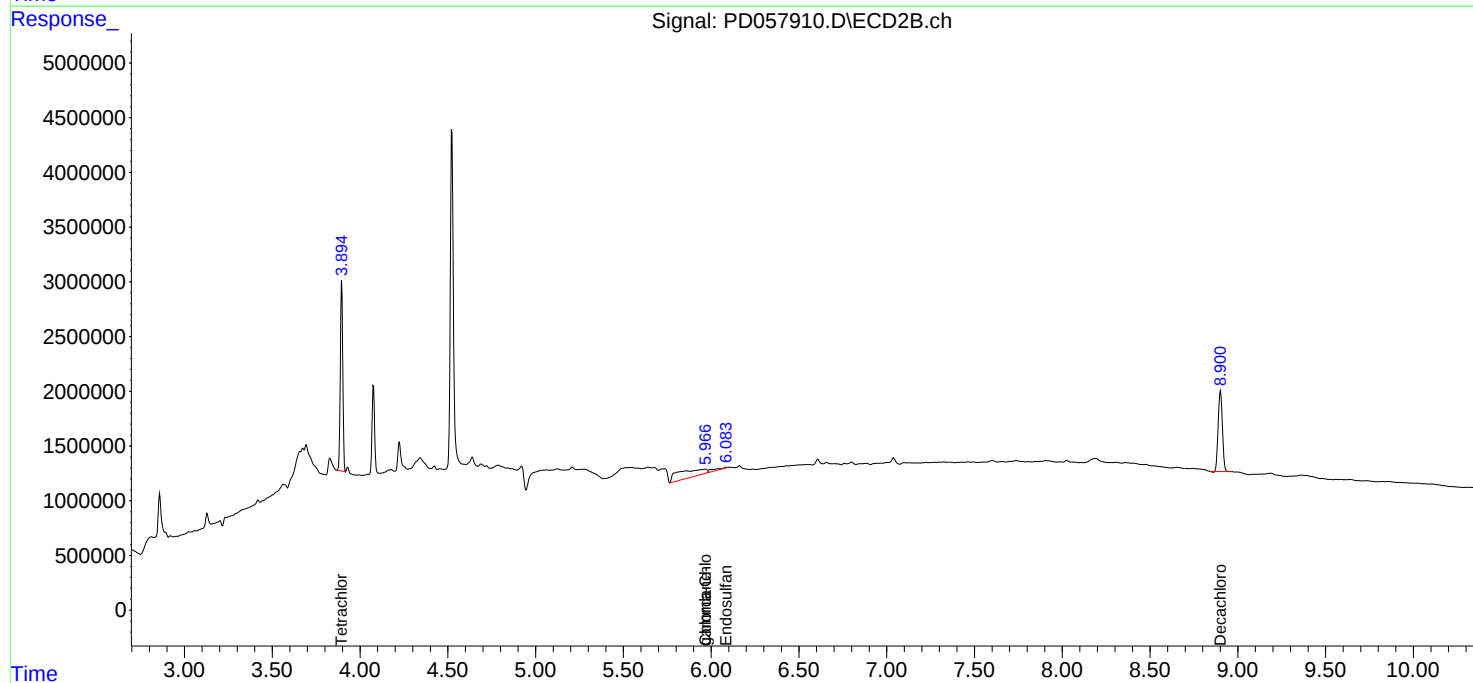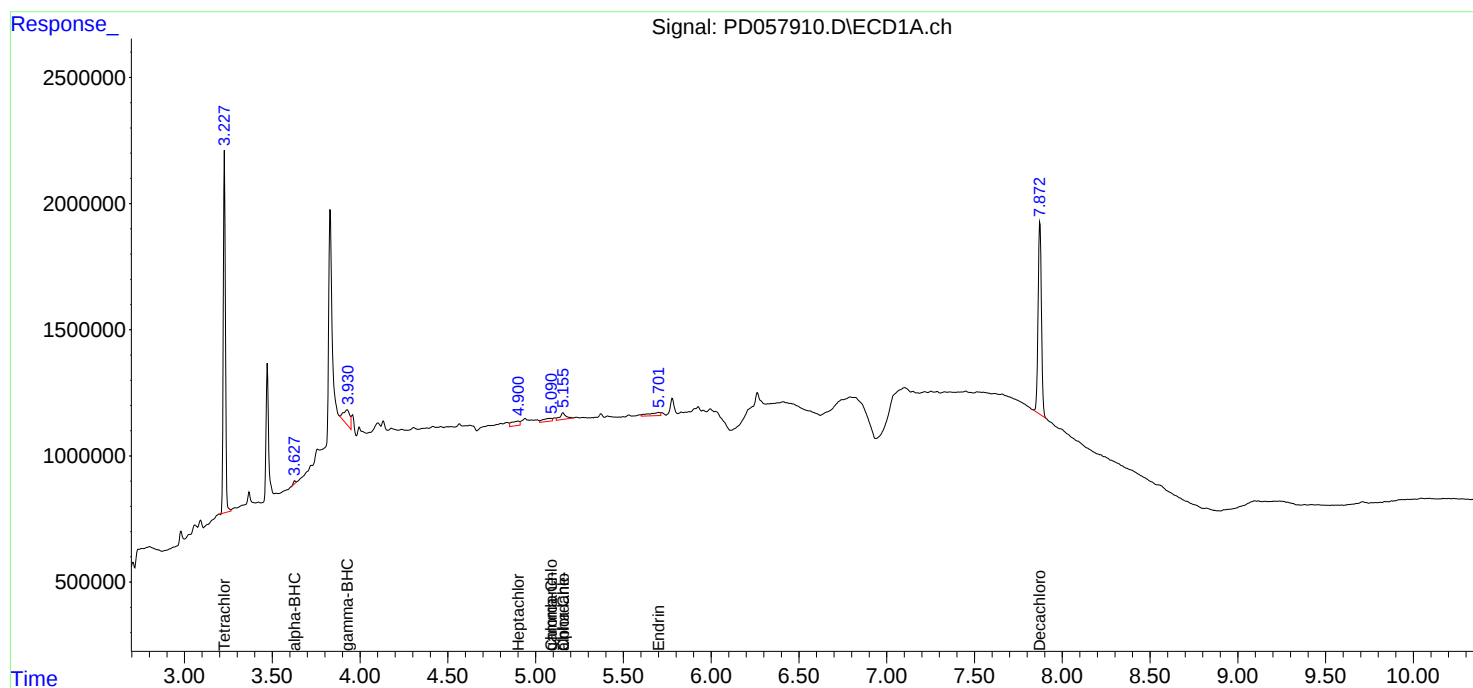


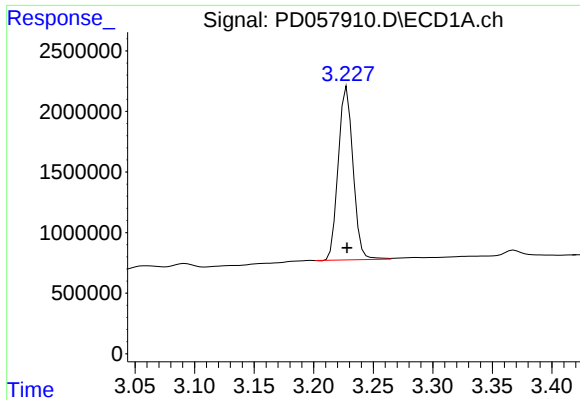

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 12283313
Conc: 14.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

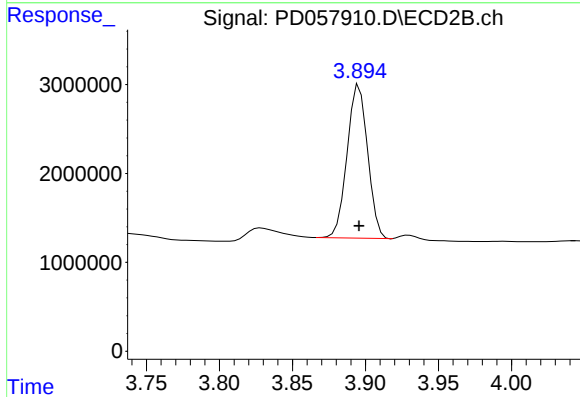


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 16905820
Conc: 14.37 ng/ml

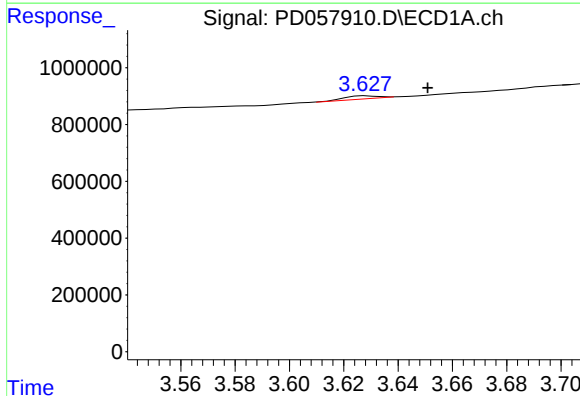


#2 alpha-BHC

R.T.: 3.628 min
Delta R.T.: -0.023 min
Response: 90313
Conc: 0.07 ng/ml

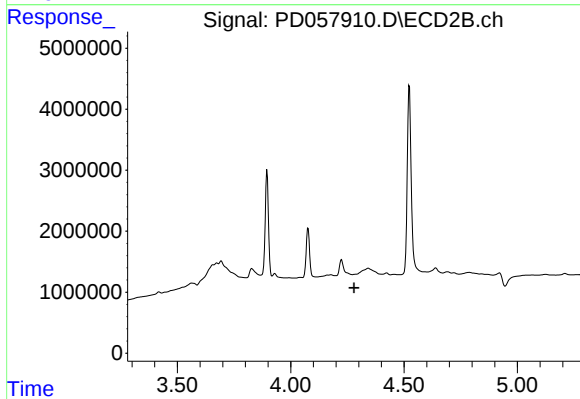

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.279 min
Response: 0
Conc: N.D.

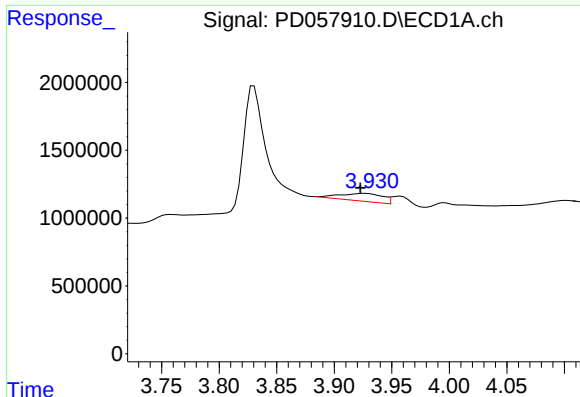

#3 gamma-BHC (Lindane)


R.T.: 3.927 min
Delta R.T.: 0.005 min
Response: 1504200
Conc: 1.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

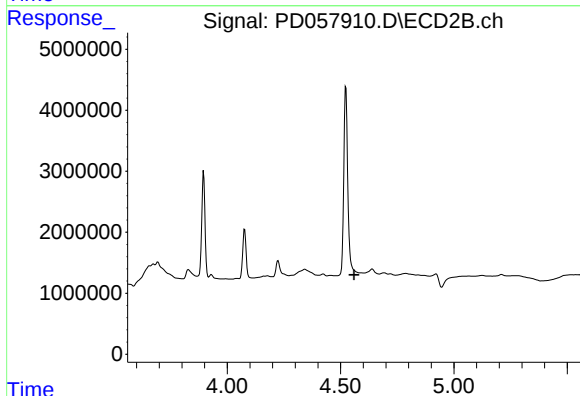


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

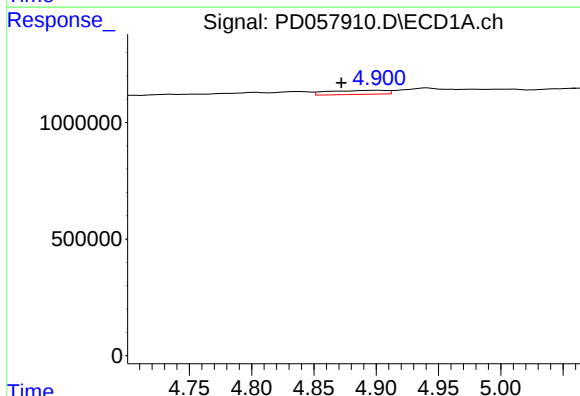


#8 Heptachlor epoxide

R.T.: 4.901 min
Delta R.T.: 0.029 min
Response: 564905
Conc: 0.52 ng/ml

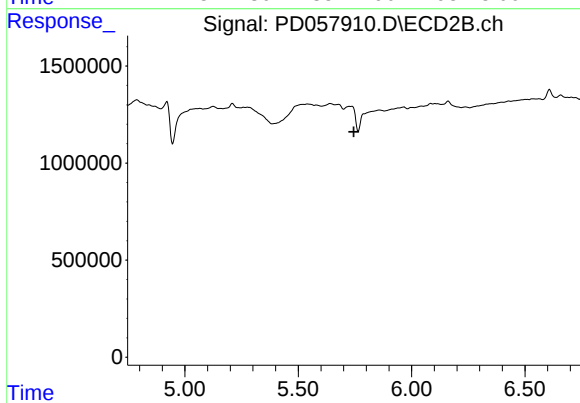

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.746 min
Response: 0
Conc: N.D.

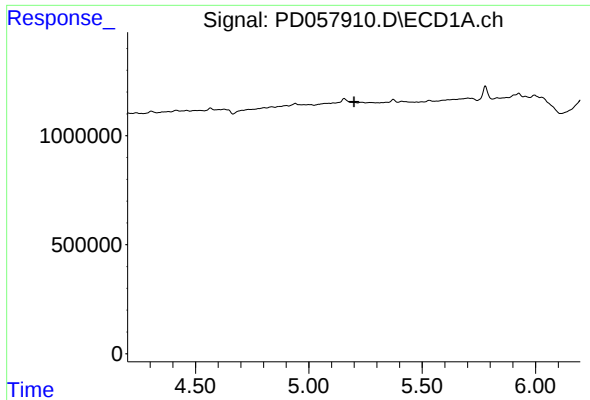

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

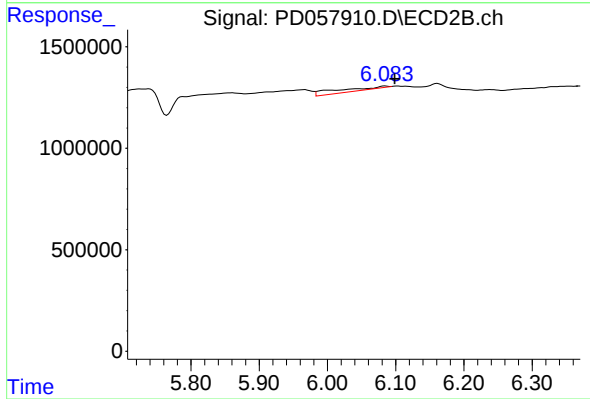


#9 Endosulfan I

R.T.: 6.084 min
Delta R.T.: -0.014 min
Response: 781252
Conc: 0.56 ng/ml

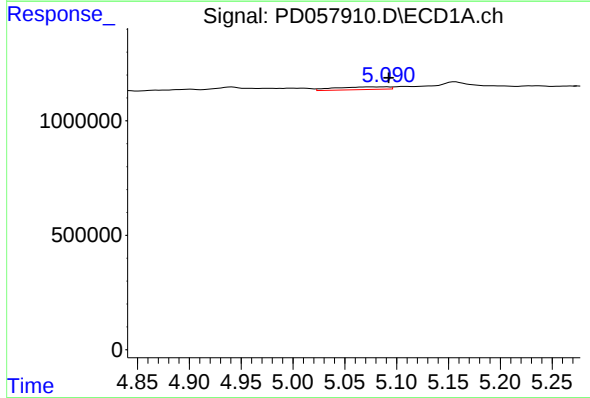


#10 gamma-Chlordane

R.T.: 5.090 min
Delta R.T.: -0.002 min
Response: 419178
Conc: 0.37 ng/ml

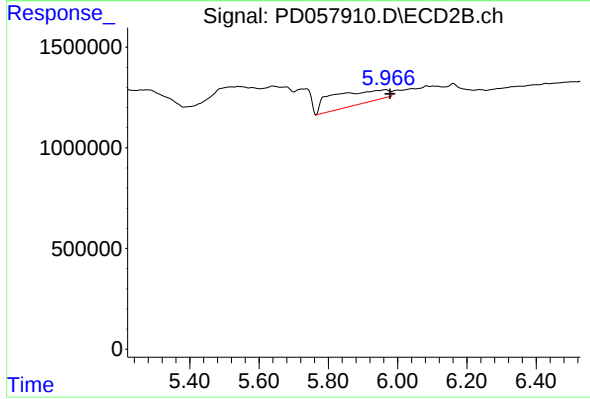

#10 gamma-Chlordane


R.T.: 5.966 min
Delta R.T.: -0.012 min
Response: 7417772
Conc: 4.83 ng/ml

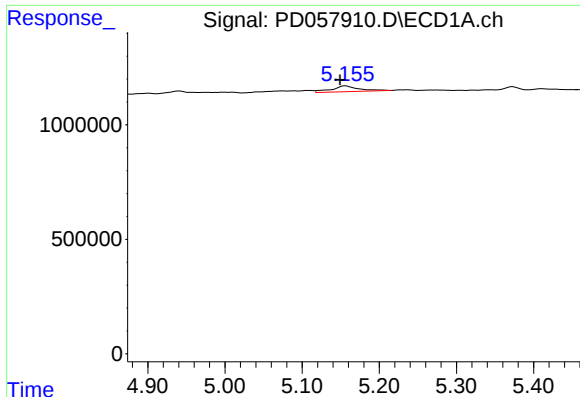

#11 alpha-Chlordane


R.T.: 5.157 min
Delta R.T.: 0.007 min
Response: 624887
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

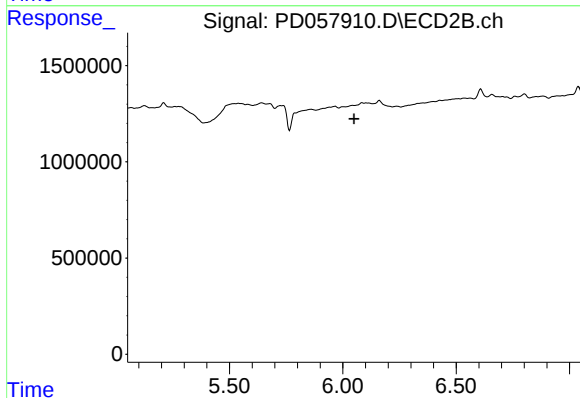


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

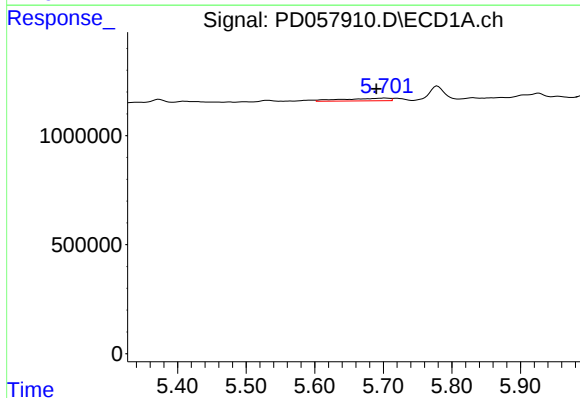


#14 Endrin

R.T.: 5.703 min
Delta R.T.: 0.013 min
Response: 572969
Conc: 0.59 ng/ml

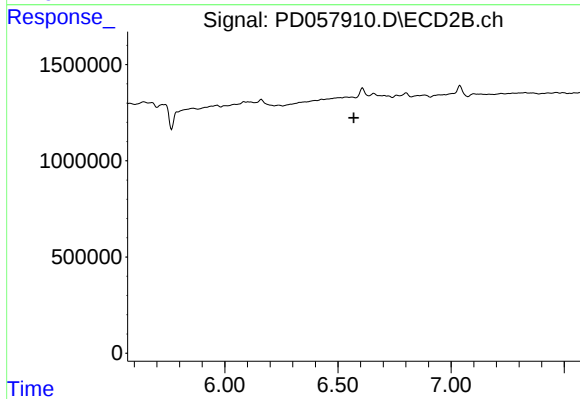

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

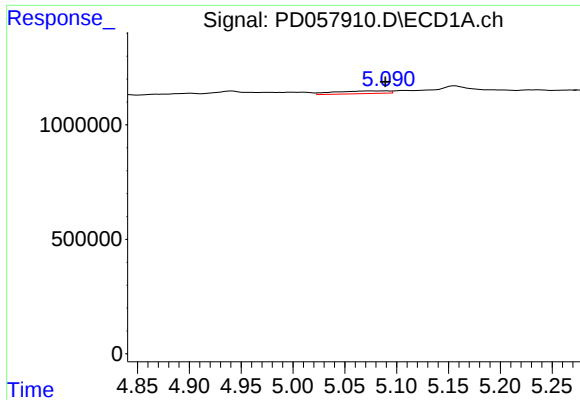

#25 Chlordane-3


R.T.: 5.090 min
Delta R.T.: 0.001 min
Response: 419178
Conc: 4.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

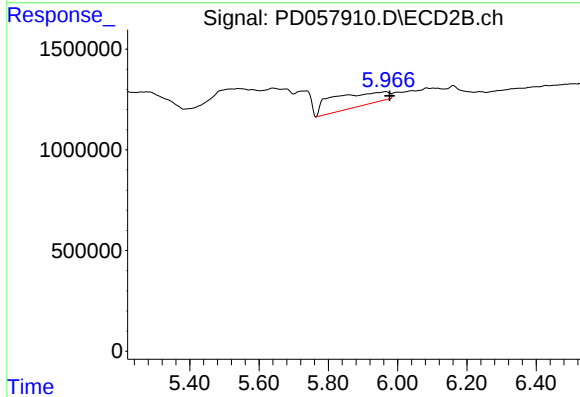


#25 Chlordane-3

R.T.: 5.966 min
Delta R.T.: -0.011 min
Response: 7417772
Conc: 39.11 ng/ml

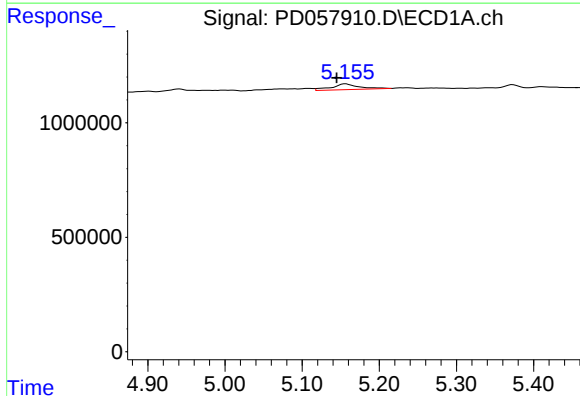


#26 Chlordane-4

R.T.: 5.157 min
Delta R.T.: 0.012 min
Response: 624887
Conc: 6.74 ng/ml

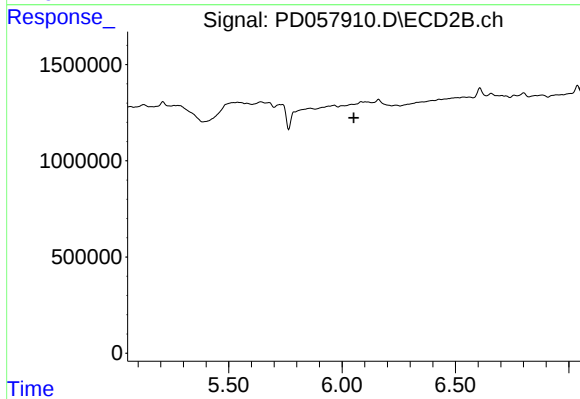

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.052 min
Response: 0
Conc: N.D.

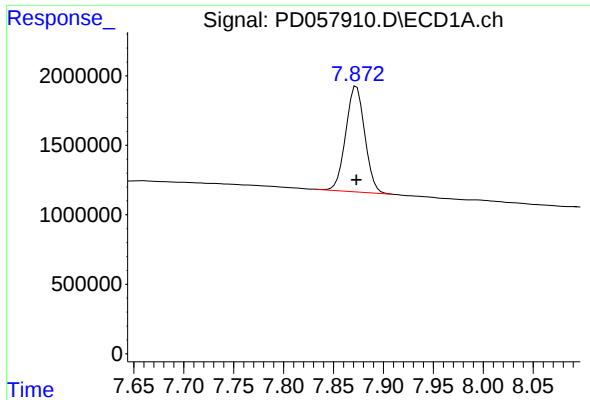

#28 Decachlorobiphenyl

R.T.: 7.873 min
Delta R.T.: 0.000 min
Response: 10040741
Conc: 11.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

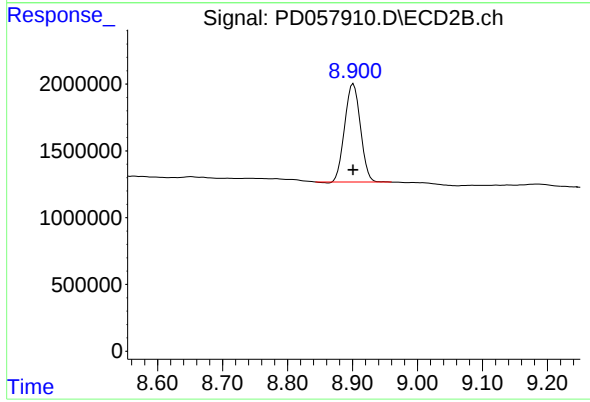

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 12412359
Conc: 10.89 ng/ml