

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
 Data File : PD057878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 11:03
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 11:58:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 11:58:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.232	3.896	45649406	55763699	50.000	50.000
28)	SA Decachlor...	7.879	8.903	41091777	52210195	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.063	4.875	14088881	22016558	500.000	500.000
24)	Chlordane-2	4.549	5.339	16889820	25542297	500.000	500.000
25)	Chlordane-3	5.100	5.980	50624564	94820684	500.000	500.000
26)	Chlordane-4	5.155	6.053	46337564	113.7E6	500.000	500.000
27)	Chlordane-5	5.973	6.853	16397890	20438076	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
Data File : PD057878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 11:03
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 11:58:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 11:58:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

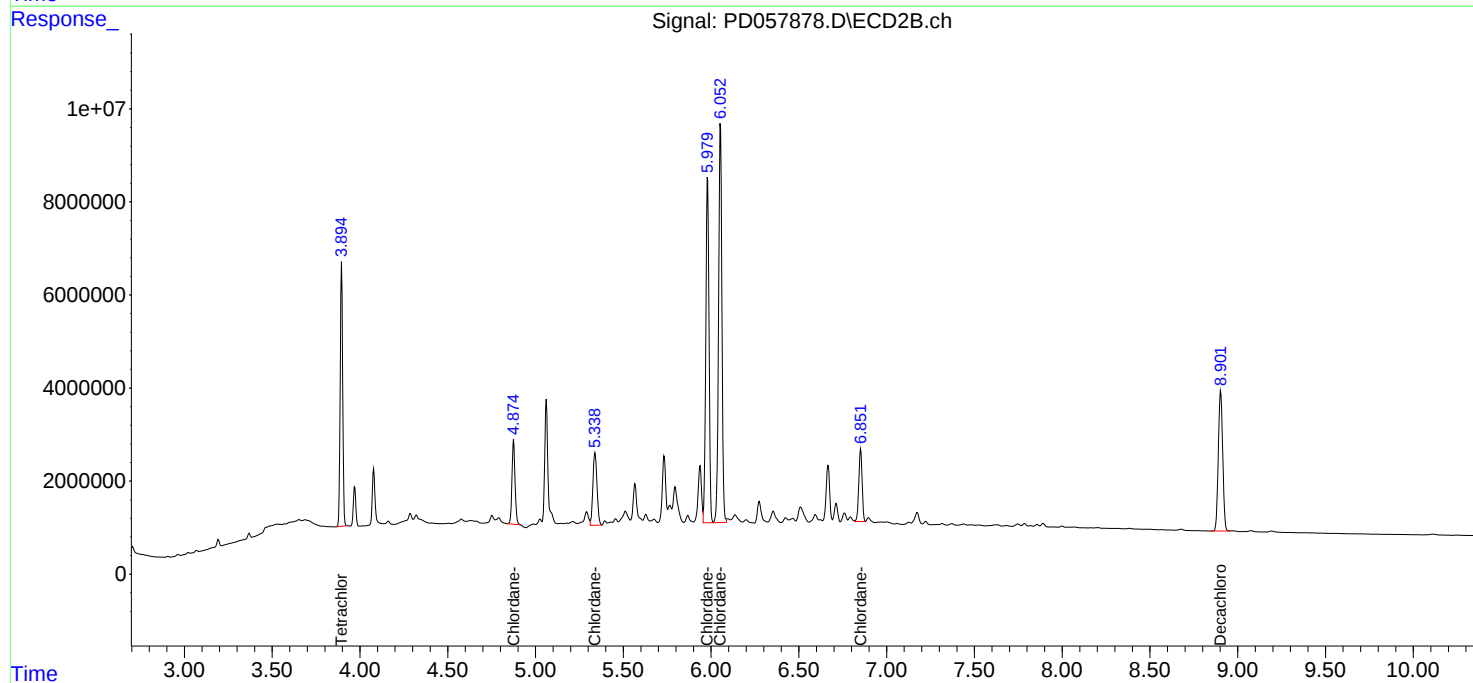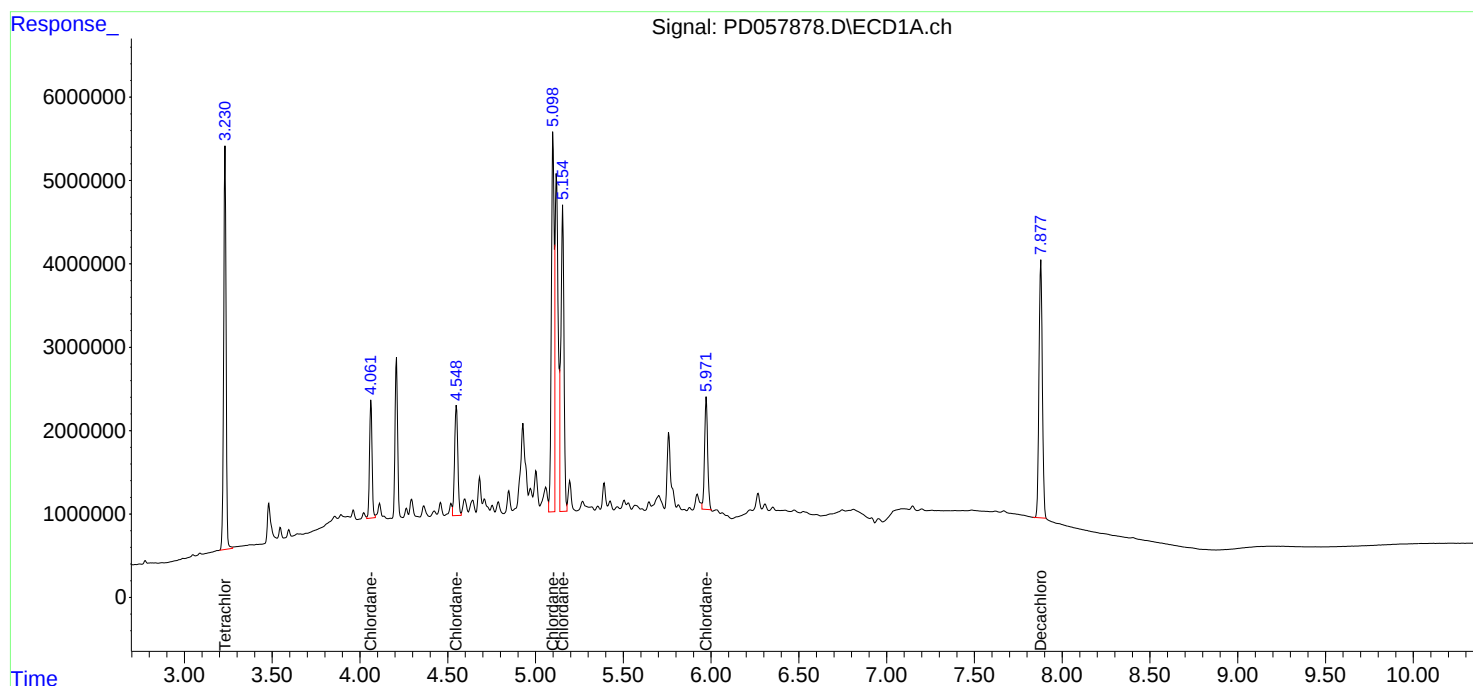


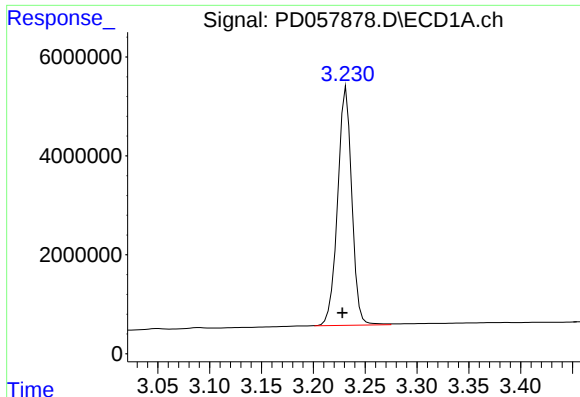

#1 Tetrachloro-m-xylene


R.T.: 3.232 min
Delta R.T.: 0.004 min
Response: 45649406
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

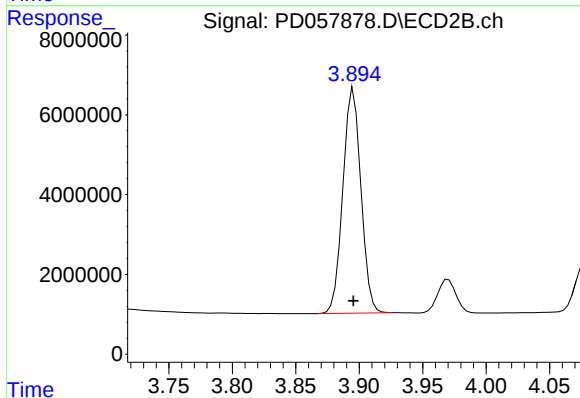


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 55763699
Conc: 50.00 ng/ml

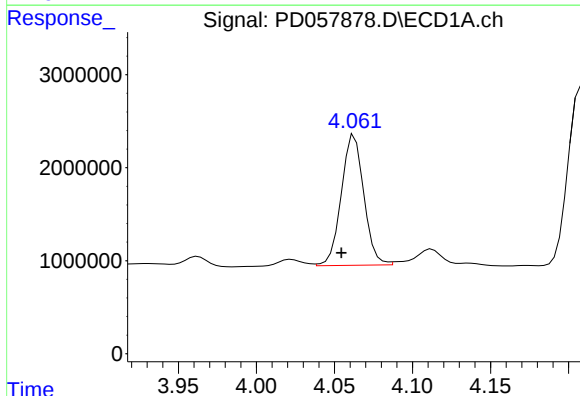


#23 Chlordane-1

R.T.: 4.063 min
Delta R.T.: 0.008 min
Response: 14088881
Conc: 500.00 ng/ml

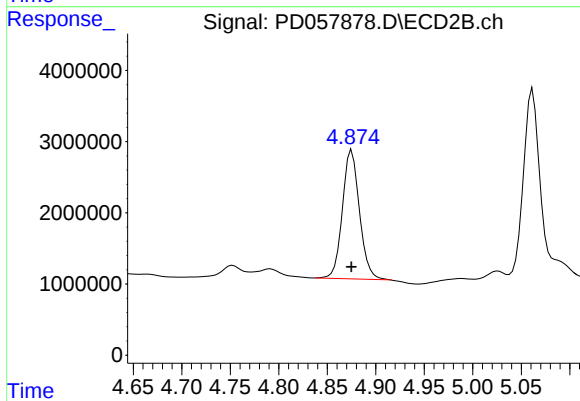

#23 Chlordane-1


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 22016558
Conc: 500.00 ng/ml

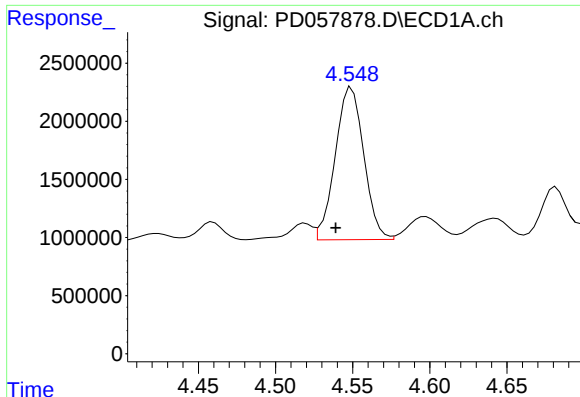

#24 Chlordane-2


R.T.: 4.549 min
Delta R.T.: 0.010 min
Response: 16889820
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

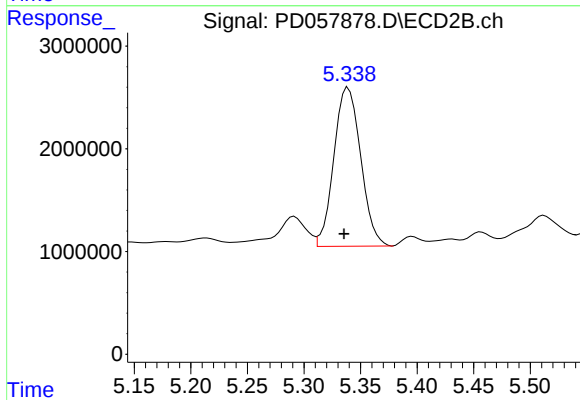


#24 Chlordane-2

R.T.: 5.339 min
Delta R.T.: 0.004 min
Response: 25542297
Conc: 500.00 ng/ml

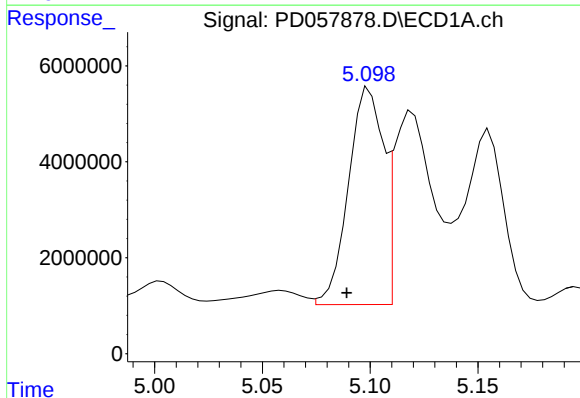


#25 Chlordane-3

R.T.: 5.100 min
Delta R.T.: 0.011 min
Response: 50624564
Conc: 500.00 ng/ml

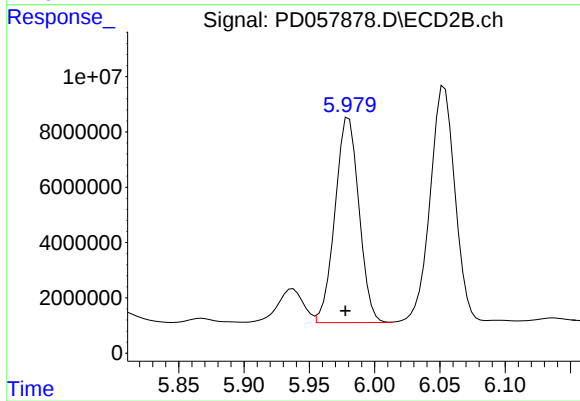

#25 Chlordane-3


R.T.: 5.980 min
Delta R.T.: 0.003 min
Response: 94820684
Conc: 500.00 ng/ml

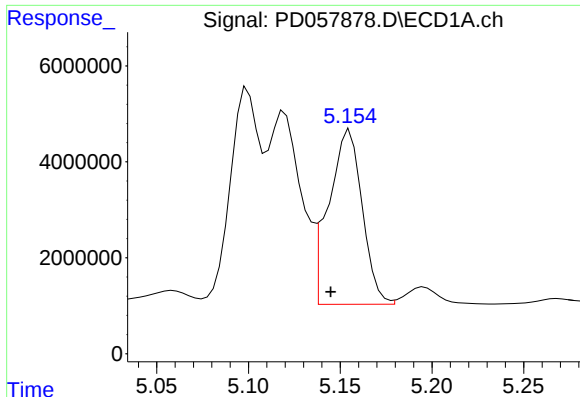

#26 Chlordane-4


R.T.: 5.155 min
Delta R.T.: 0.010 min
Response: 46337564
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

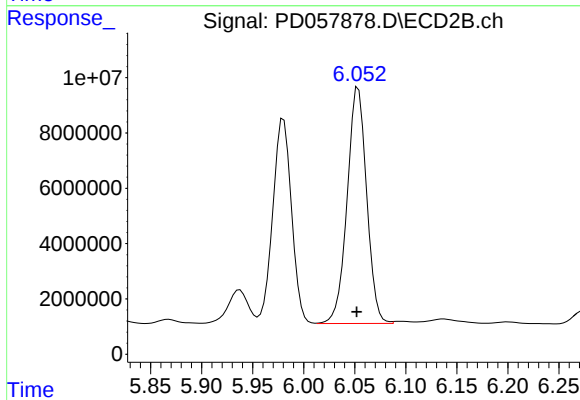


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.002 min
Response: 113656517
Conc: 500.00 ng/ml

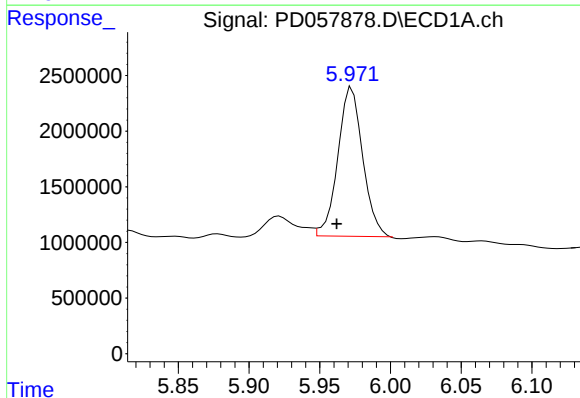


#27 Chlordane-5

R.T.: 5.973 min
Delta R.T.: 0.011 min
Response: 16397890
Conc: 500.00 ng/ml

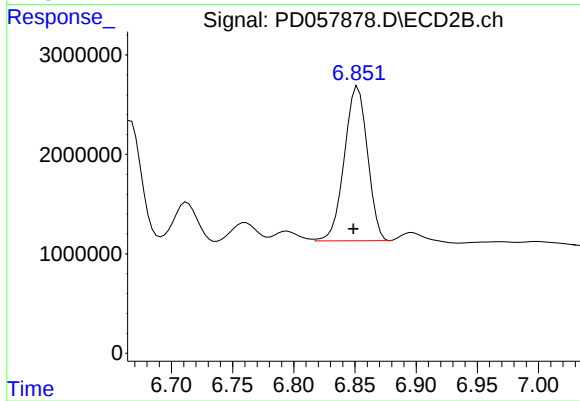

#27 Chlordane-5


R.T.: 6.853 min
Delta R.T.: 0.004 min
Response: 20438076
Conc: 500.00 ng/ml

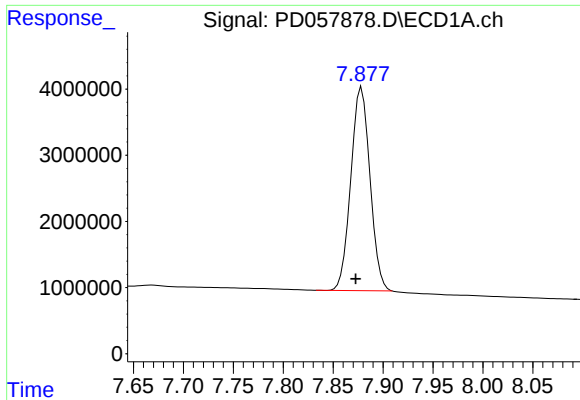

#28 Decachlorobiphenyl

R.T.: 7.879 min
Delta R.T.: 0.006 min
Response: 41091777
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

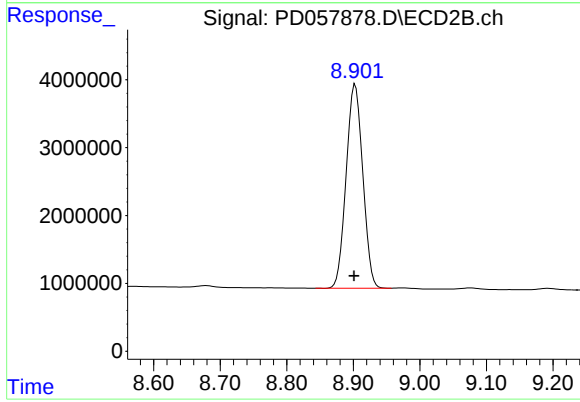

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.002 min
Response: 52210195
Conc: 50.00 ng/ml