

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
 Data File : PD057911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 19:23
 Operator : AJ\MA
 Sample : L2571-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BUS-LANE-3

Manual Integrations
 APPROVED

mohammad
 5/14/2020 12:05:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:05:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	17247447	23556255	19.907m	20.025
28)	SA Decachlor...	7.874	8.902	15017493	19742627	16.668	17.325

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051220\
Data File : PD057911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 19:23
Operator : AJ\MA
Sample : L2571-04
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BUS-LANE-3


Manual Integrations
APPROVED

mohammad
5/14/2020 12:05:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:05:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

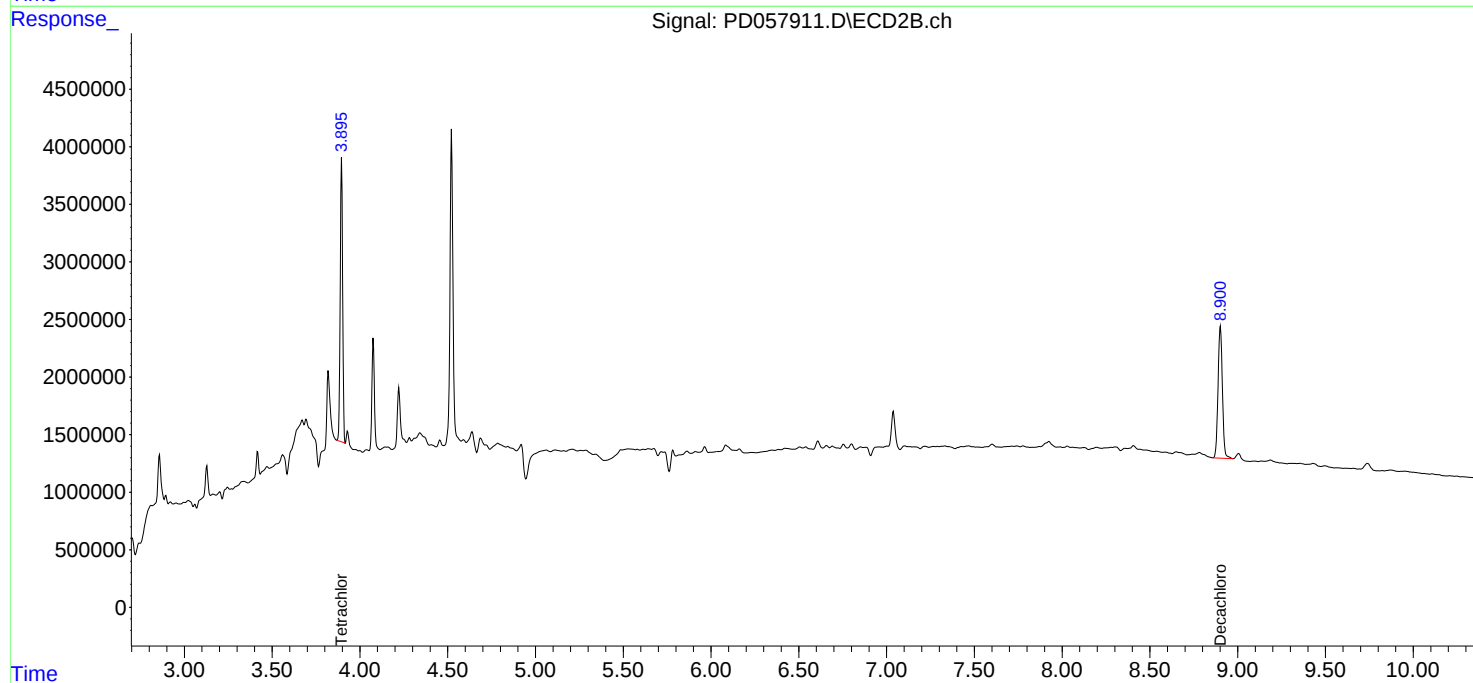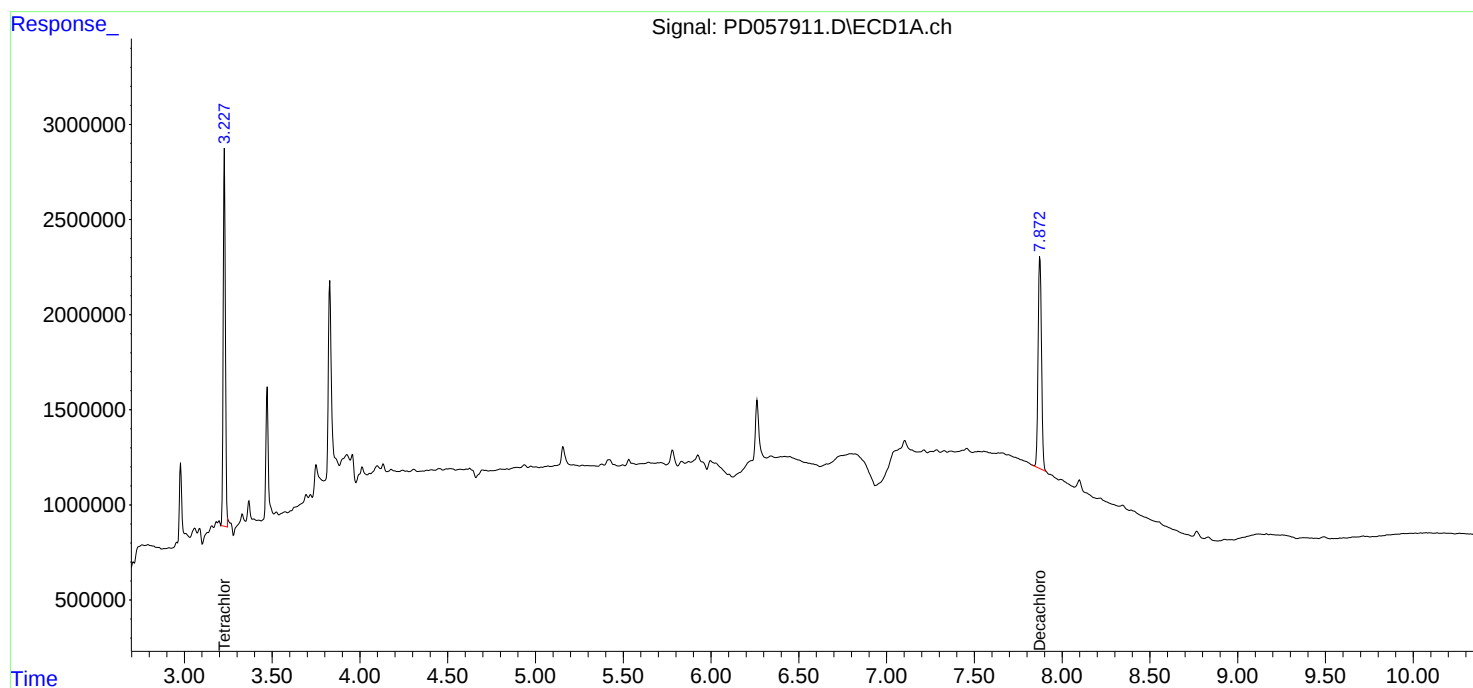

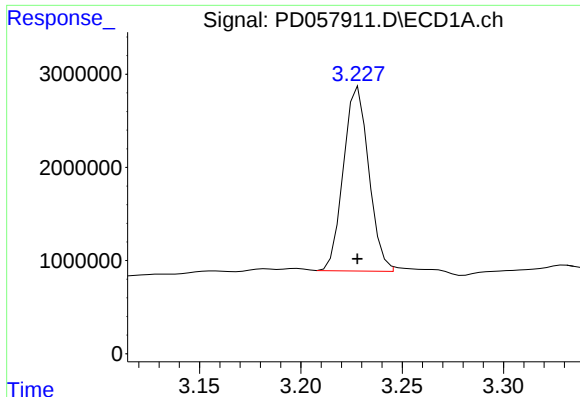


#1 Tetrachloro-m-xylene

R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 17247447
Conc: 19.91 ng/ml m

Instrument :
ECD_D
ClientSampleId :
BUS-LANE-3


Manual Integrations
APPROVED

mohammad
5/14/2020 12:05:19 PM

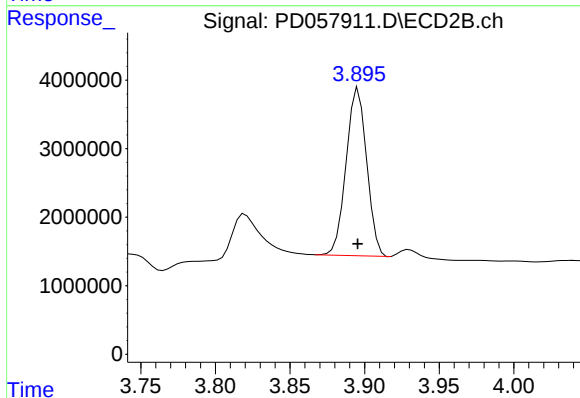


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 23556255
Conc: 20.03 ng/ml

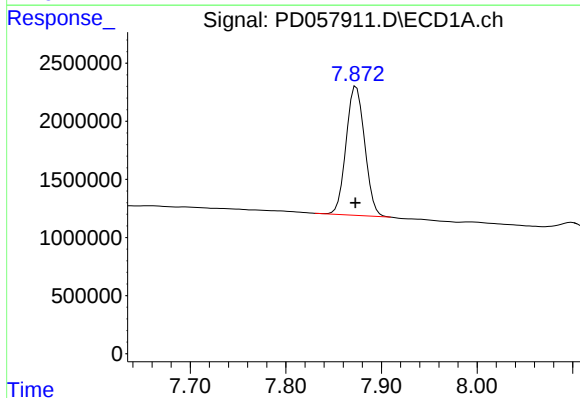

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: 0.000 min
Response: 15017493
Conc: 16.67 ng/ml

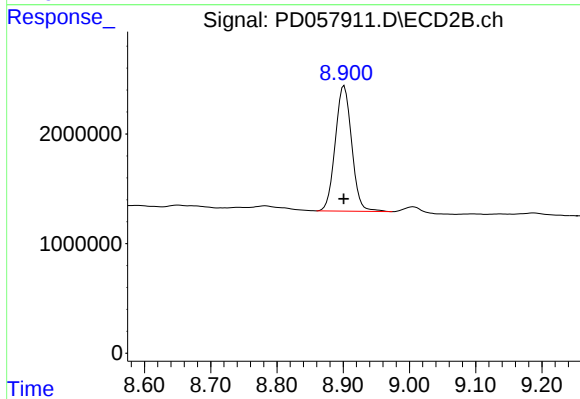

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 19742627
Conc: 17.33 ng/ml