

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
 Data File : PD062864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 10:34
 Operator : AR\AJ
 Sample : PB136254BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB136254BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 03:55:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	3.971	21195672	260.7E6	23.836	22.518
28)	SA Decachlor...	8.204	9.030	25862368	277.0E6	24.428	24.005
Target Compounds							
2)	A alpha-BHC	0.000	4.383f	0 14167248	N.D.	0.736	#
6)	B beta-BHC	4.379f	0.000	489665 0	0.817	N.D.	#
7)	B delta-BHC	0.000	5.008f	0 29949144	N.D.	1.659	#
8)	B Heptachlo...	0.000	5.854	0 9472936	N.D.	0.593	#
14)	MA Endrin	0.000	6.683	0 5114022	N.D.	0.364	#
15)	B Endosulfa...	0.000	6.898	0 10180998	N.D.	0.762	#
18)	B Endrin al...	6.439	0.000	673160 0	0.722	N.D.	#
27)	Chlordane-5	0.000	6.961	0 4786453	N.D.	9.732	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
Data File : PD062864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 10:34
Operator : AR\AJ
Sample : PB136254BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB136254BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 03:55:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

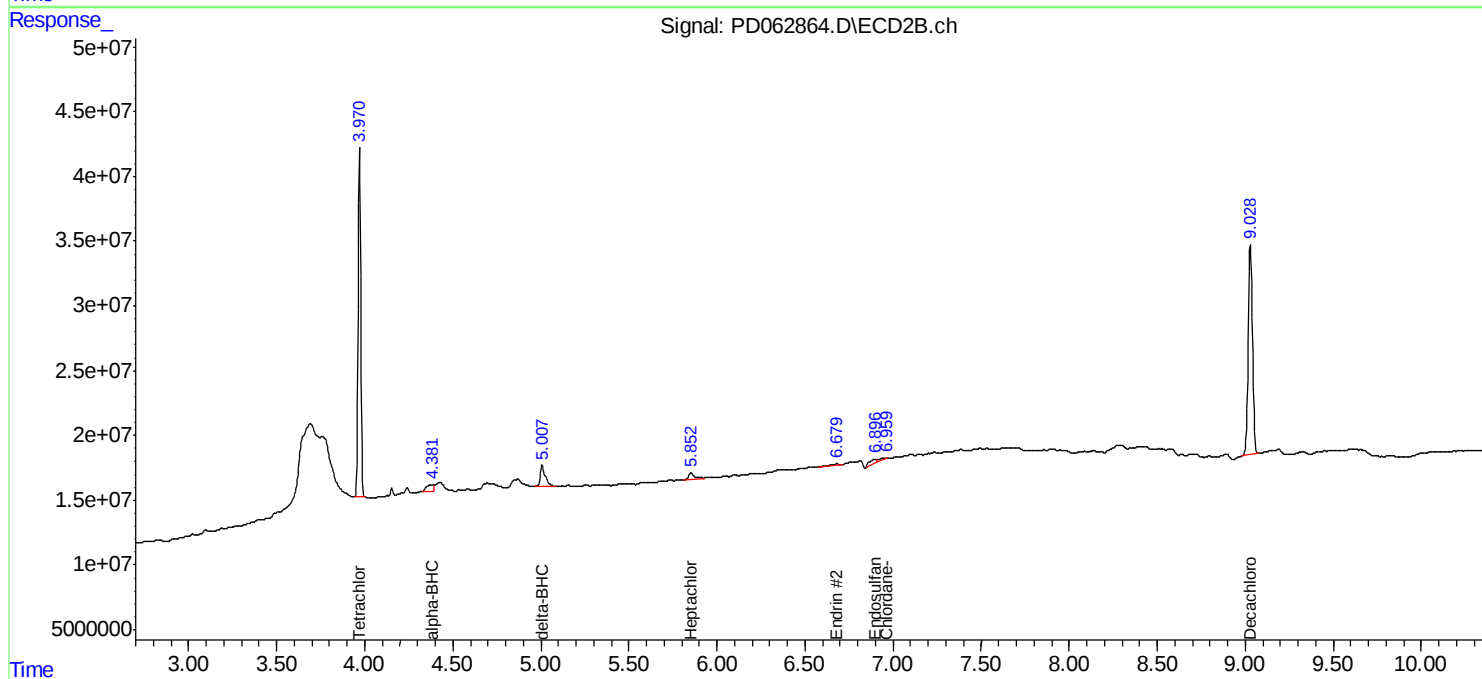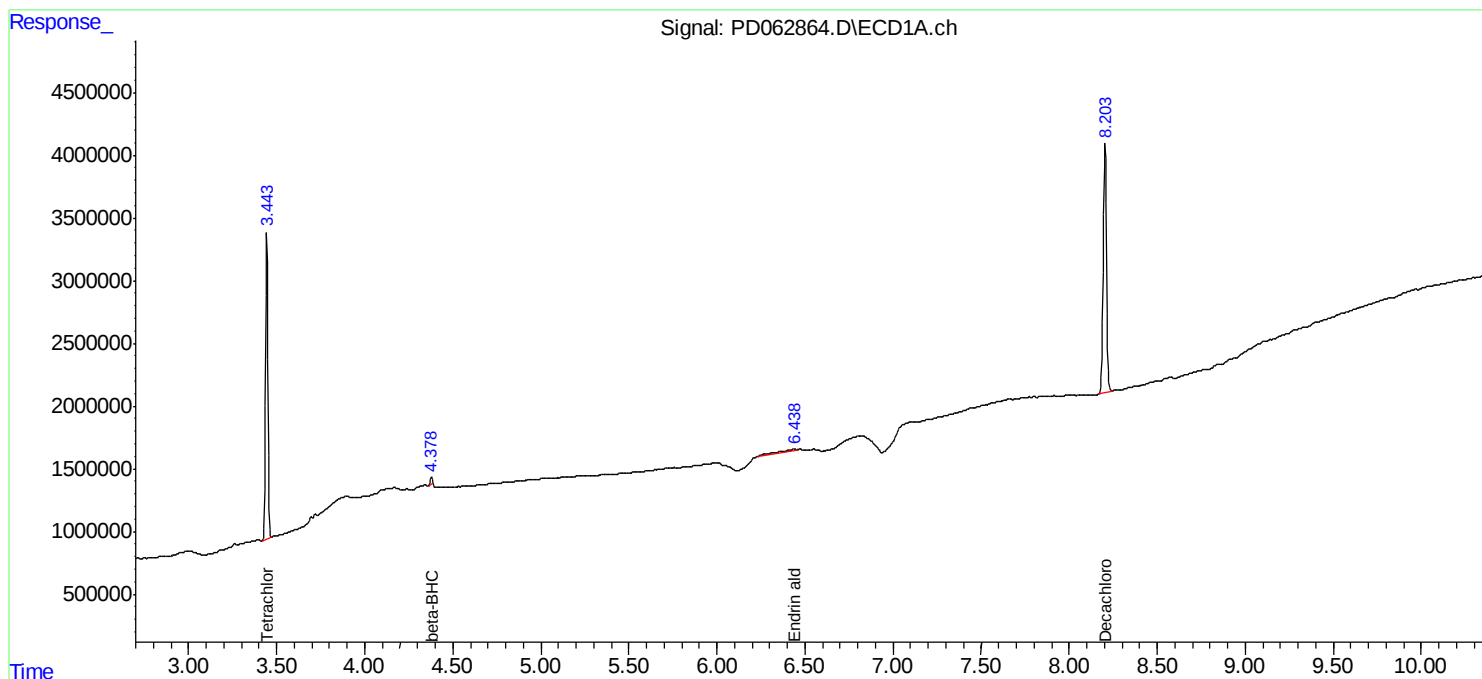


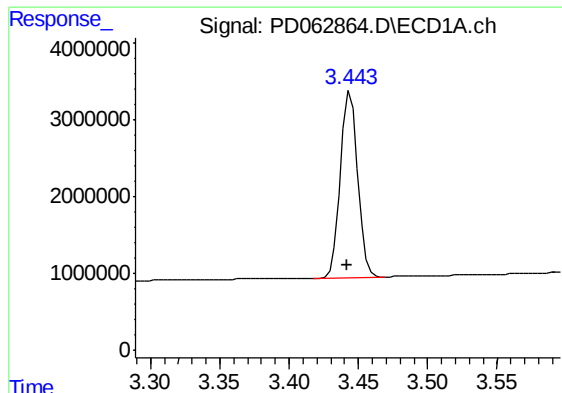

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.002 min
Response: 21195672
Conc: 23.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136254BL

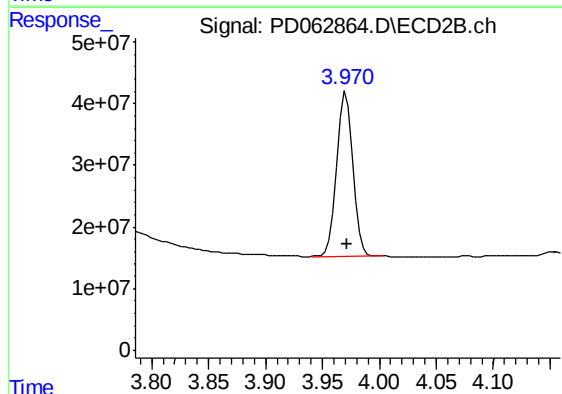


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 260695448
Conc: 22.52 ng/ml

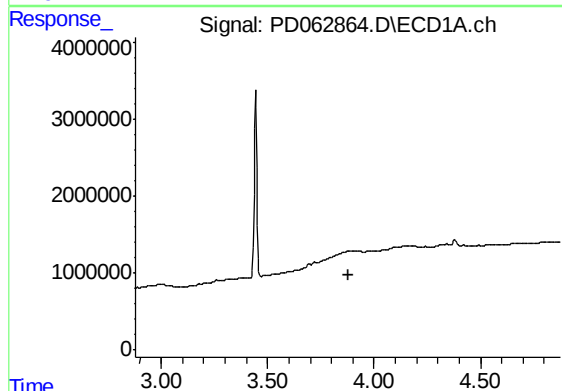


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.879 min
Response: 0
Conc: N.D.

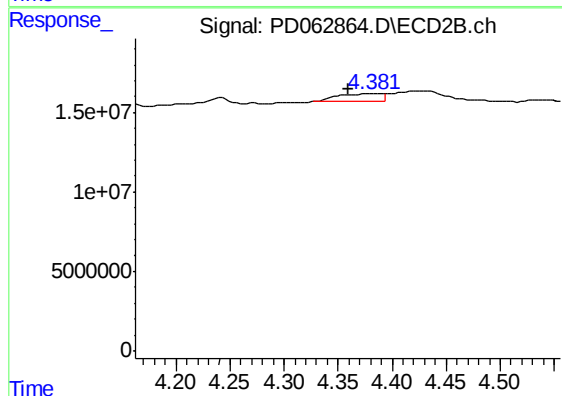

#2 alpha-BHC


R.T.: 4.383 min
Delta R.T.: 0.022 min
Response: 14167248
Conc: 0.74 ng/ml

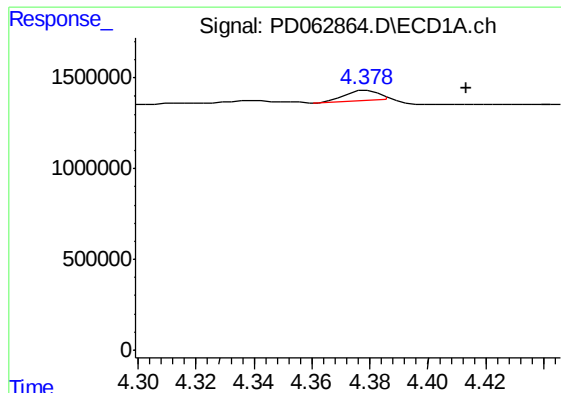

#6 beta-BHC


R.T.: 4.379 min
Delta R.T.: -0.034 min
Response: 489665
Conc: 0.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136254BL

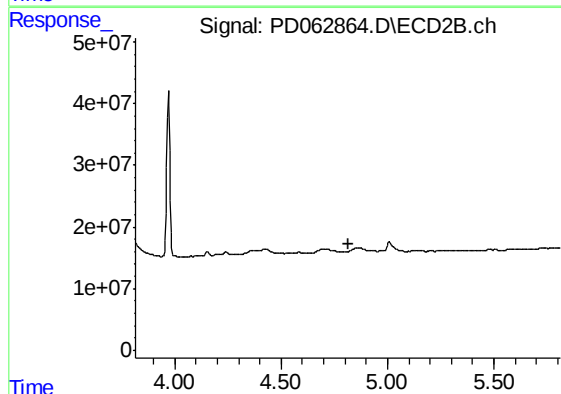


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.816 min
Response: 0
Conc: N.D.

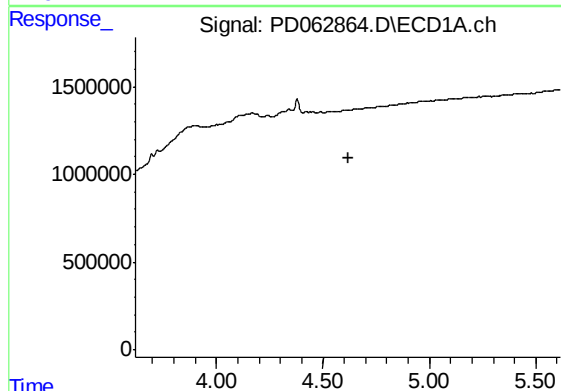


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

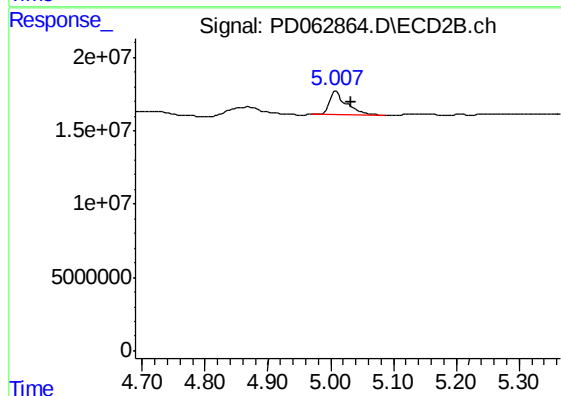

#7 delta-BHC


R.T.: 5.008 min
Delta R.T.: -0.024 min
Response: 29949144
Conc: 1.66 ng/ml

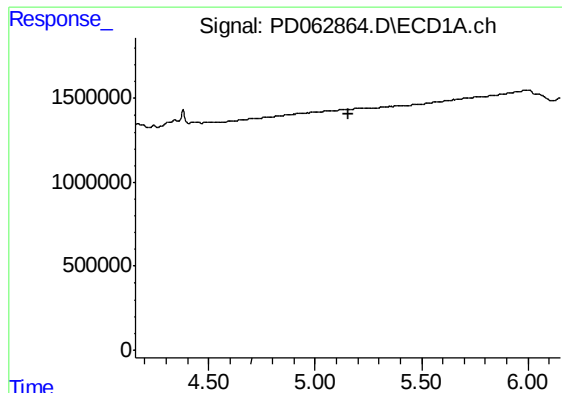

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136254BL

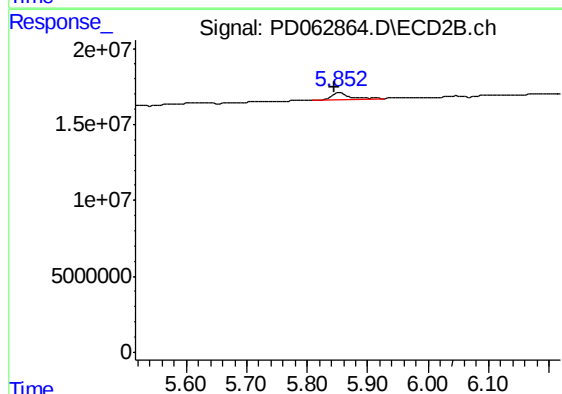


#8 Heptachlor epoxide

R.T.: 5.854 min
Delta R.T.: 0.009 min
Response: 9472936
Conc: 0.59 ng/ml

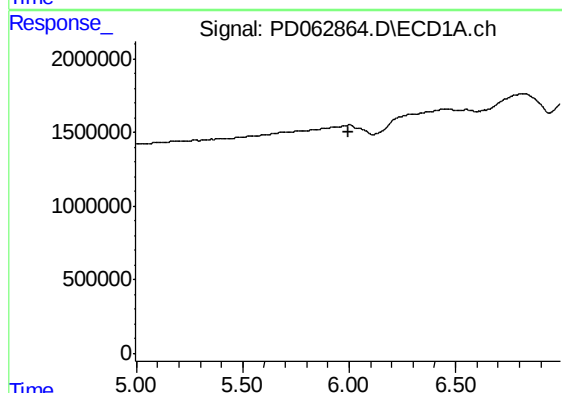


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

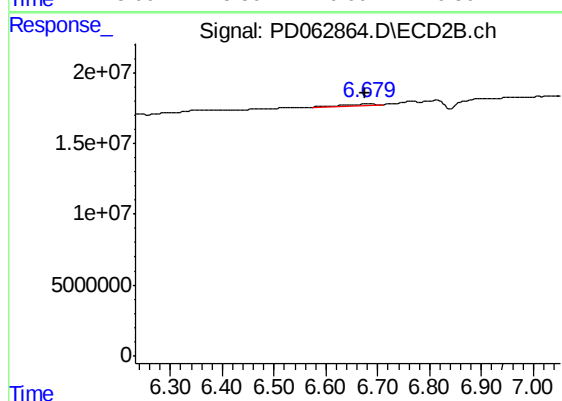

#14 Endrin


R.T.: 6.683 min
Delta R.T.: 0.007 min
Response: 5114022
Conc: 0.36 ng/ml

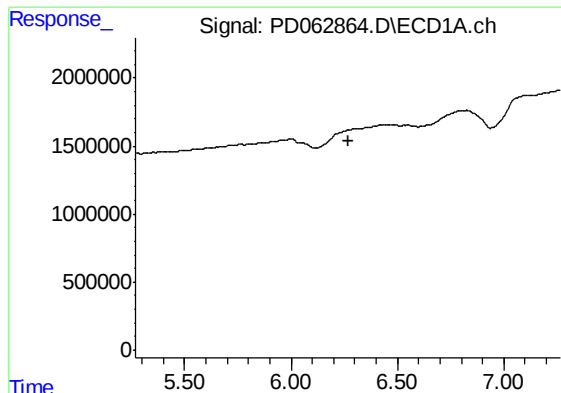

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136254BL

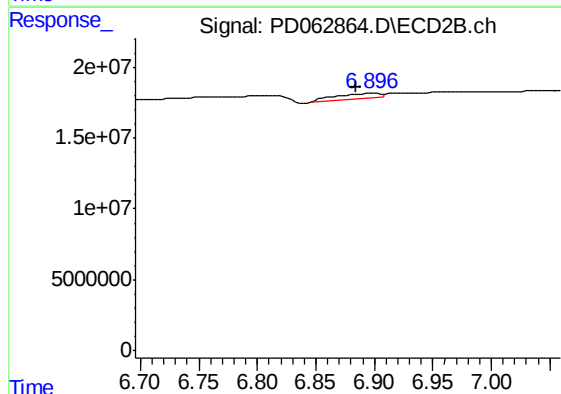


#15 Endosulfan II

R.T.: 6.898 min
Delta R.T.: 0.013 min
Response: 10180998
Conc: 0.76 ng/ml

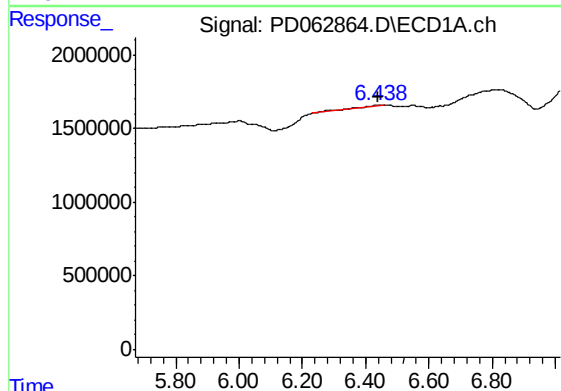


#18 Endrin aldehyde

R.T.: 6.439 min
Delta R.T.: 0.001 min
Response: 673160
Conc: 0.72 ng/ml

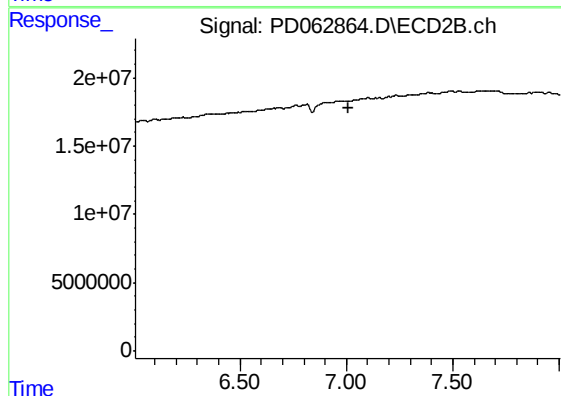

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

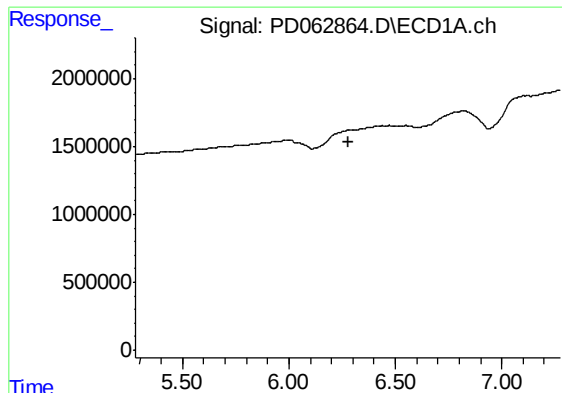

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136254BL

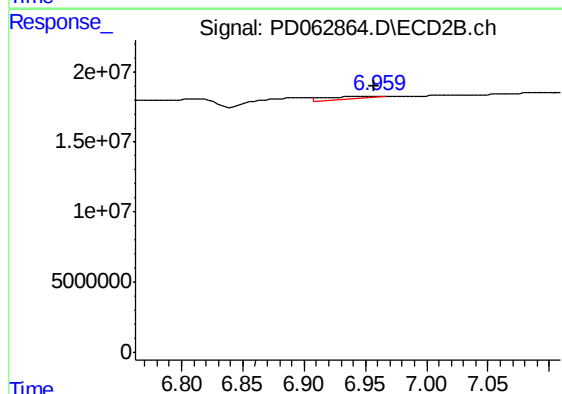


#27 Chlordane-5

R.T.: 6.961 min
Delta R.T.: 0.004 min
Response: 4786453
Conc: 9.73 ng/ml

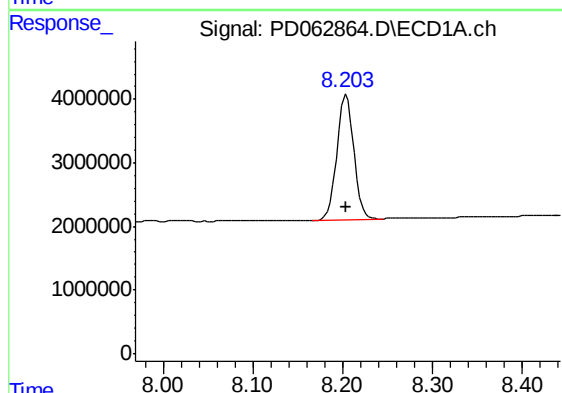

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 25862368
Conc: 24.43 ng/ml

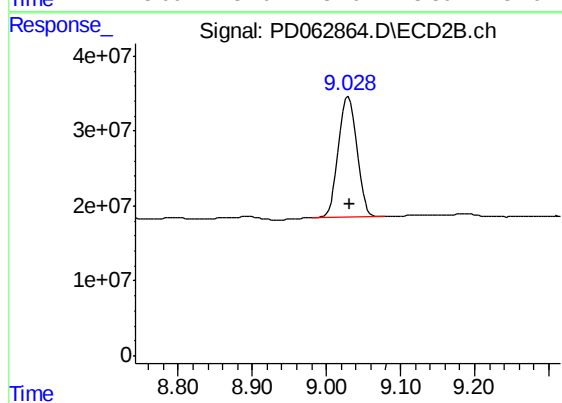

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 276991973
Conc: 24.00 ng/ml