

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
 Data File : PD062873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 13:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 03:57:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	3.971	21254804	256.8E6	23.903	22.181
28)	SA Decachlor...	8.203	9.031	25639213	276.4E6	24.217	23.952
Target Compounds							
2)	A alpha-BHC	0.000	4.361	0 12372089	N.D.	0.643	#
7)	B delta-BHC	0.000	5.007f	0 22071272	N.D.	1.223	#
8)	B Heptachlo...	0.000	5.854	0 4459159	N.D.	0.279	#
14)	MA Endrin	0.000	6.678	0 4795214	N.D.	0.341	#
15)	B Endosulfa...	0.000	6.899	0 10577705	N.D.	0.792	#
21)	B Endrin ke...	0.000	7.730f	0 1483119	N.D.	0.109	#
27)	Chlordane-5	0.000	6.935f	0 2105589	N.D.	4.281	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
Data File : PD062873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 13:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 03:57:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

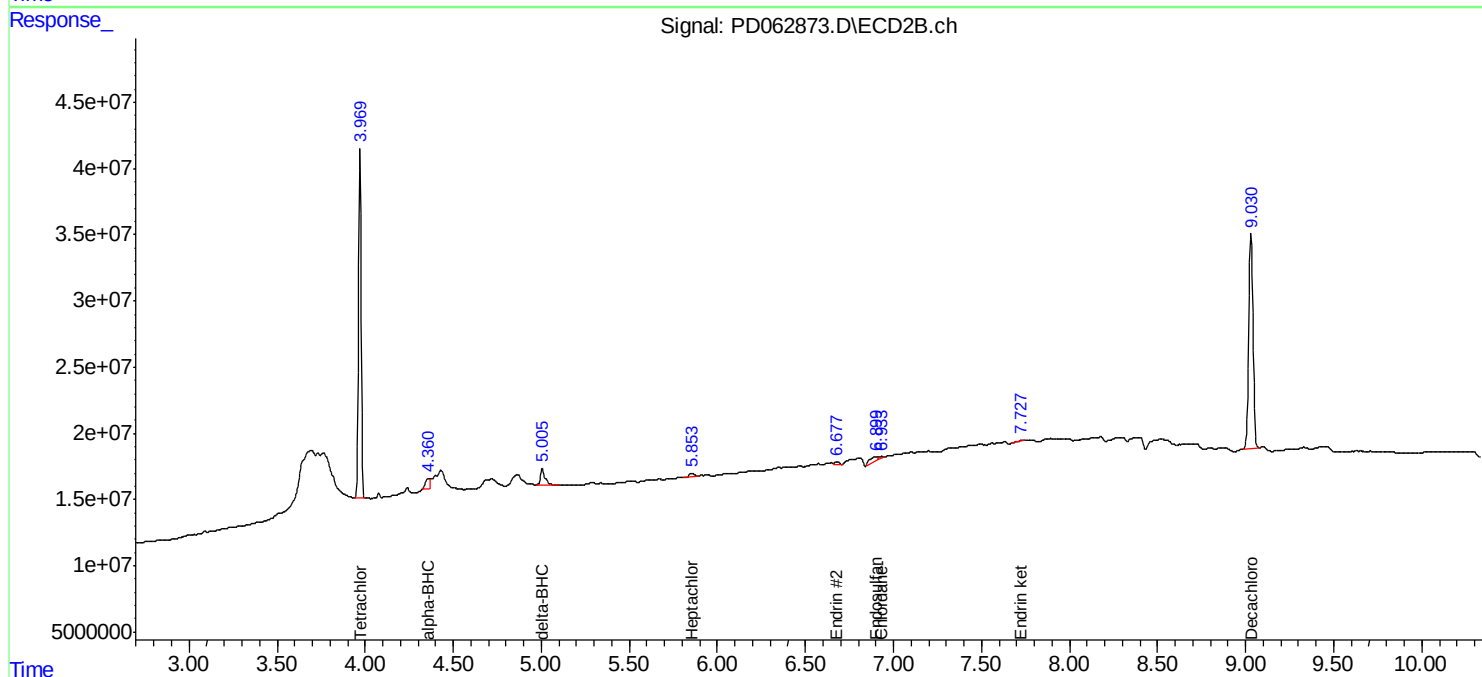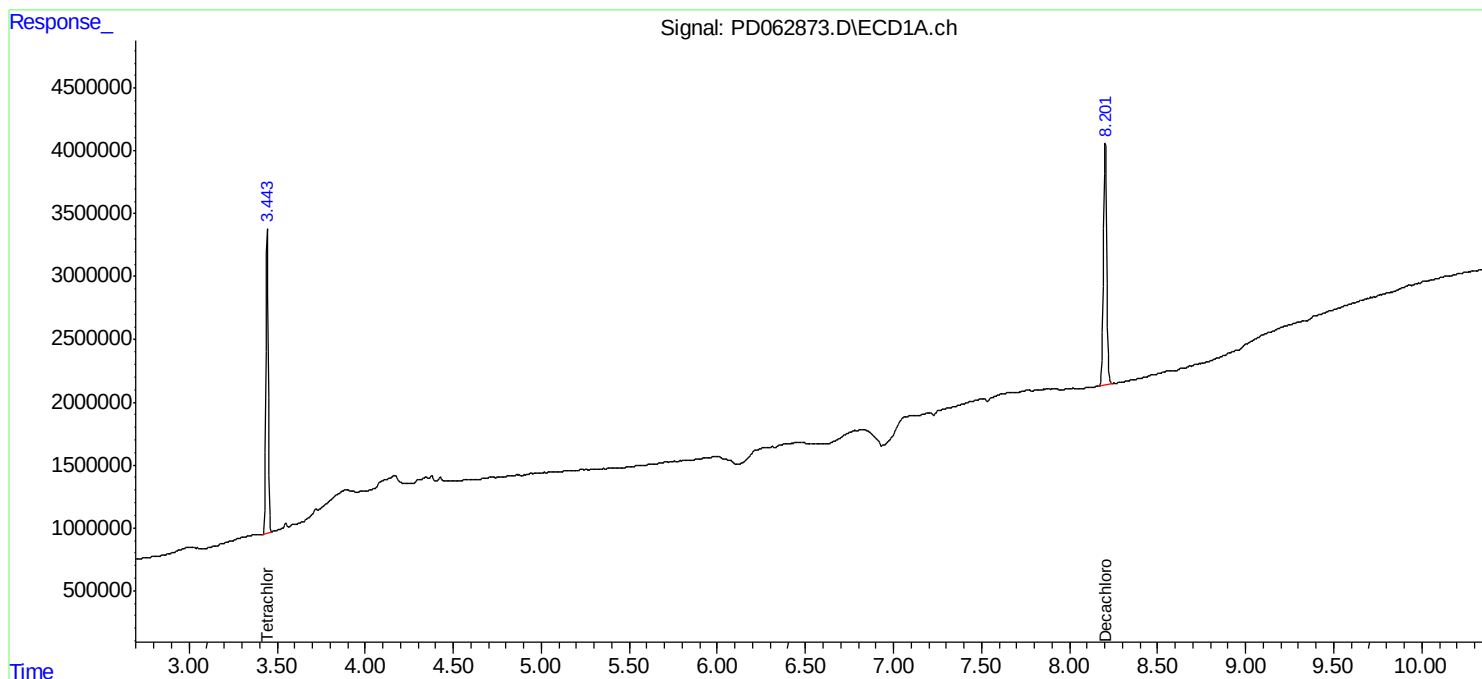


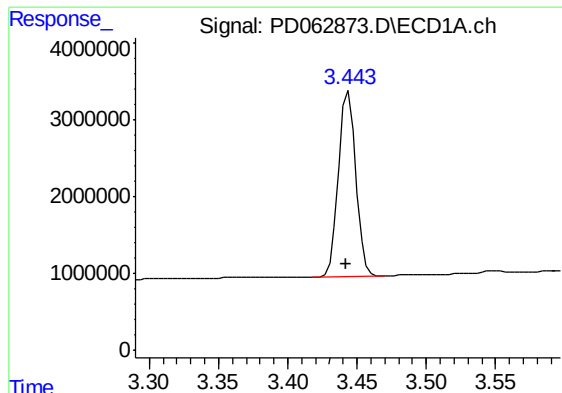

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.002 min
Response: 21254804
Conc: 23.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

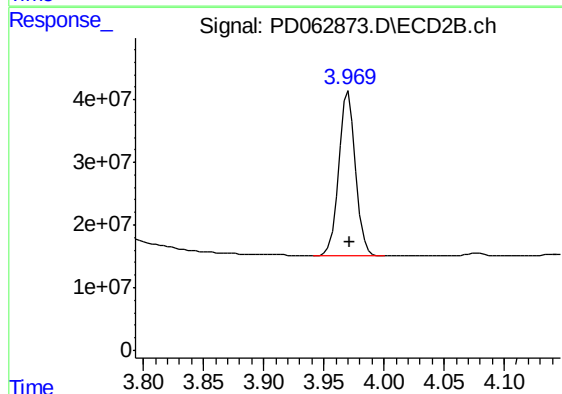


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.001 min
Response: 256789333
Conc: 22.18 ng/ml

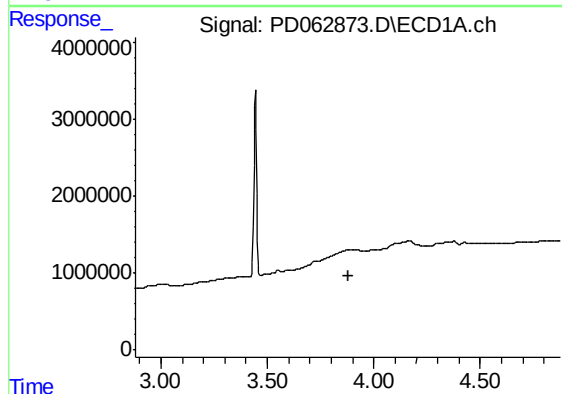


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.879 min
Response: 0
Conc: N.D.

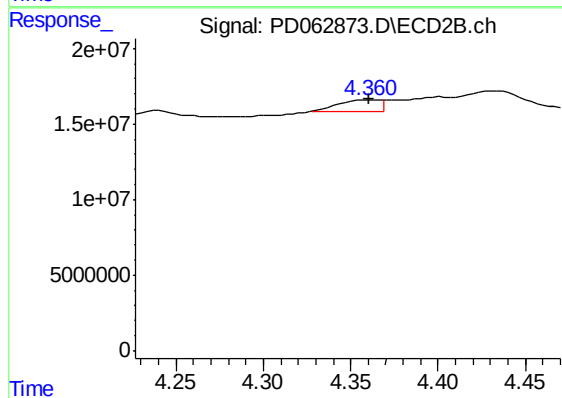

#2 alpha-BHC


R.T.: 4.361 min
Delta R.T.: 0.001 min
Response: 12372089
Conc: 0.64 ng/ml

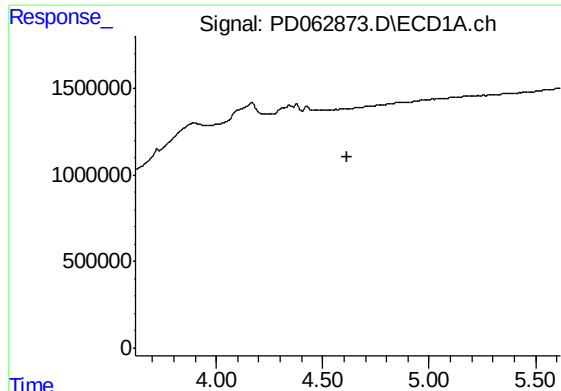

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

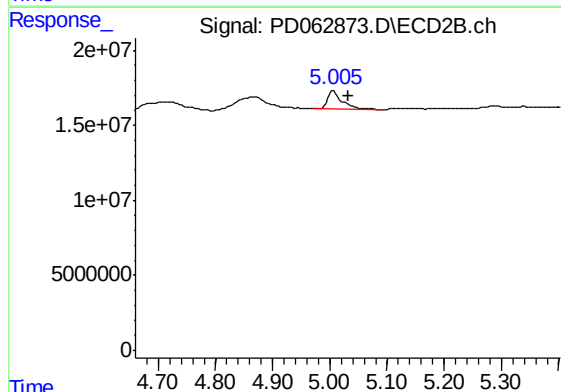


#7 delta-BHC

R.T.: 5.007 min
Delta R.T.: -0.025 min
Response: 22071272
Conc: 1.22 ng/ml

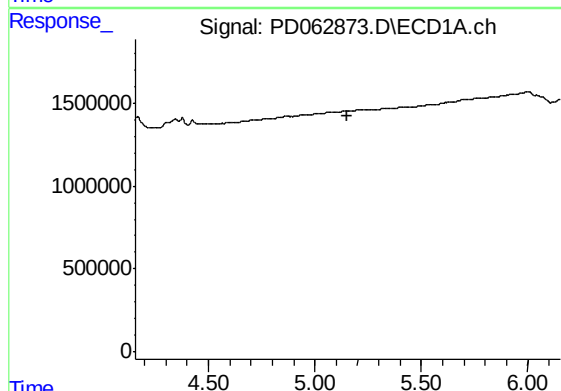


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

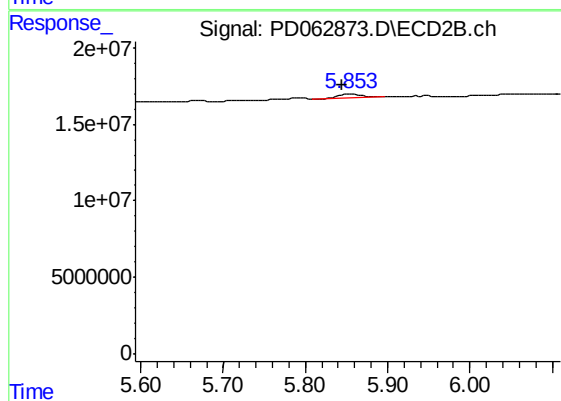

#8 Heptachlor epoxide


R.T.: 5.854 min
Delta R.T.: 0.009 min
Response: 4459159
Conc: 0.28 ng/ml

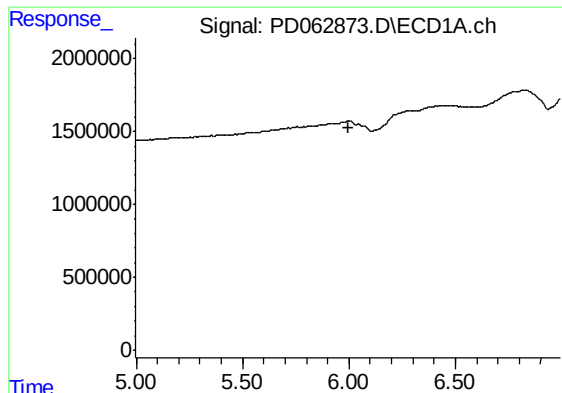

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

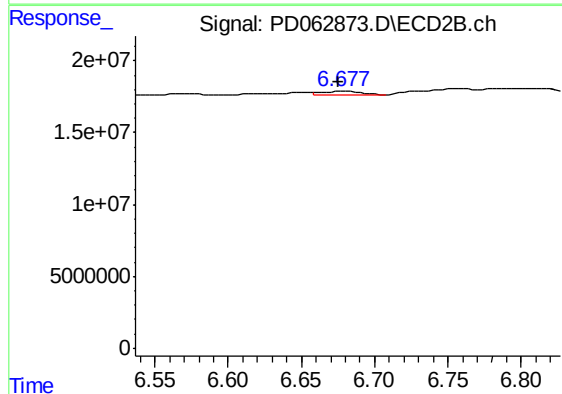


#14 Endrin

R.T.: 6.678 min
Delta R.T.: 0.003 min
Response: 4795214
Conc: 0.34 ng/ml

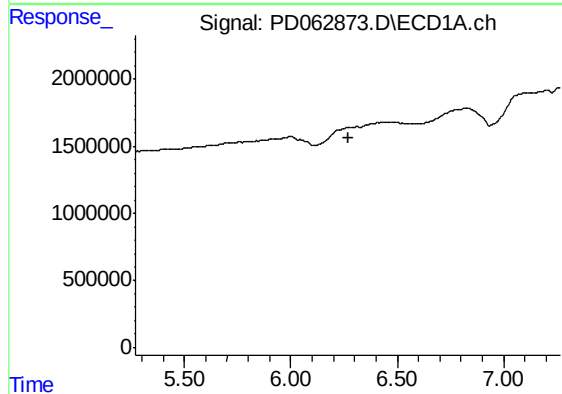


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

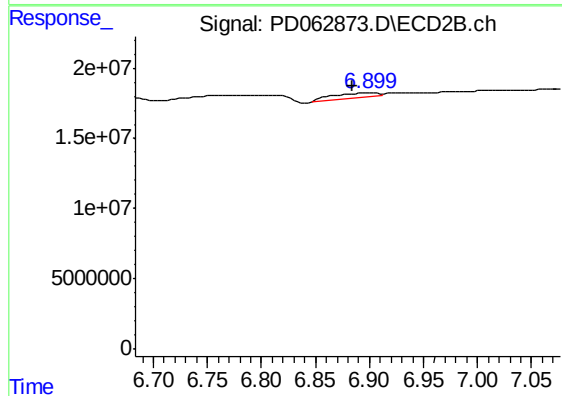

#15 Endosulfan II


R.T.: 6.899 min
Delta R.T.: 0.014 min
Response: 10577705
Conc: 0.79 ng/ml

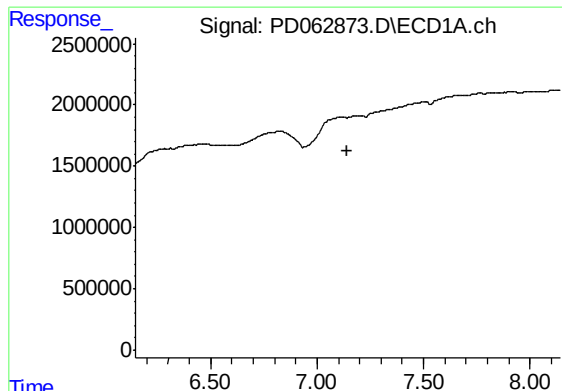

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

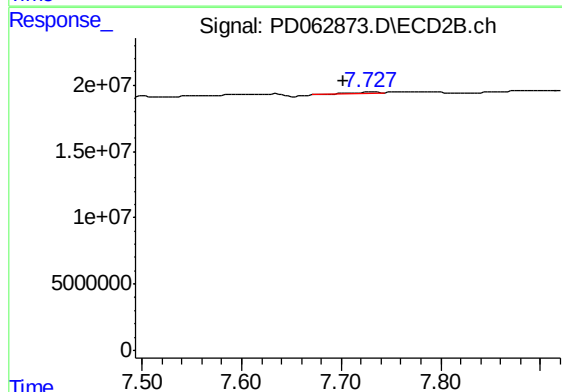


#21 Endrin ketone

R.T.: 7.730 min
Delta R.T.: 0.027 min
Response: 1483119
Conc: 0.11 ng/ml

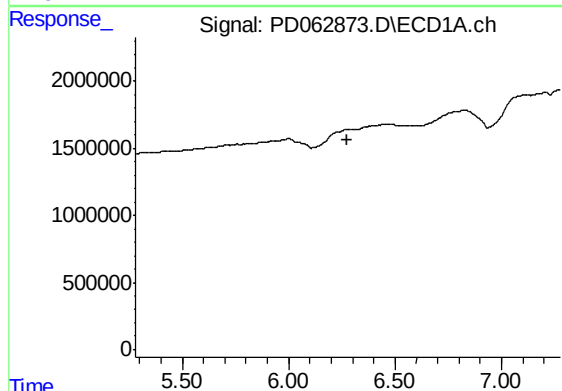


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.278 min
Response: 0
Conc: N.D.

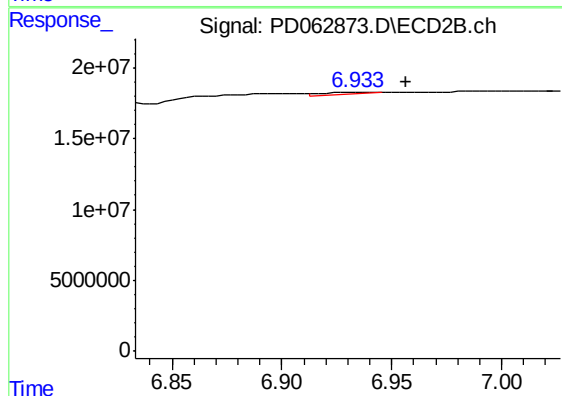

#27 Chlordane-5


R.T.: 6.935 min
Delta R.T.: -0.022 min
Response: 2105589
Conc: 4.28 ng/ml

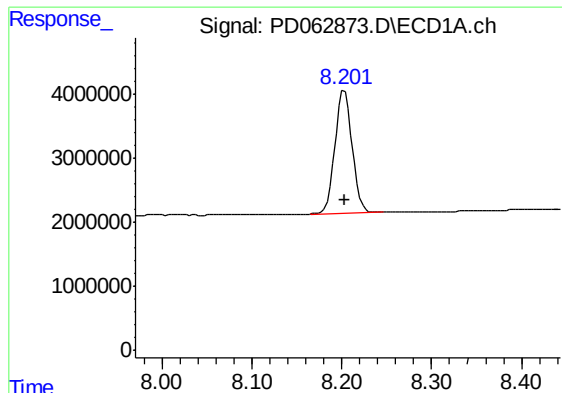

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 25639213
Conc: 24.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

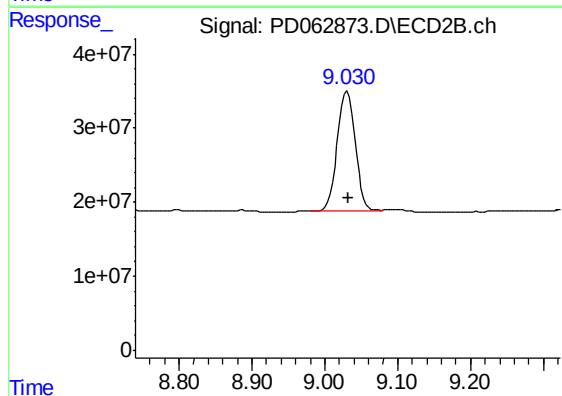

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.001 min
Response: 276376549
Conc: 23.95 ng/ml