

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
 Data File : PD062876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 15:31
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:56:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 05:54:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 11:04:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.446	3.971	51817224	562.6E6	55.379	46.354
7) SA Decachlor...	8.206	9.032	61549446	625.4E6	54.976	52.809
Target Compounds						
2) Toxaphene-1	5.703	6.547	4407448	75325781	572.552m	505.965
3) Toxaphene-2	6.188	7.054	4741199	63241944	570.098	508.025
4) Toxaphene-3	6.307	7.130	10635443	177.3E6	560.103	491.133
5) Toxaphene-4	6.554	7.217	11113443	111.8E6	568.155	499.894
6) Toxaphene-5	7.041	7.630	12274234	79297765	554.050	500.880

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
Data File : PD062876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 15:31
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 05:54:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 11:04:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

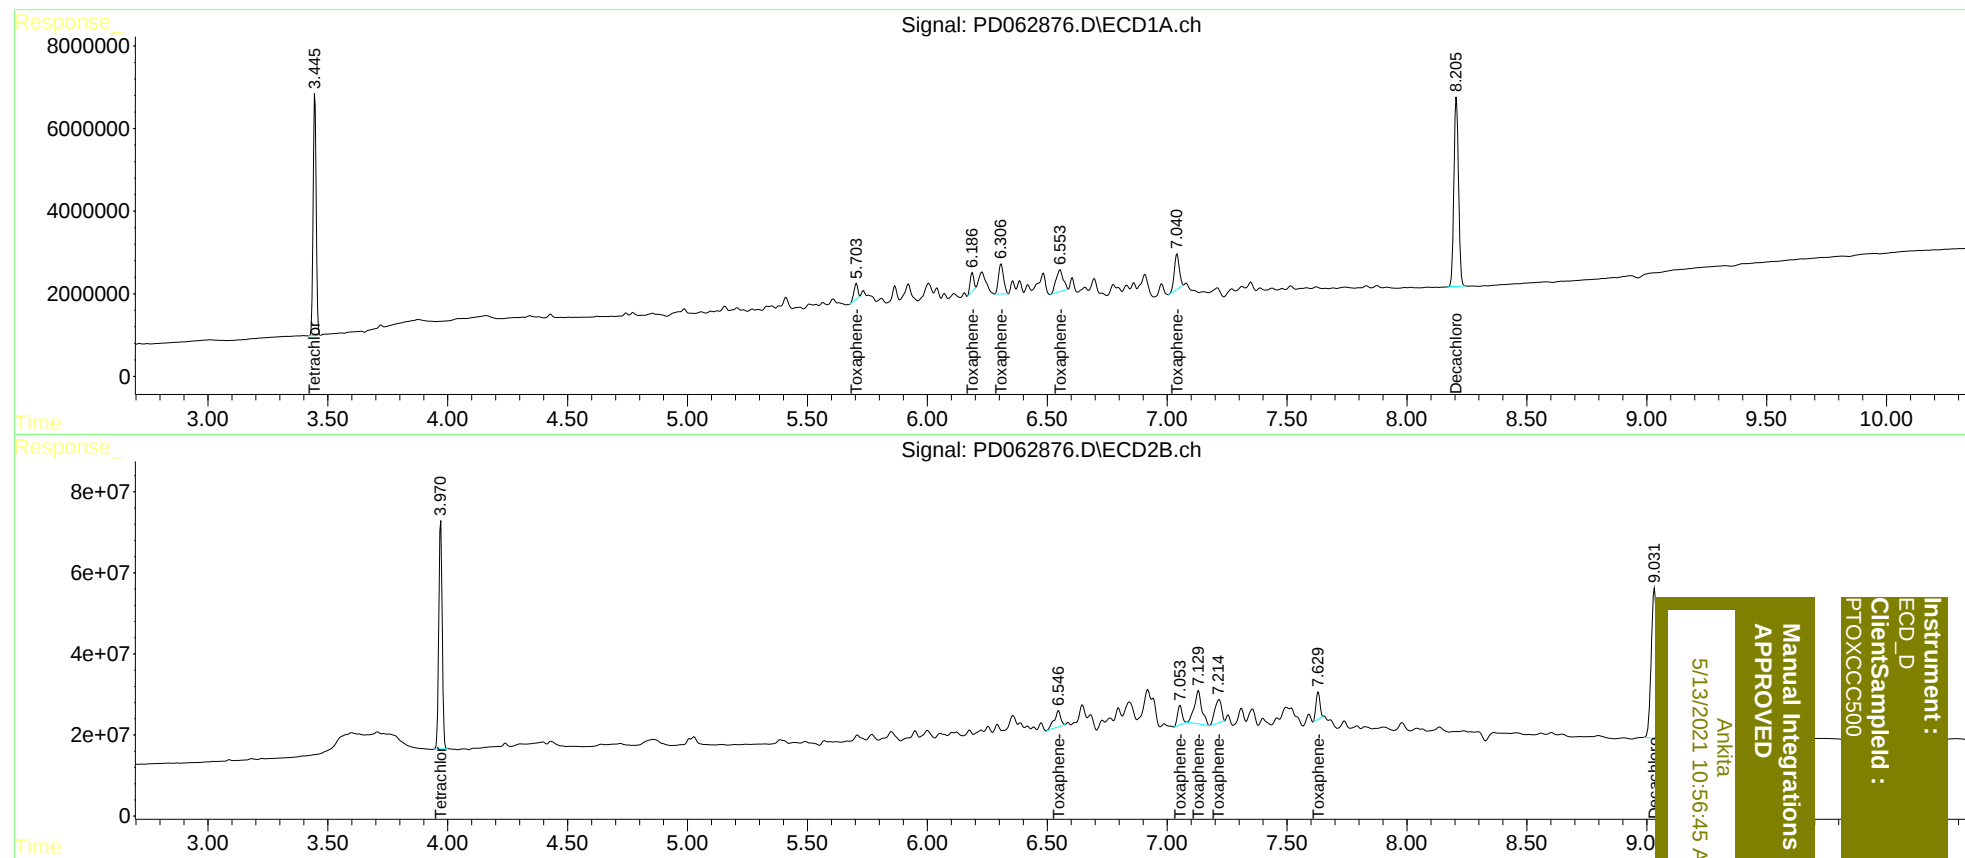

Manual Integrations
APPROVED

5/13/2021 10:56:45 AM

Ankita

Instrument :
ECD_D
Client Sampled :
PTOXCCC500