

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 08:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 12:55:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.895	18849139	26314558	21.756	22.370
28)	SA Decachlor...	7.873	8.898	19051197	24472643	21.145	21.476
Target Compounds							
3)	MA gamma-BHC...	3.934	0.000	1697226	0	1.228	N.D. #
5)	MB Aldrin	4.463f	0.000	2651954	0	2.272	N.D. #
8)	B Heptachlo...	0.000	5.742	0	5186423	N.D.	3.377 #
9)	A Endosulfan I	5.183f	0.000	142948	0	0.139	N.D. #
10)	B gamma-Chl...	5.083	0.000	1892728	0	1.691	N.D. #
11)	B alpha-Chl...	5.152	0.000	742448	0	0.666	N.D. #
13)	MA Dieldrin	5.440	0.000	2534051	0	2.302	N.D. #
14)	MA Endrin	5.710f	0.000	1994386	0	2.051	N.D. #
16)	A 4,4'-DDD	5.824	0.000	171259	0	0.201	N.D. #
25)	Chlordane-3	5.083	0.000	1892728	0	18.694	N.D. #
26)	Chlordane-4	5.152	0.000	742448	0	8.011	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 08:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 12:55:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

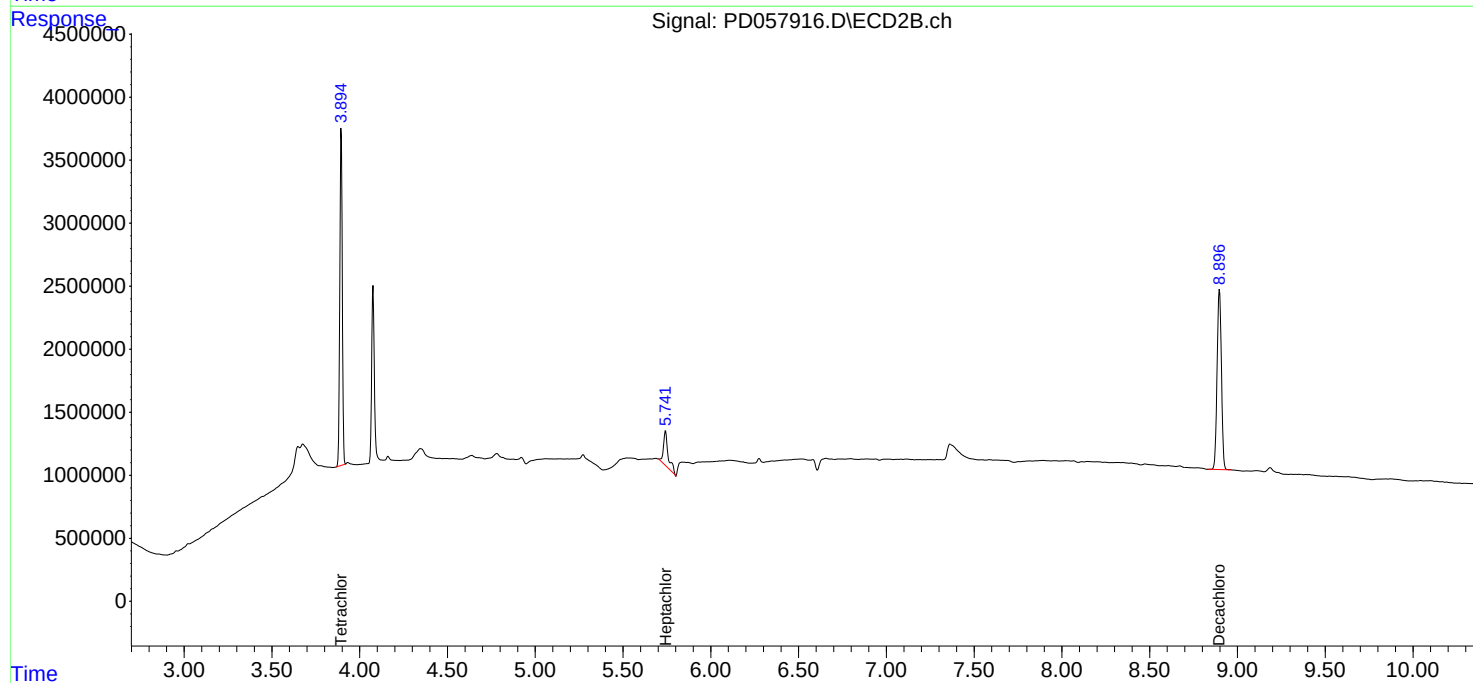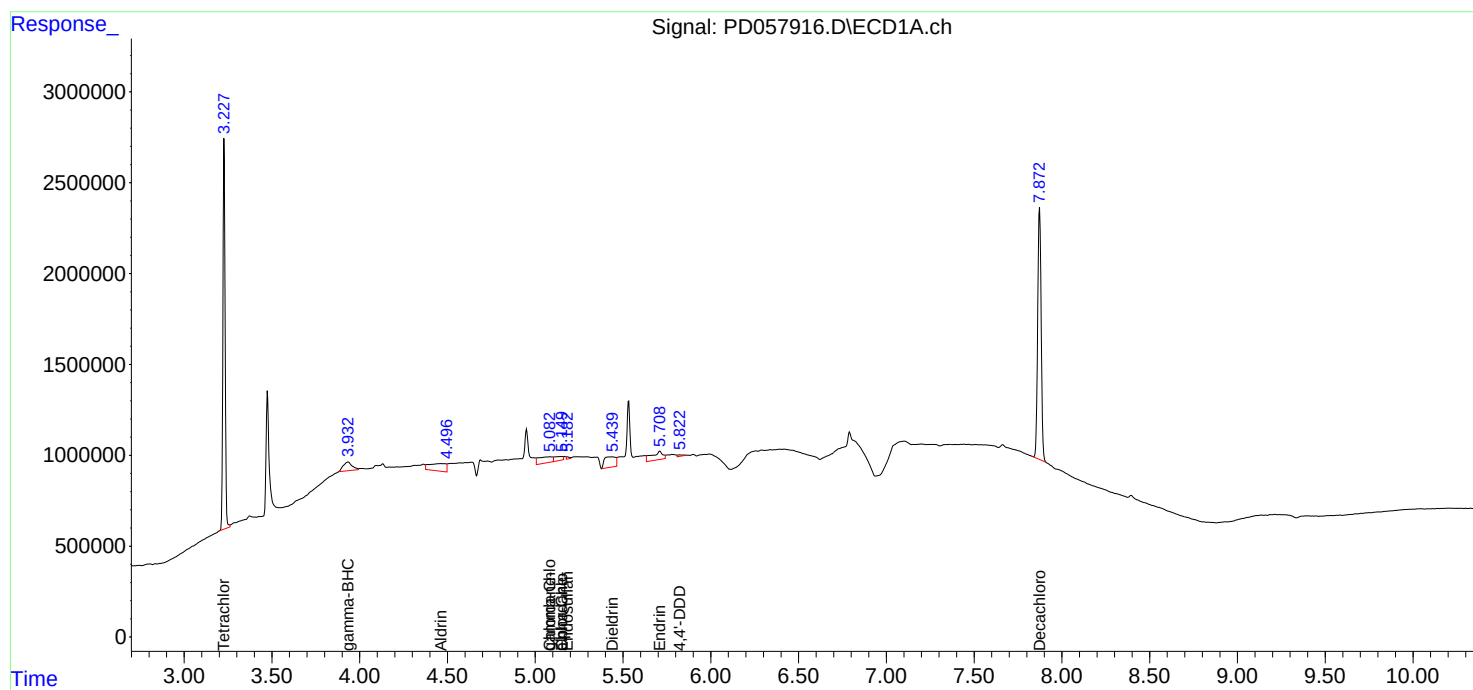


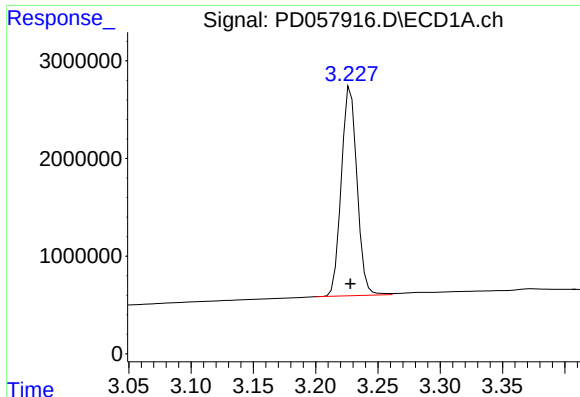

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 18849139
Conc: 21.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

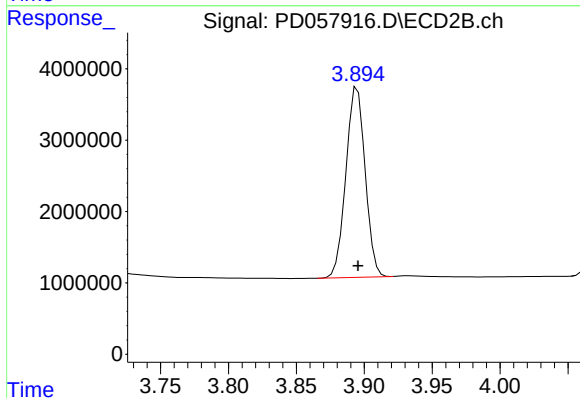


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 26314558
Conc: 22.37 ng/ml

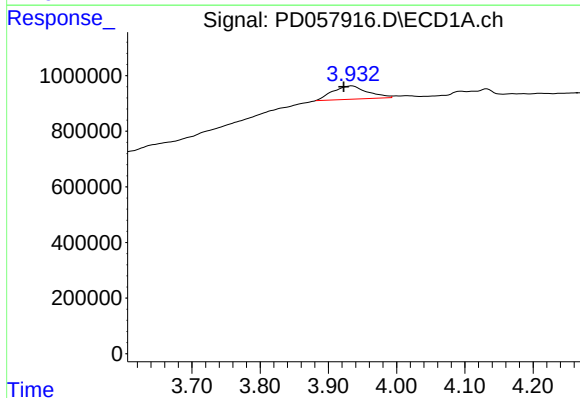


#3 gamma-BHC (Lindane)

R.T.: 3.934 min
Delta R.T.: 0.012 min
Response: 1697226
Conc: 1.23 ng/ml

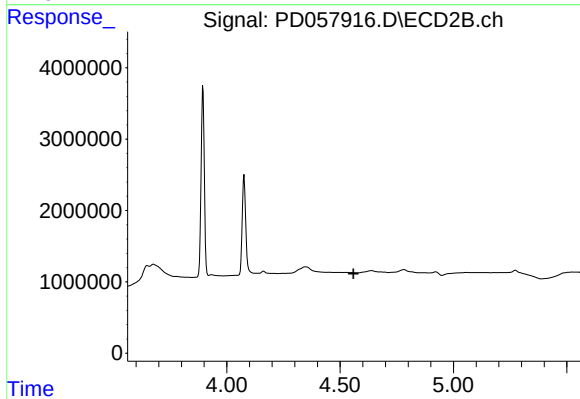

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

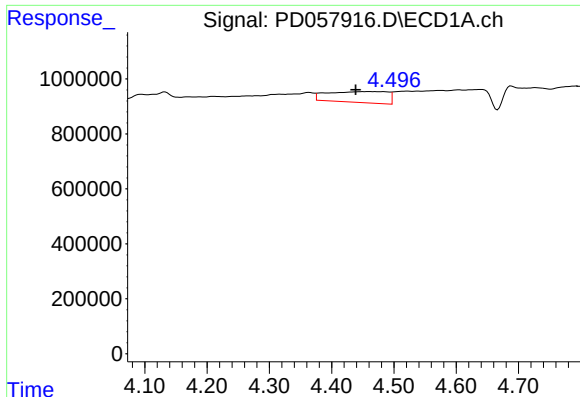

#5 Aldrin


R.T.: 4.463 min
Delta R.T.: 0.025 min
Response: 2651954
Conc: 2.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

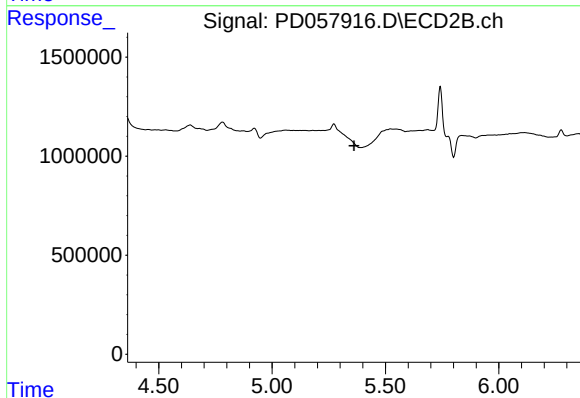


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

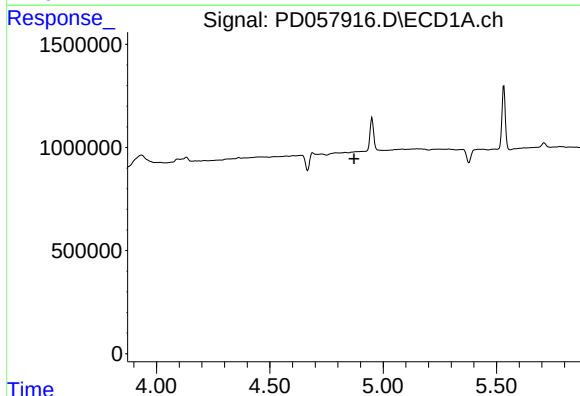


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

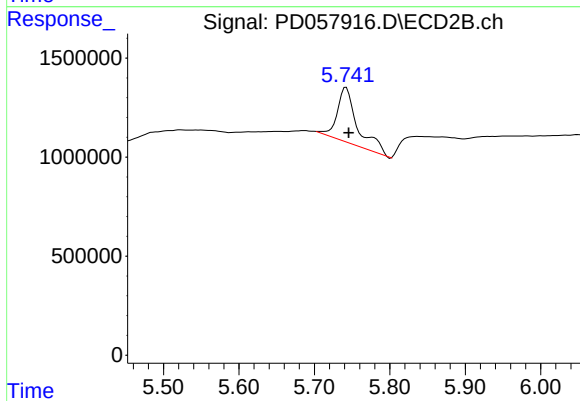

#8 Heptachlor epoxide


R.T.: 5.742 min
Delta R.T.: -0.003 min
Response: 5186423
Conc: 3.38 ng/ml

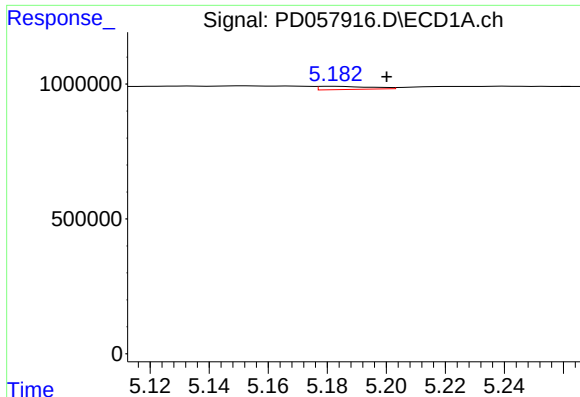

#9 Endosulfan I


R.T.: 5.183 min
Delta R.T.: -0.017 min
Response: 142948
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

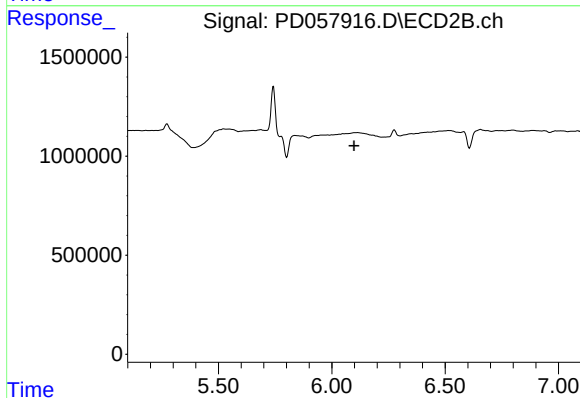


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.099 min
Response: 0
Conc: N.D.

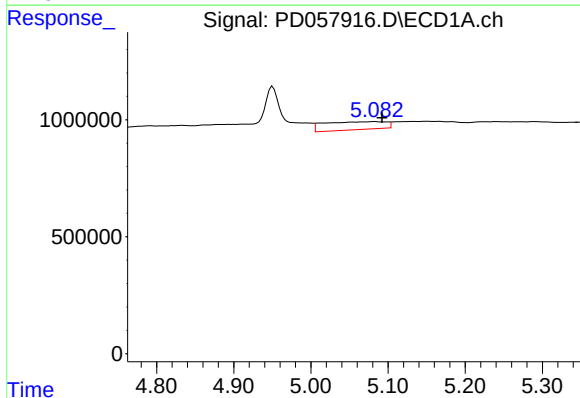


#10 gamma-Chlordane

R.T.: 5.083 min
Delta R.T.: -0.009 min
Response: 1892728
Conc: 1.69 ng/ml

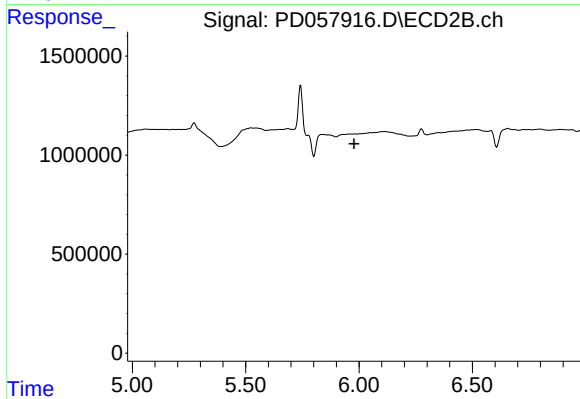

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

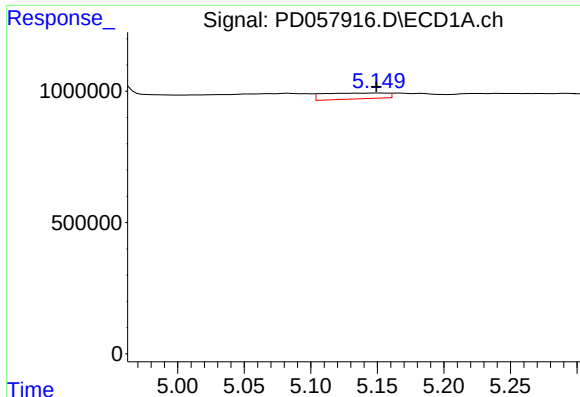

#11 alpha-Chlordane


R.T.: 5.152 min
Delta R.T.: 0.002 min
Response: 742448
Conc: 0.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

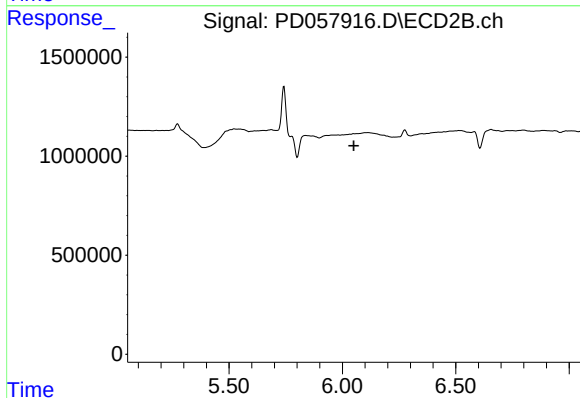


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

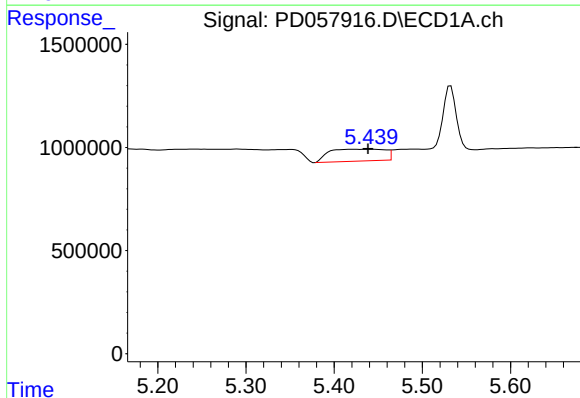


#13 Dieldrin

R.T.: 5.440 min
Delta R.T.: 0.002 min
Response: 2534051
Conc: 2.30 ng/ml

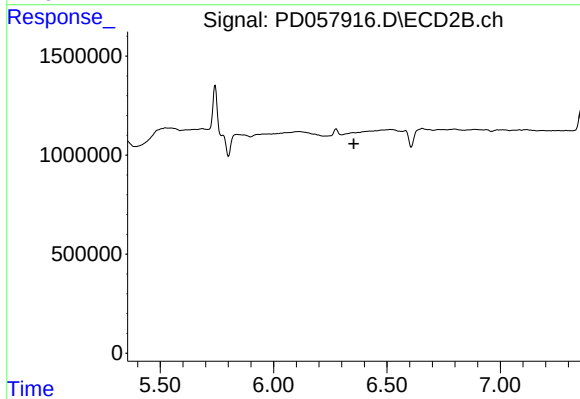

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

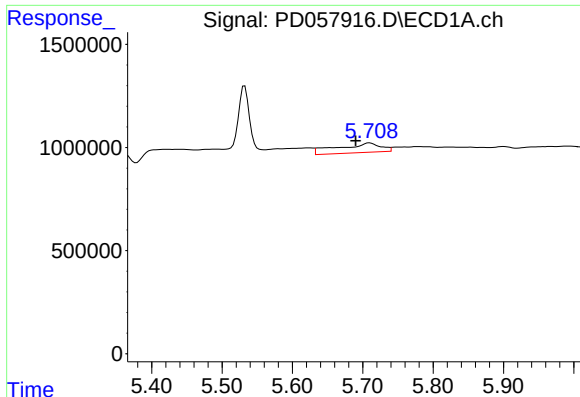

#14 Endrin


R.T.: 5.710 min
Delta R.T.: 0.020 min
Response: 1994386
Conc: 2.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

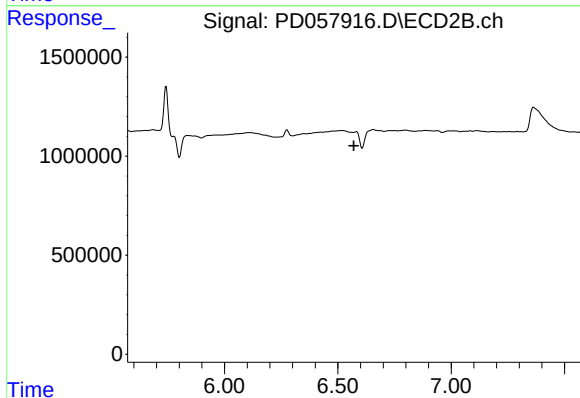


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

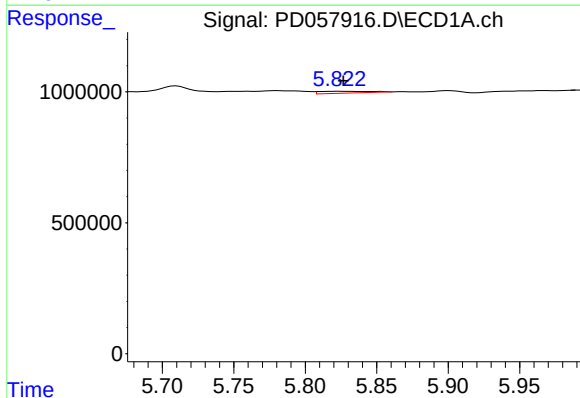


#16 4,4'-DDD

R.T.: 5.824 min
Delta R.T.: -0.003 min
Response: 171259
Conc: 0.20 ng/ml

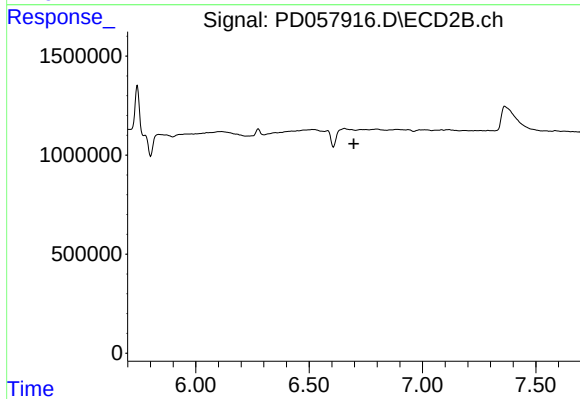

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.697 min
Response: 0
Conc: N.D.

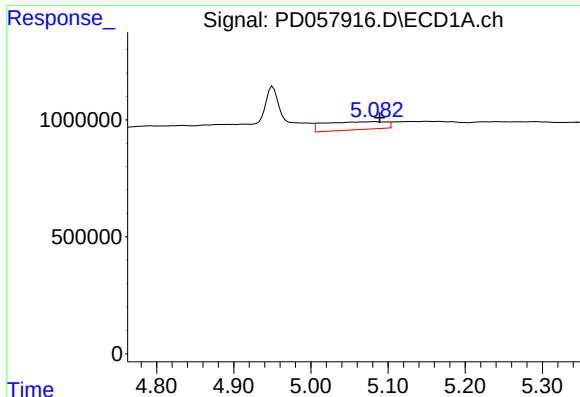

#25 Chlordane-3


R.T.: 5.083 min
Delta R.T.: -0.006 min
Response: 1892728
Conc: 18.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

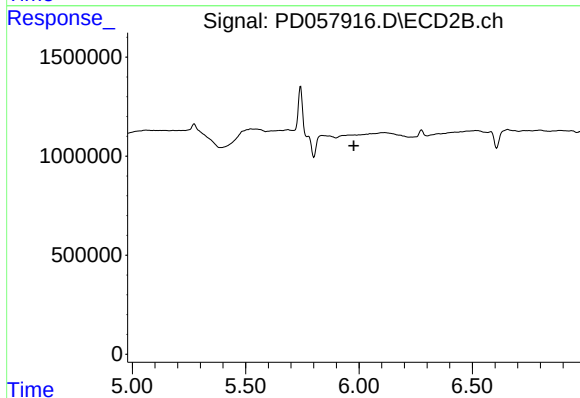


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

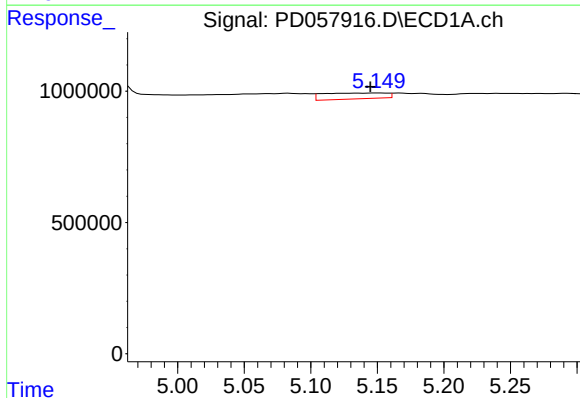


#26 Chlordane-4

R.T.: 5.152 min
Delta R.T.: 0.007 min
Response: 742448
Conc: 8.01 ng/ml

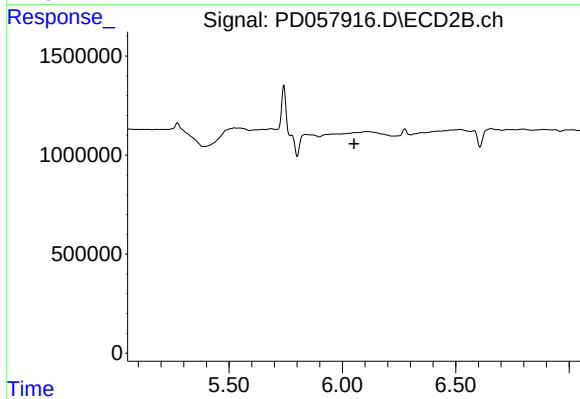

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

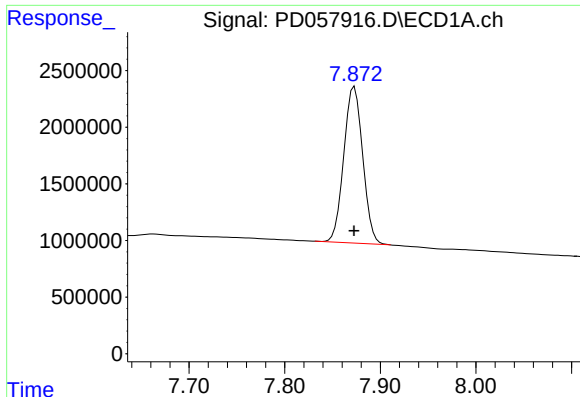

#28 Decachlorobiphenyl

R.T.: 7.873 min
Delta R.T.: 0.000 min
Response: 19051197
Conc: 21.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

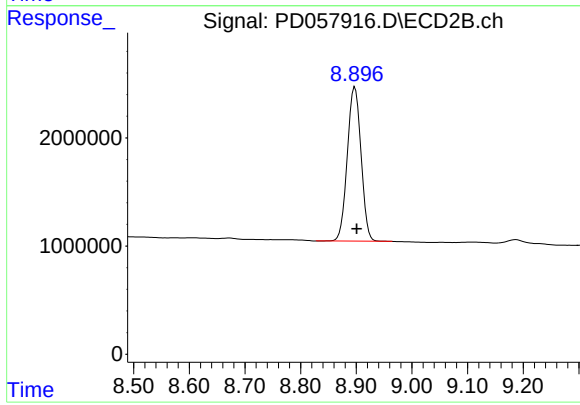

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: -0.003 min
Response: 24472643
Conc: 21.48 ng/ml