

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 11:19
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 12:56:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.894	19194663	26370297	22.155	22.417
28)	SA Decachlor...	7.873	8.898	16760306	25771054	18.602	22.616
Target Compounds							
3)	MA gamma-BHC...	3.931	0.000	1187974	0	0.860	N.D. #
5)	MB Aldrin	4.465f	0.000	2116160	0	1.813	N.D. #
7)	B delta-BHC	4.382f	0.000	1591452	0	1.252	N.D. #
8)	B Heptachlo...	0.000	5.741	0	4797255	N.D.	3.124 #
11)	B alpha-Chl...	5.167f	0.000	3952924	0	3.545	N.D. #
13)	MA Dieldrin	5.446	0.000	1084253	0	0.985	N.D. #
14)	MA Endrin	5.709f	0.000	4251764	0	4.372	N.D. #
16)	A 4,4'-DDD	5.824	0.000	191139	0	0.225	N.D. #
26)	Chlordane-4	5.167f	0.000	3952924	0	42.654	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 11:19
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 12:56:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

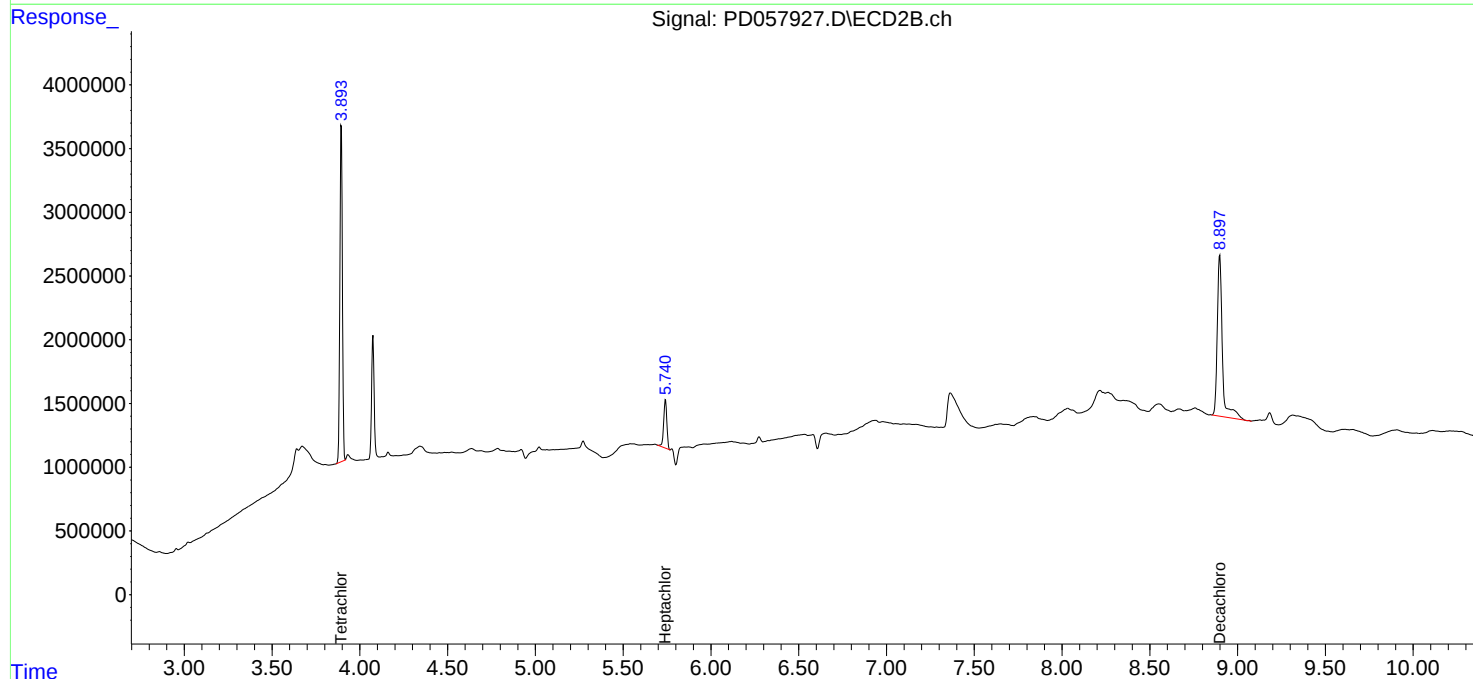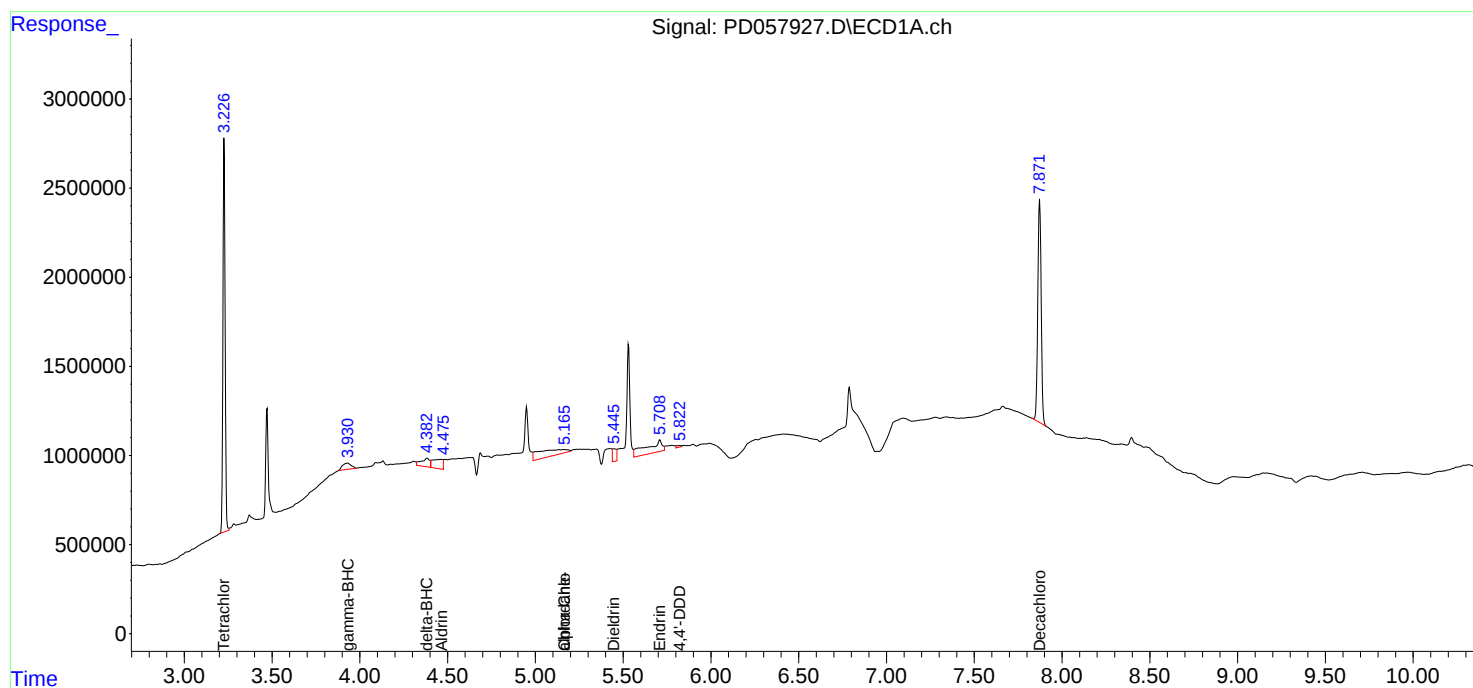


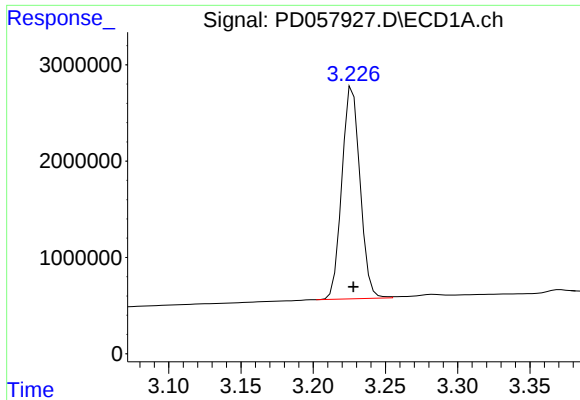

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 19194663
Conc: 22.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

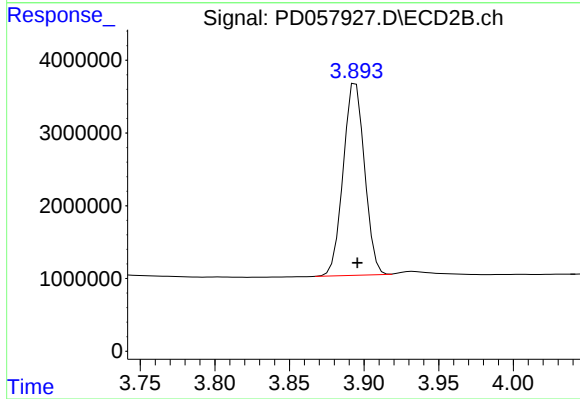


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.001 min
Response: 26370297
Conc: 22.42 ng/ml

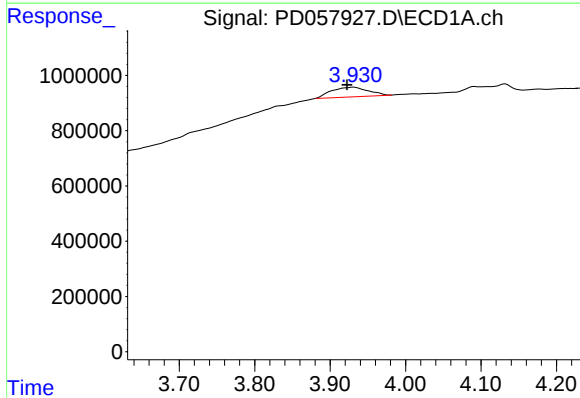


#3 gamma-BHC (Lindane)

R.T.: 3.931 min
Delta R.T.: 0.009 min
Response: 1187974
Conc: 0.86 ng/ml

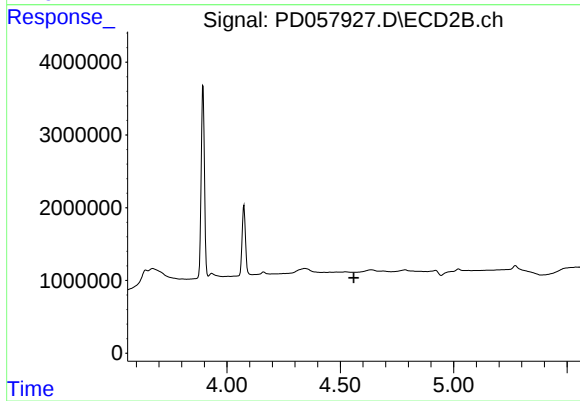

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

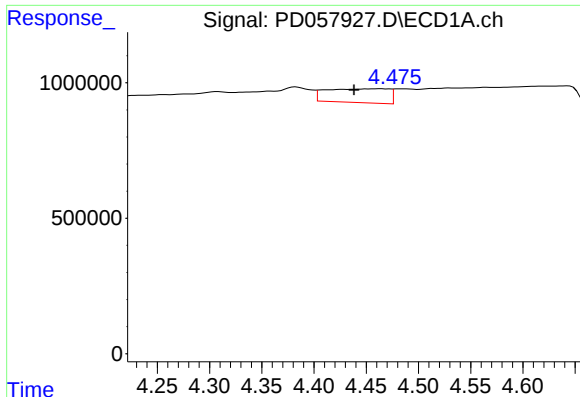

#5 Aldrin


R.T.: 4.465 min
Delta R.T.: 0.026 min
Response: 2116160
Conc: 1.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

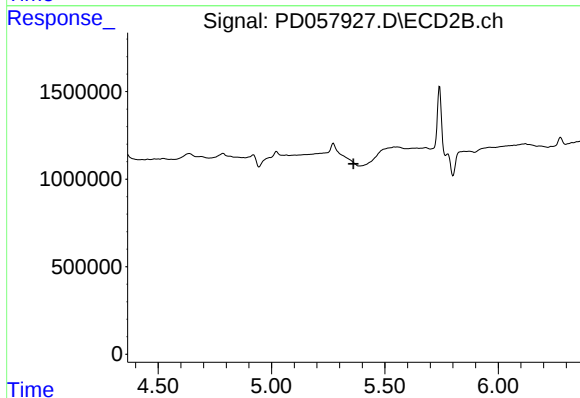


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

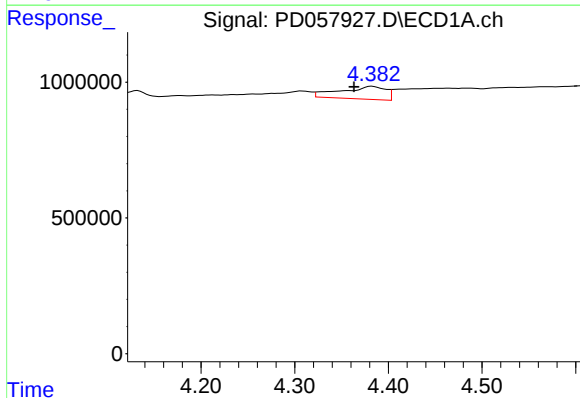


#7 delta-BHC

R.T.: 4.382 min
Delta R.T.: 0.019 min
Response: 1591452
Conc: 1.25 ng/ml

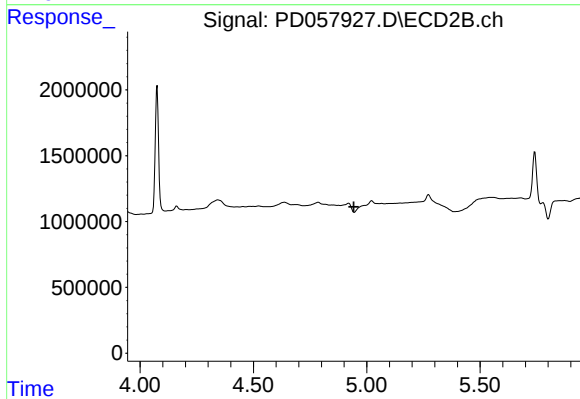

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

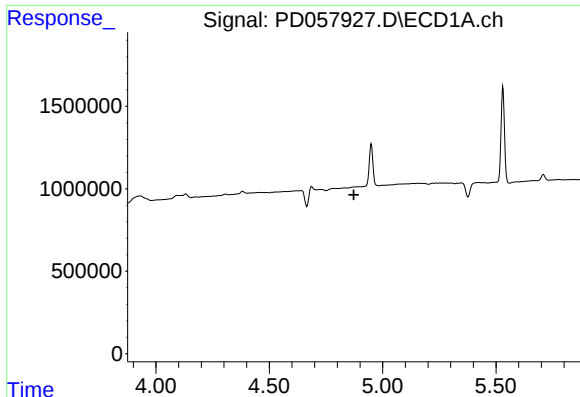

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

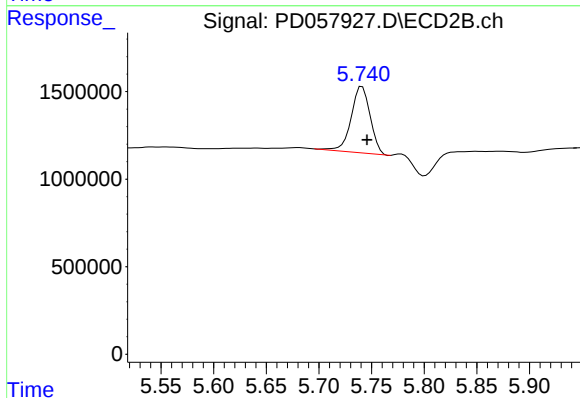


#8 Heptachlor epoxide

R.T.: 5.741 min
Delta R.T.: -0.005 min
Response: 4797255
Conc: 3.12 ng/ml

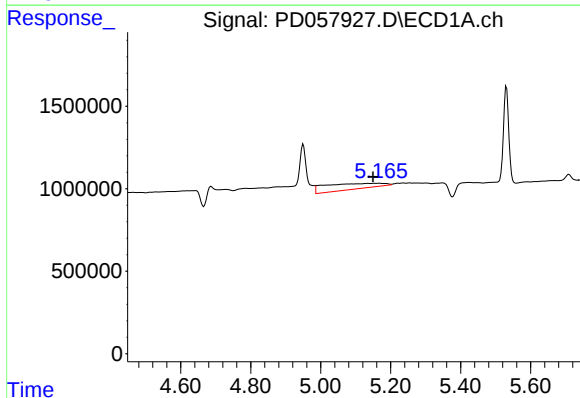


#11 alpha-Chlordane

R.T.: 5.167 min
Delta R.T.: 0.018 min
Response: 3952924
Conc: 3.54 ng/ml

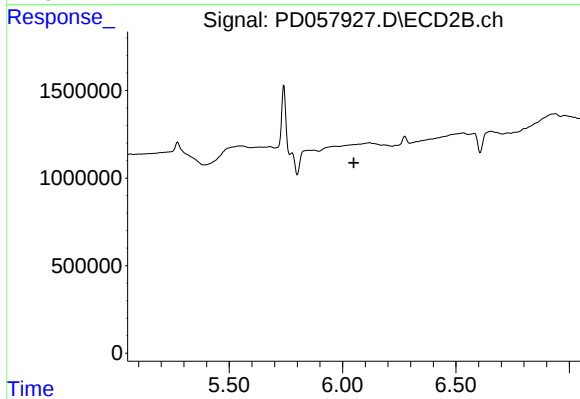

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

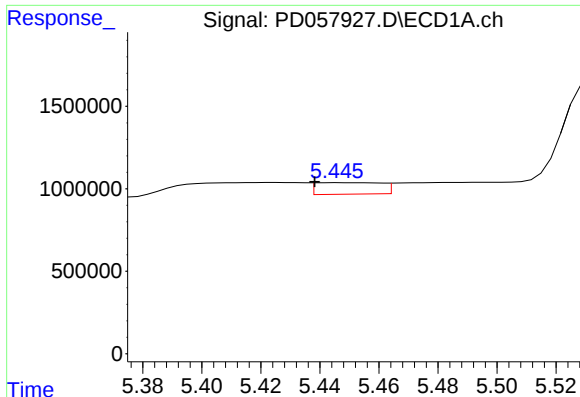

#13 Dieldrin


R.T.: 5.446 min
Delta R.T.: 0.008 min
Response: 1084253
Conc: 0.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

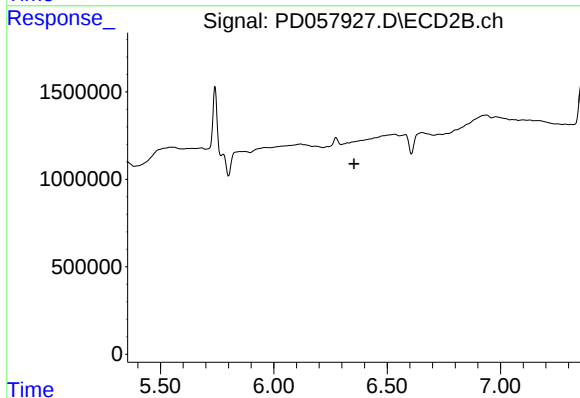


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

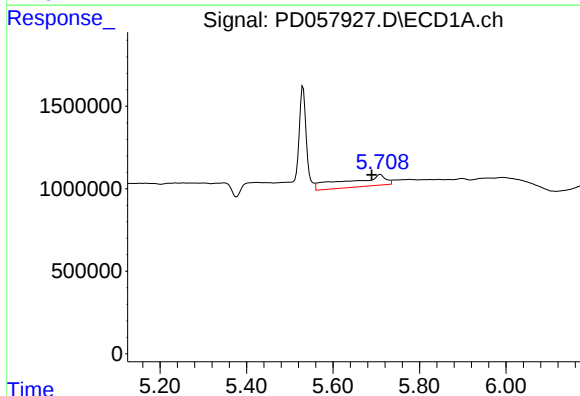


#14 Endrin

R.T.: 5.709 min
Delta R.T.: 0.019 min
Response: 4251764
Conc: 4.37 ng/ml

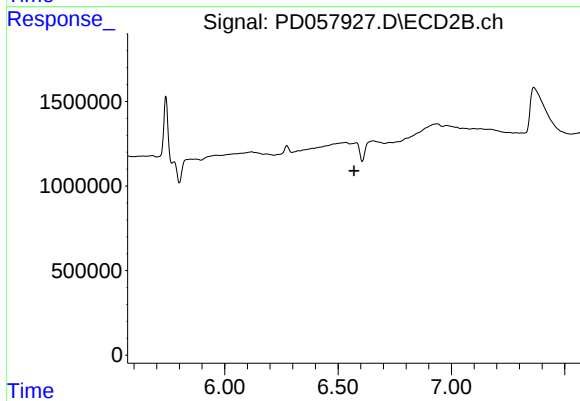

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

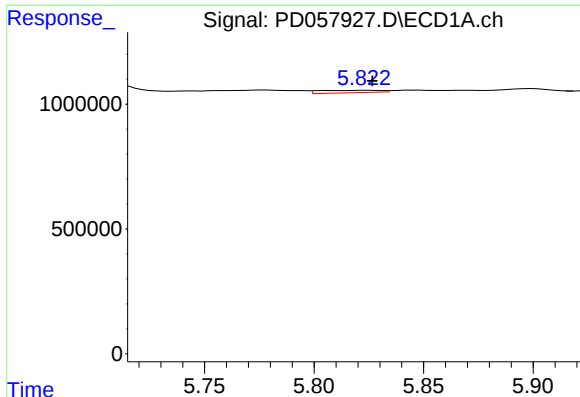

#16 4,4'-DDD


R.T.: 5.824 min
Delta R.T.: -0.003 min
Response: 191139
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

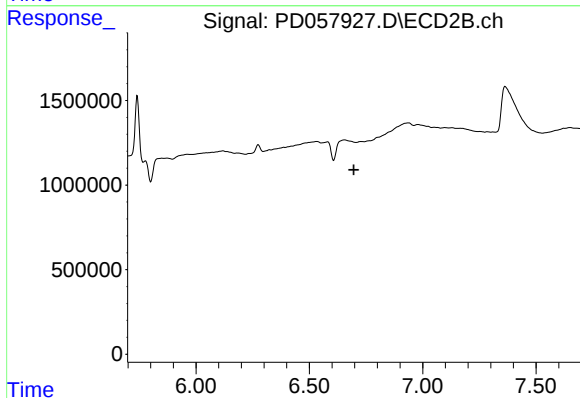


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.697 min
Response: 0
Conc: N.D.

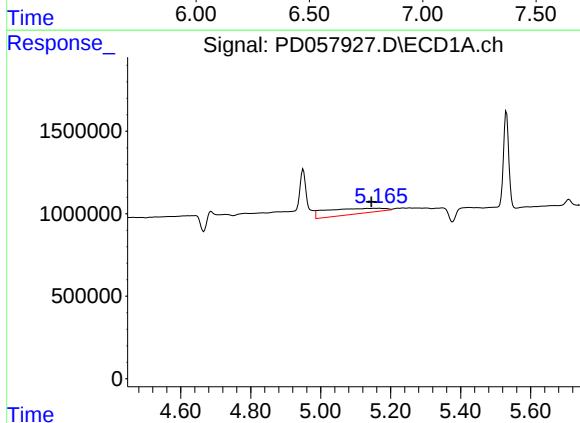


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.023 min
Response: 3952924
Conc: 42.65 ng/ml

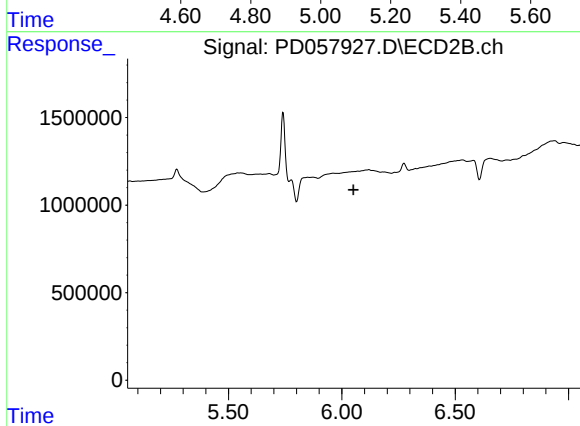

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

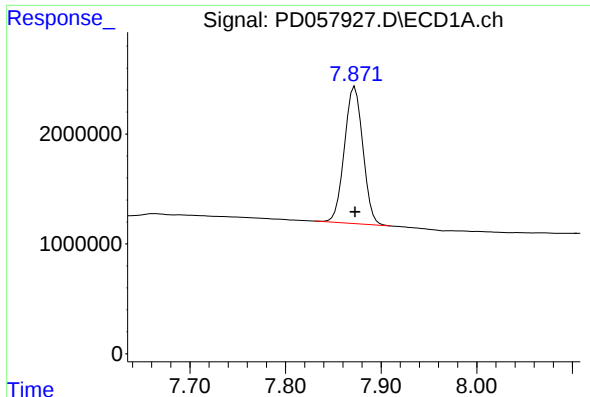

#28 Decachlorobiphenyl


R.T.: 7.873 min

Delta R.T.: 0.000 min

Response: 16760306

Conc: 18.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

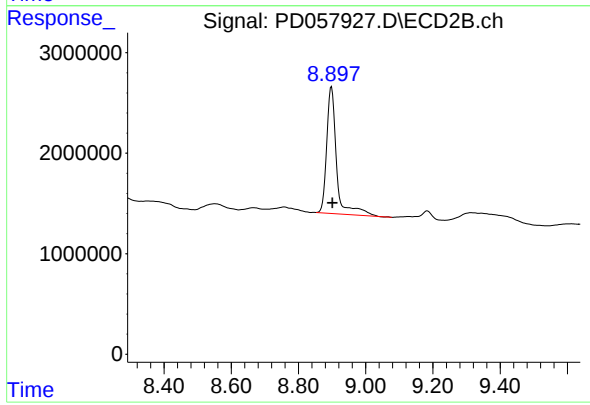

#28 Decachlorobiphenyl

R.T.: 8.898 min

Delta R.T.: -0.003 min

Response: 25771054

Conc: 22.62 ng/ml