

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 17:47
 Operator : AJ\MA
 Sample : L2505-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:08:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.896	17730933	24435501	20.465	20.772
28)	SA Decachlor...	7.873	8.899	12154622	15746559	13.490	13.819
Target Compounds							
3)	MA gamma-BHC...	3.929	0.000	2741639	0	1.984	N.D. #
4)	MA Heptachlor	4.178f	0.000	226427	0	0.201	N.D. #
6)	B beta-BHC	4.178	0.000	226427	0	0.435	N.D. #
10)	B gamma-Chl...	0.000	5.965	0	6929293	N.D.	4.516 #
13)	MA Dieldrin	5.427	0.000	412817	0	0.375	N.D. #
23)	Chlordane-1	4.073f	0.000	131913	0	4.681	N.D. #
24)	Chlordane-2	4.565f	0.000	782553	0	23.166	N.D. #
25)	Chlordane-3	0.000	5.965	0	6929293	N.D.	36.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 17:47
Operator : AJ\MA
Sample : L2505-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:08:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

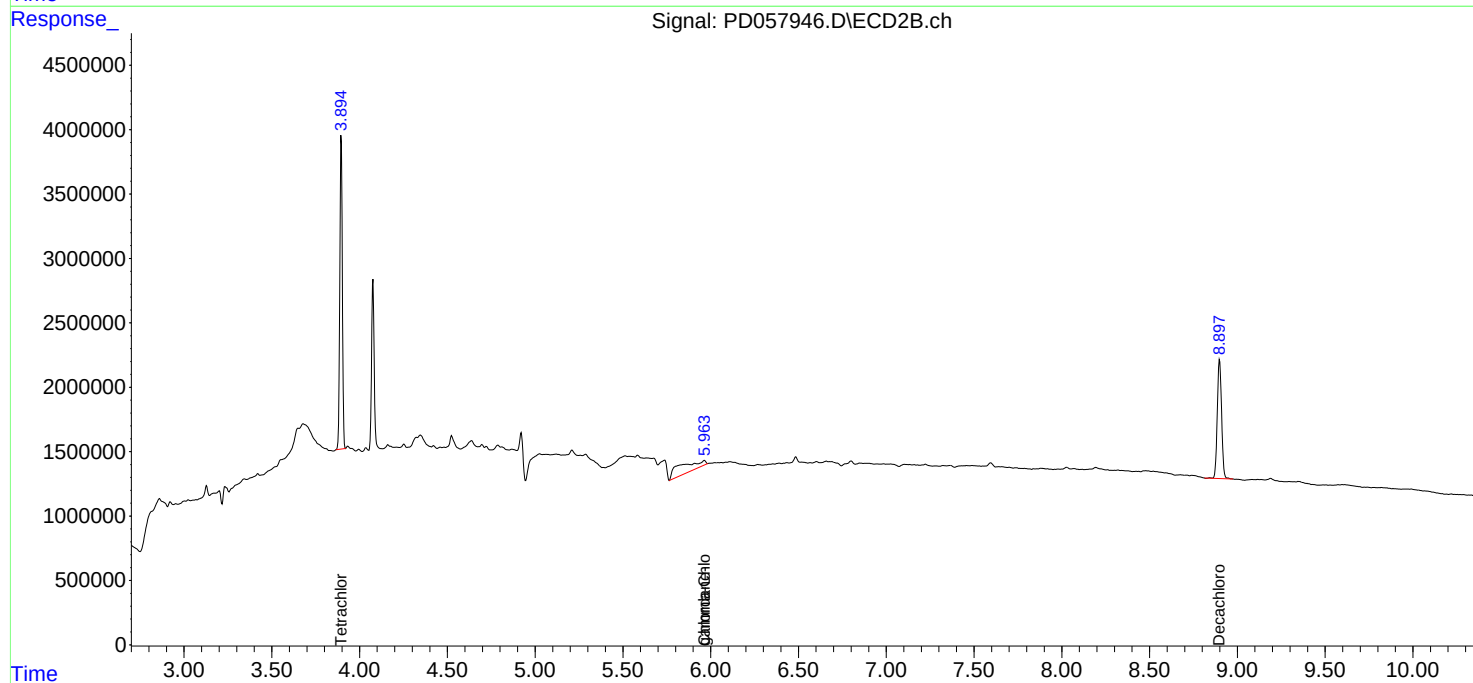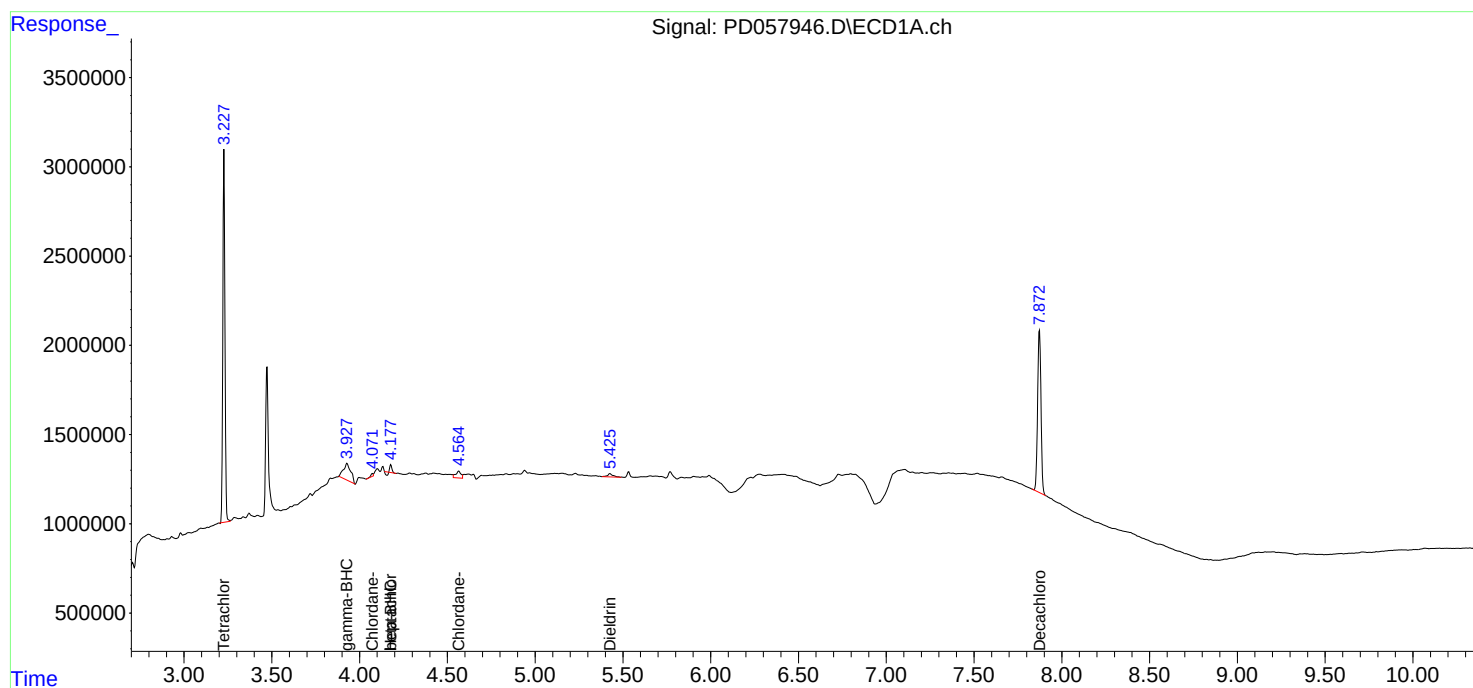


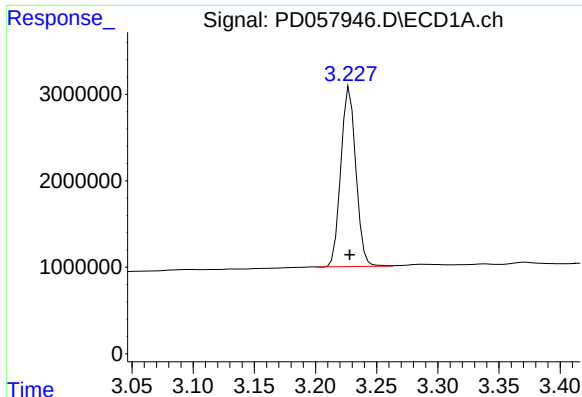

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 17730933
Conc: 20.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

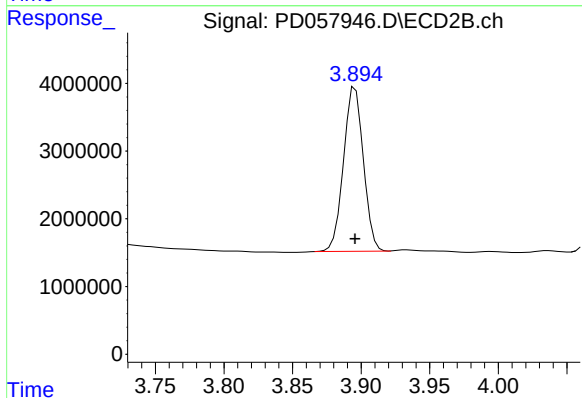


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 24435501
Conc: 20.77 ng/ml

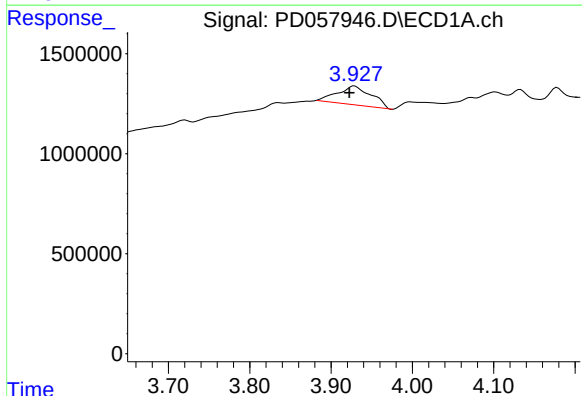


#3 gamma-BHC (Lindane)

R.T.: 3.929 min
Delta R.T.: 0.006 min
Response: 2741639
Conc: 1.98 ng/ml

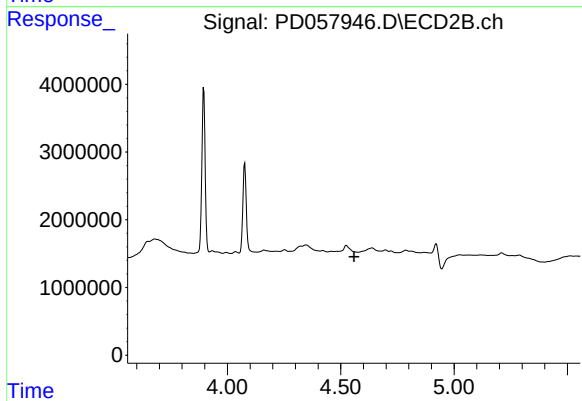

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

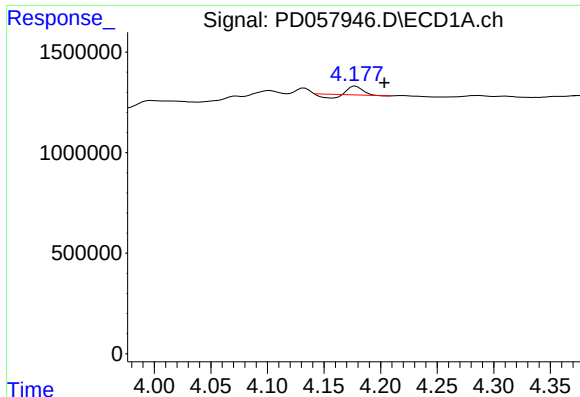

#4 Heptachlor


R.T.: 4.178 min
Delta R.T.: -0.025 min
Response: 226427
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

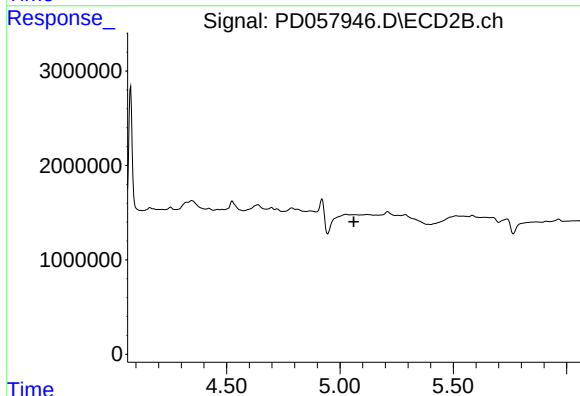


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

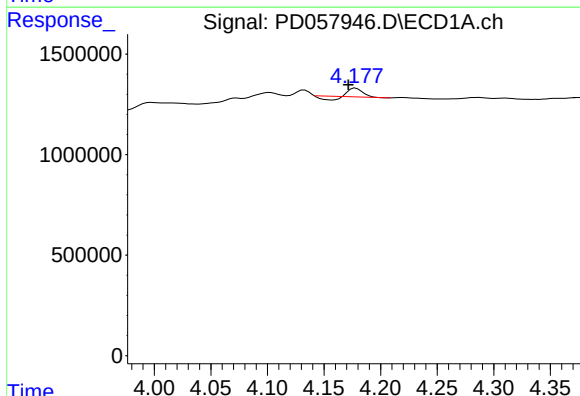


#6 beta-BHC

R.T.: 4.178 min
Delta R.T.: 0.007 min
Response: 226427
Conc: 0.44 ng/ml

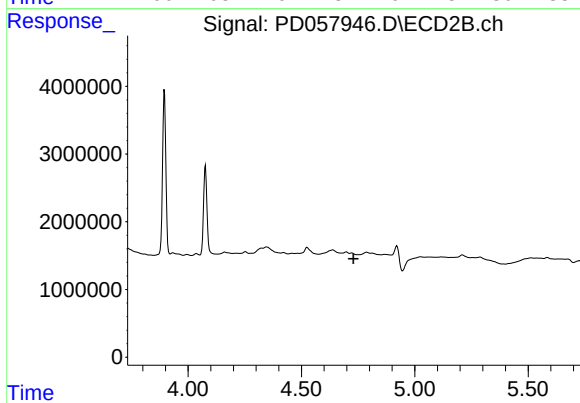

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.730 min
Response: 0
Conc: N.D.

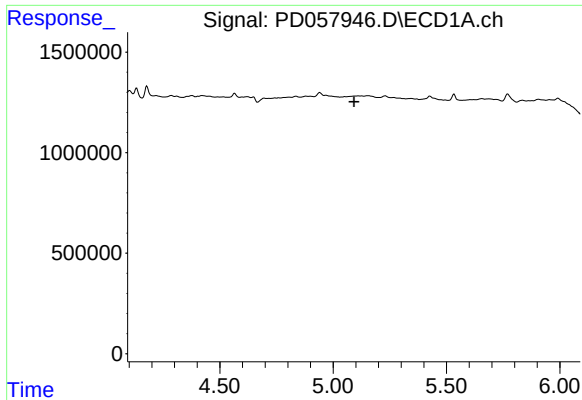

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

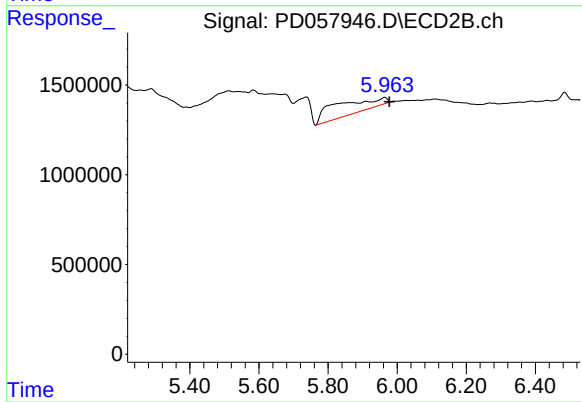


#10 gamma-Chlordane

R.T.: 5.965 min
Delta R.T.: -0.014 min
Response: 6929293
Conc: 4.52 ng/ml

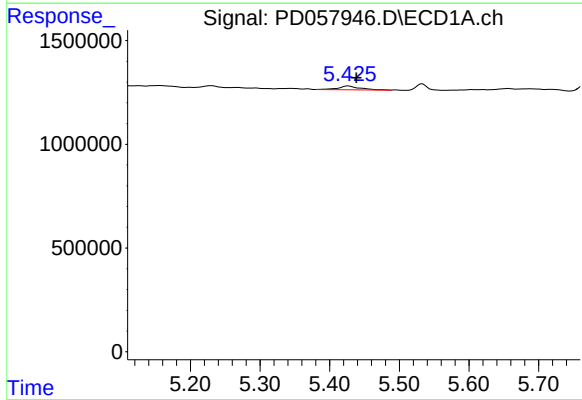


#13 Dieldrin

R.T.: 5.427 min
Delta R.T.: -0.012 min
Response: 412817
Conc: 0.38 ng/ml

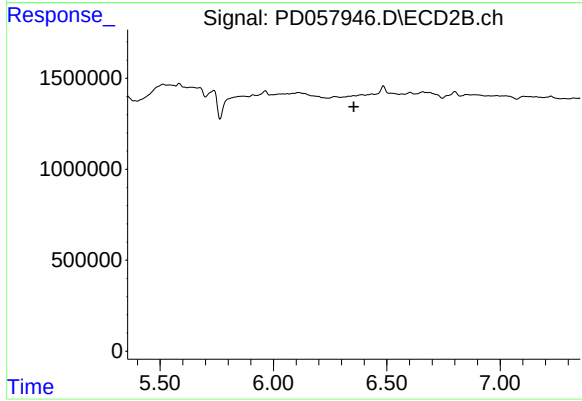

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.354 min
Response: 0
Conc: N.D.

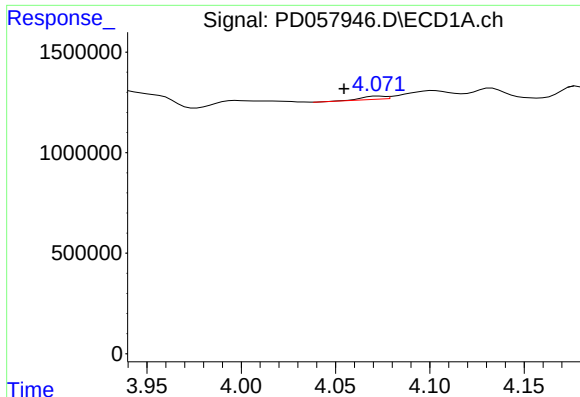

#23 Chlordane-1


R.T.: 4.073 min
Delta R.T.: 0.019 min
Response: 131913
Conc: 4.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

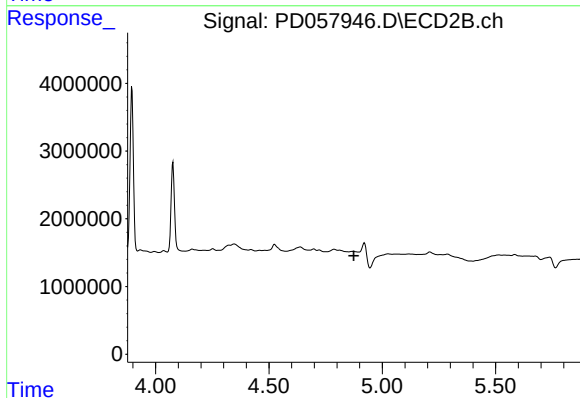


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

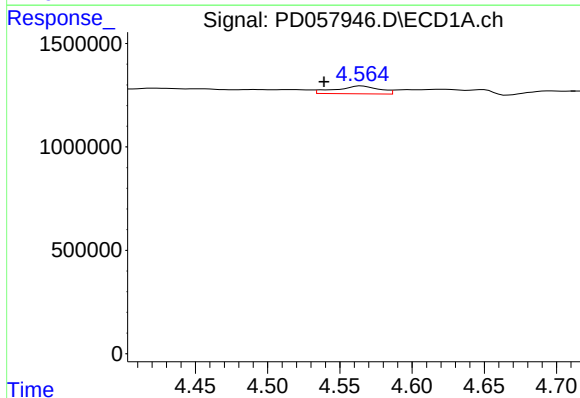


#24 Chlordane-2

R.T.: 4.565 min
Delta R.T.: 0.026 min
Response: 782553
Conc: 23.17 ng/ml

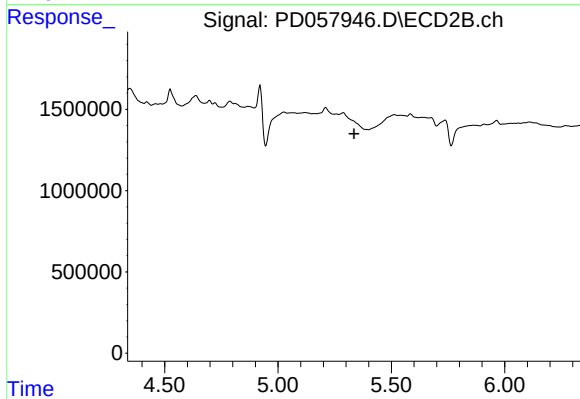

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

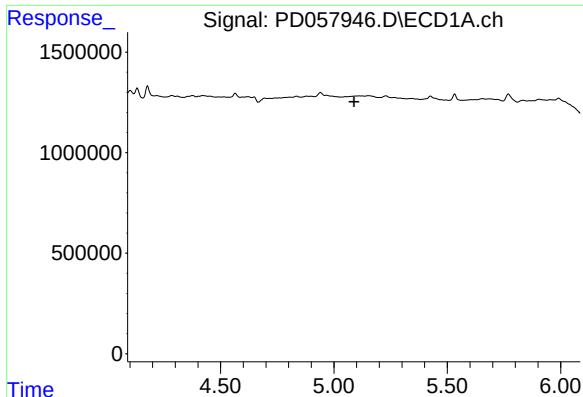

#25 Chloroform-3


R.T.: 0.000 min
Exp R.T.: 5.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

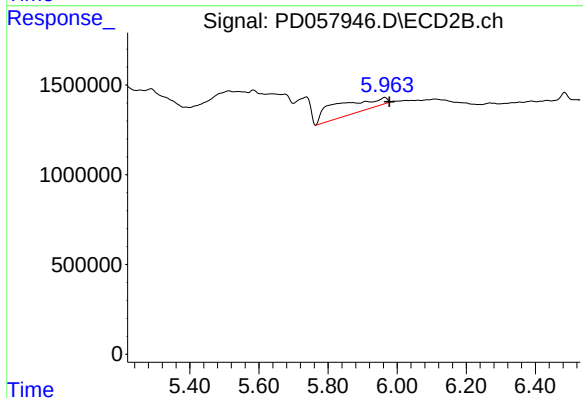


#25 Chloroform-3

R.T.: 5.965 min
Delta R.T.: -0.013 min
Response: 6929293
Conc: 36.54 ng/ml

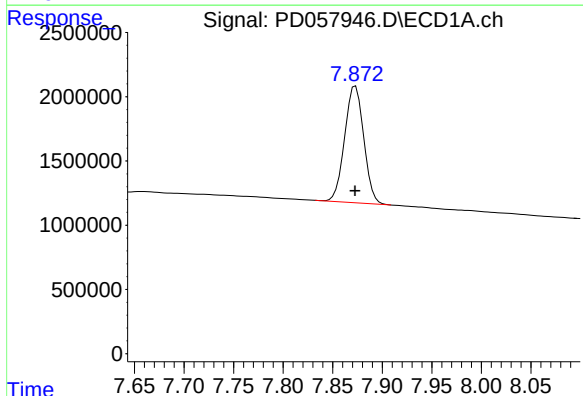

#28 Decachlorobiphenyl

R.T.: 7.873 min
Delta R.T.: 0.000 min
Response: 12154622
Conc: 13.49 ng/ml

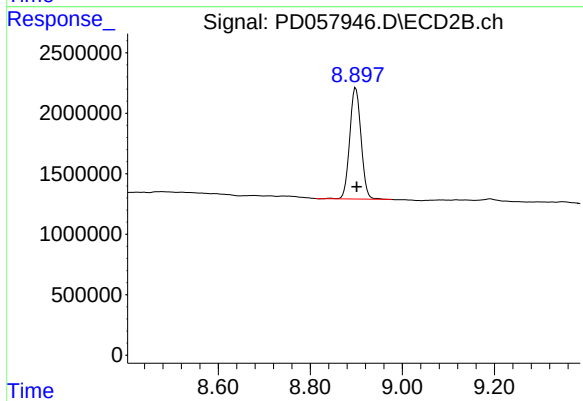

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: -0.002 min
Response: 15746559
Conc: 13.82 ng/ml