

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 19:26
 Operator : AJ\MA
 Sample : L2605-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 01:14:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.895	15920937	22073096	18.376	18.764
28)	SA Decachlor...	7.872	8.899	14030825	17790654	15.573	15.612
Target Compounds							
2)	A alpha-BHC	3.624f	0.000	845799	0	0.625	N.D. #
3)	MA gamma-BHC...	3.937	0.000	2300790	0	1.665	N.D. #
4)	MA Heptachlor	4.219f	5.058	1757246	1492371	1.559	0.894 #
7)	B delta-BHC	4.363	0.000	352568	0	0.277	N.D. #
8)	B Heptachlo...	4.867	0.000	276226	0	0.253	N.D. #
10)	B gamma-Chl...	5.094	0.000	113828	0	0.102	N.D. #
17)	MA 4,4'-DDT	6.059	0.000	889656	0	1.089	N.D. #
23)	Chlordane-1	4.073f	0.000	248742	0	8.828	N.D. #
24)	Chlordane-2	4.566f	0.000	1068294	0	31.625	N.D. #
25)	Chlordane-3	5.094	0.000	113828	0	1.124	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 19:26
Operator : AJ\MA
Sample : L2605-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 01:14:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

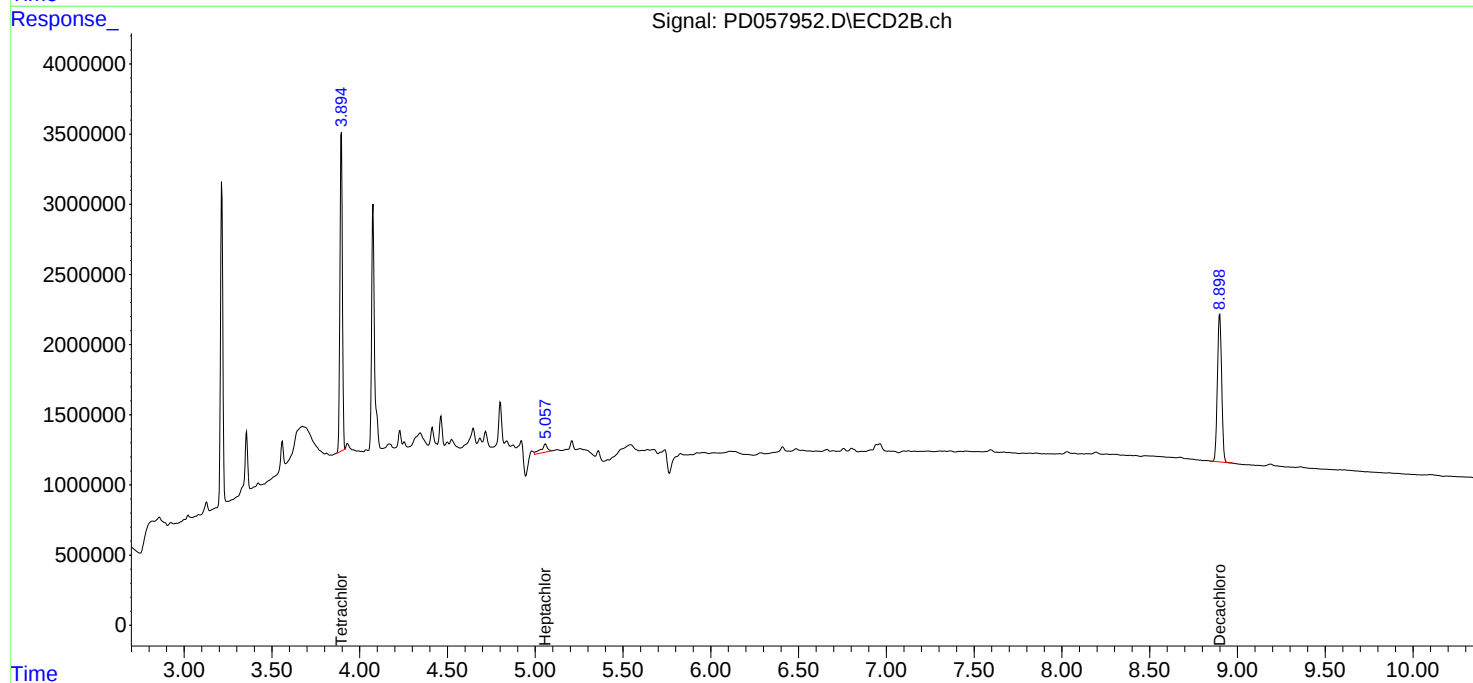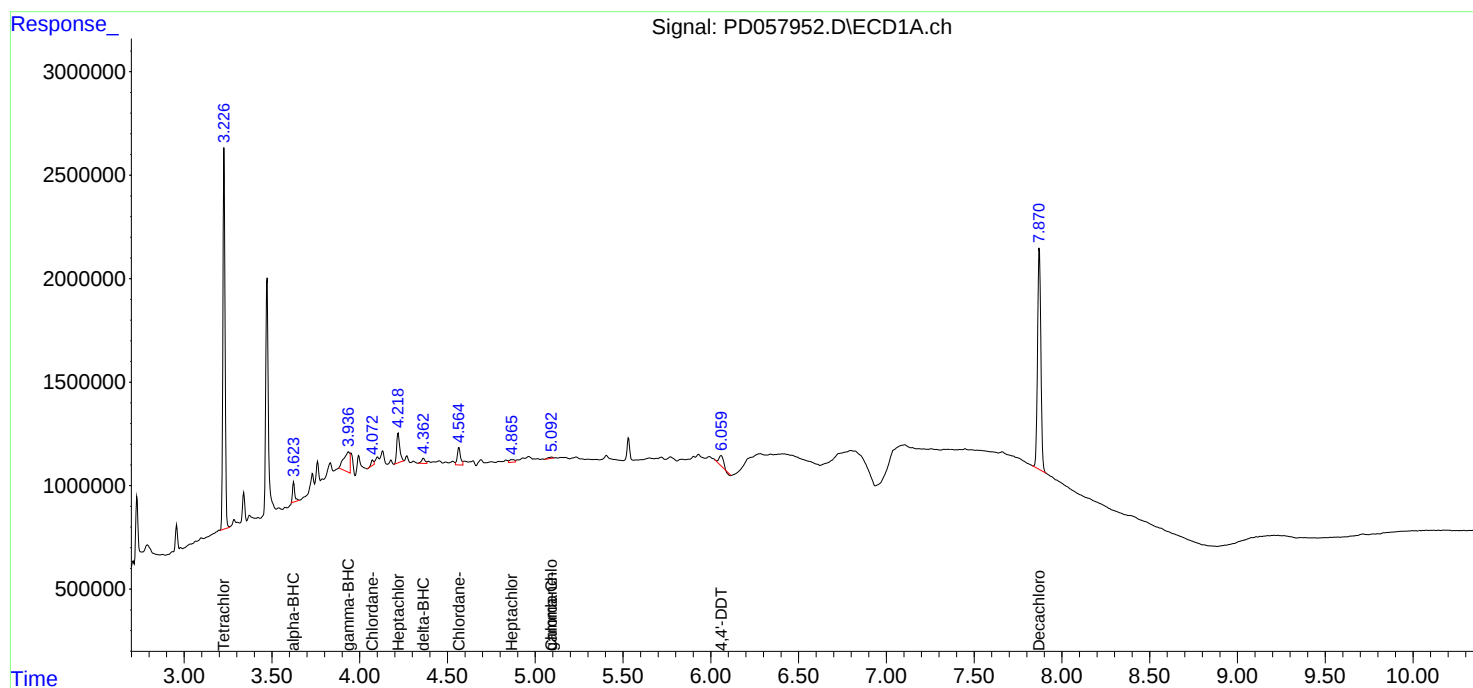


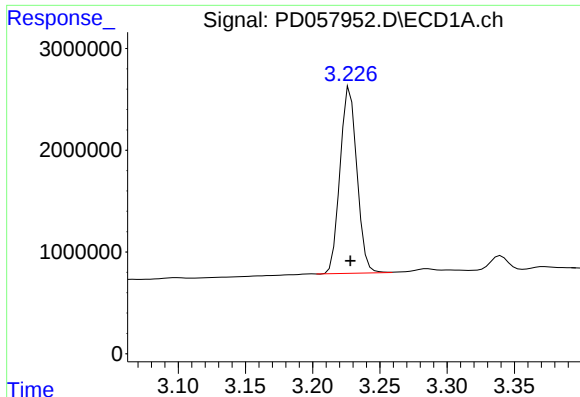

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 15920937
Conc: 18.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

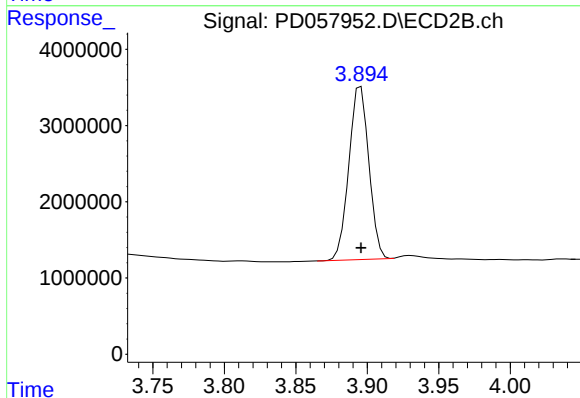


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 22073096
Conc: 18.76 ng/ml

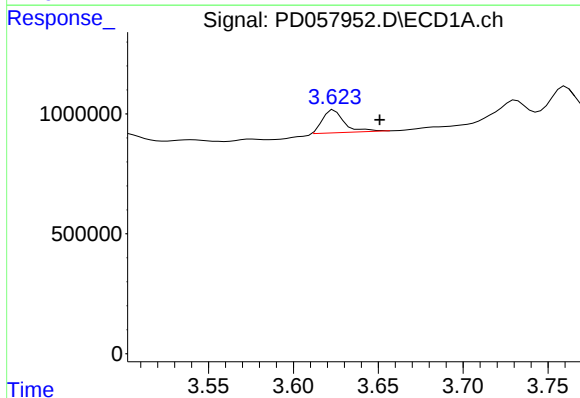


#2 alpha-BHC

R.T.: 3.624 min
Delta R.T.: -0.027 min
Response: 845799
Conc: 0.62 ng/ml

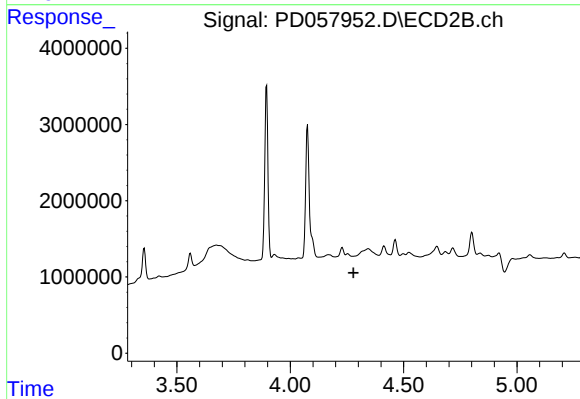

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.279 min
Response: 0
Conc: N.D.

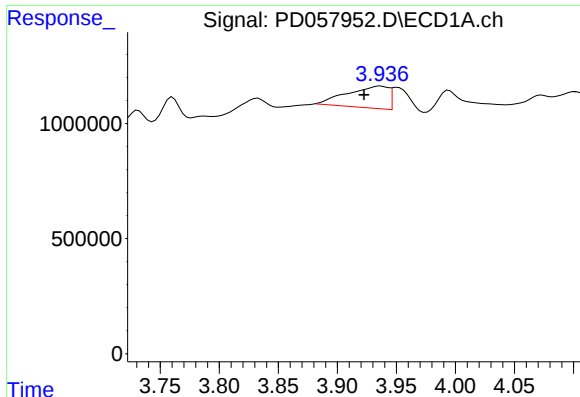

#3 gamma-BHC (Lindane)


R.T.: 3.937 min
Delta R.T.: 0.014 min
Response: 2300790
Conc: 1.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

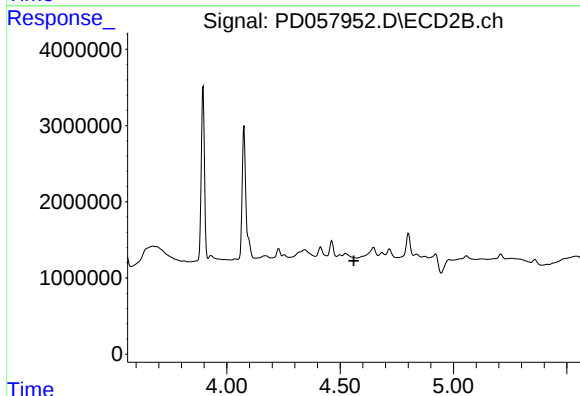


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

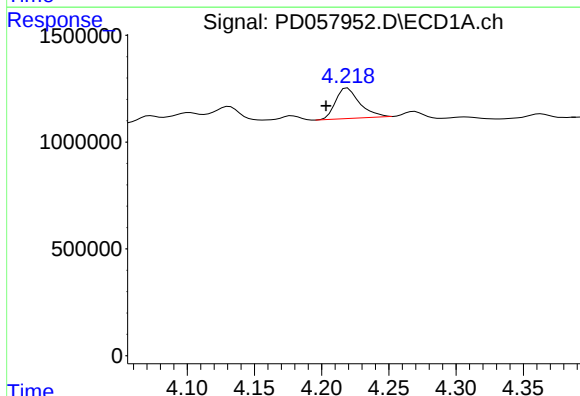


#4 Heptachlor

R.T.: 4.219 min
Delta R.T.: 0.016 min
Response: 1757246
Conc: 1.56 ng/ml

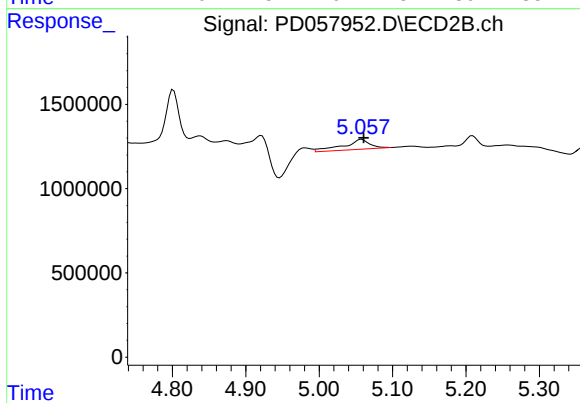

#4 Heptachlor


R.T.: 5.058 min
Delta R.T.: -0.003 min
Response: 1492371
Conc: 0.89 ng/ml

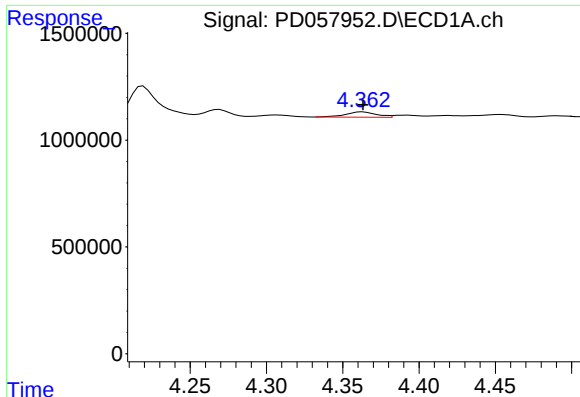

#7 delta-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 352568
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

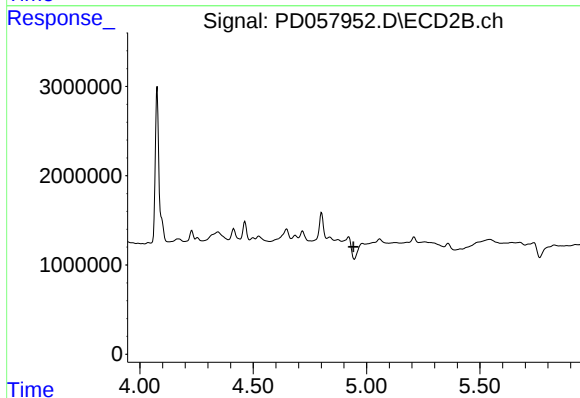


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

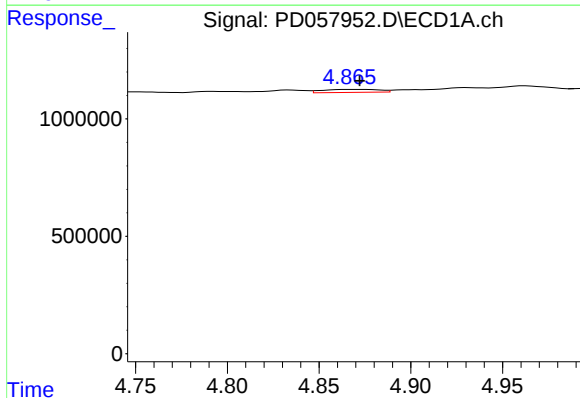


#8 Heptachlor epoxide

R.T.: 4.867 min
Delta R.T.: -0.006 min
Response: 276226
Conc: 0.25 ng/ml

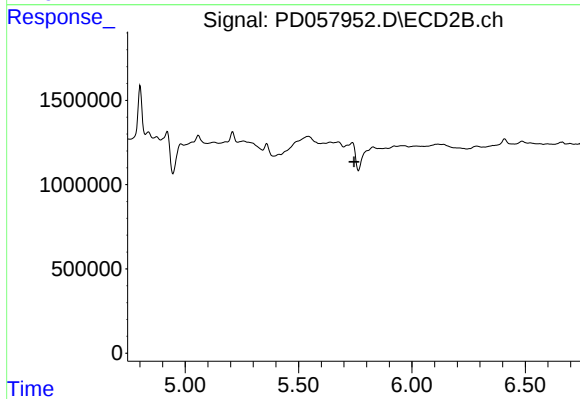

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.746 min
Response: 0
Conc: N.D.

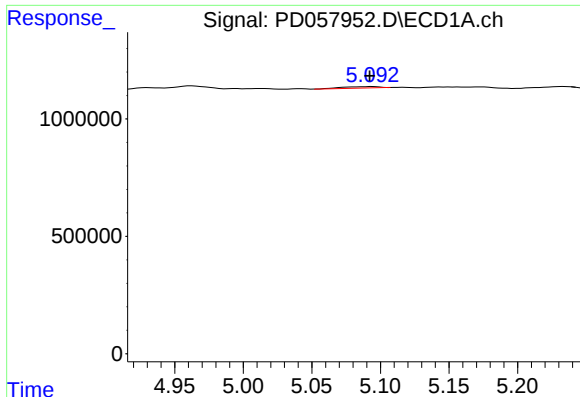

#10 gamma-Chlordane


R.T.: 5.094 min
Delta R.T.: 0.002 min
Response: 113828
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

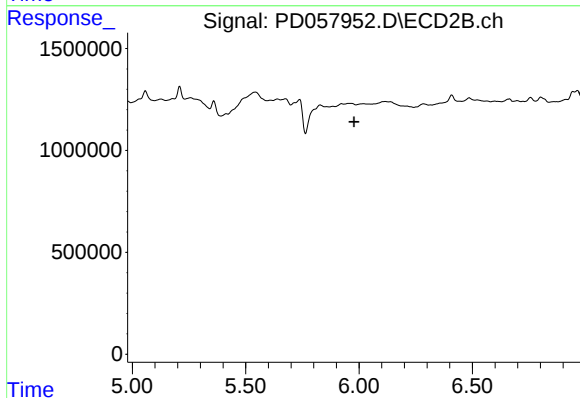


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

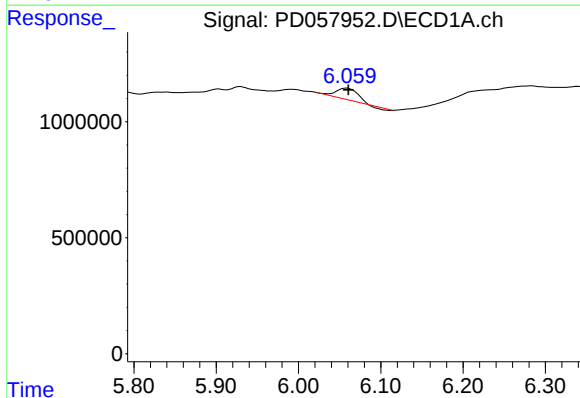


#17 4,4'-DDT

R.T.: 6.059 min
Delta R.T.: -0.002 min
Response: 889656
Conc: 1.09 ng/ml

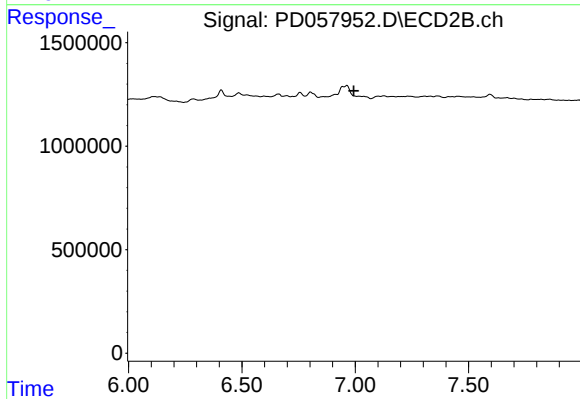

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.994 min
Response: 0
Conc: N.D.

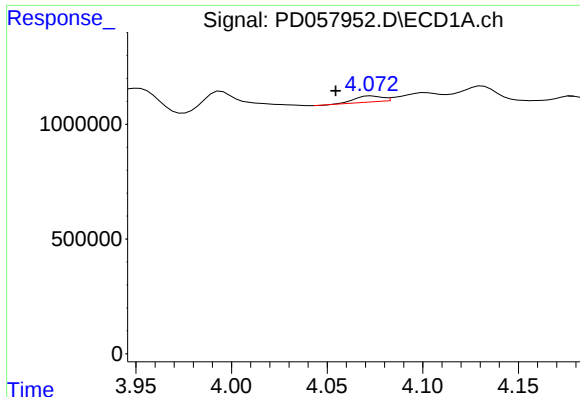

#23 Chlordane-1


R.T.: 4.073 min
Delta R.T.: 0.019 min
Response: 248742
Conc: 8.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

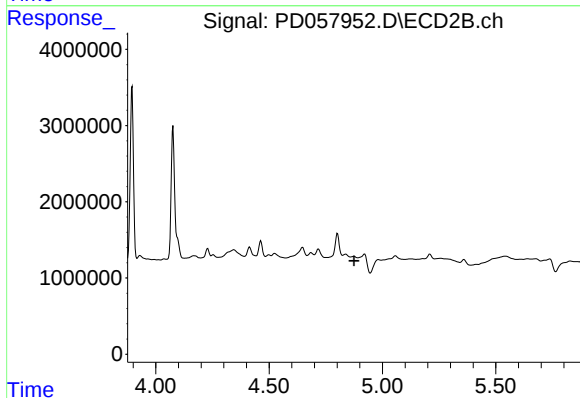


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

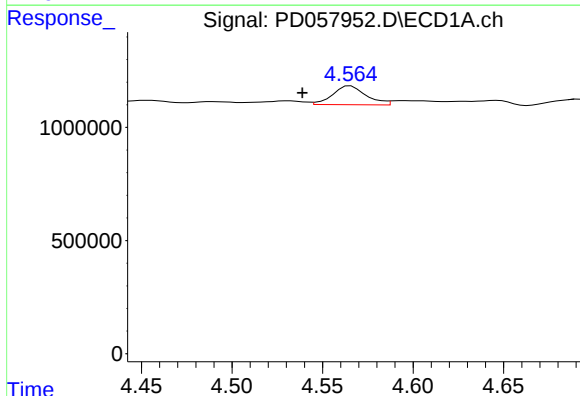


#24 Chlordane-2

R.T.: 4.566 min
Delta R.T.: 0.027 min
Response: 1068294
Conc: 31.63 ng/ml

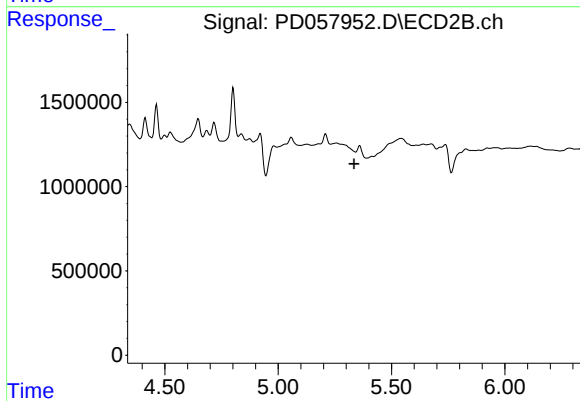

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

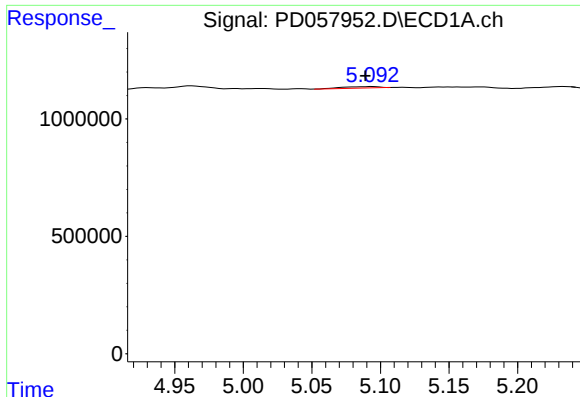

#25 Chlordane-3


R.T.: 5.094 min
Delta R.T.: 0.005 min
Response: 113828
Conc: 1.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

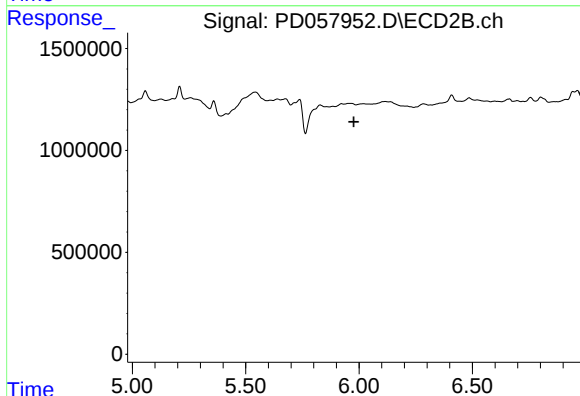


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

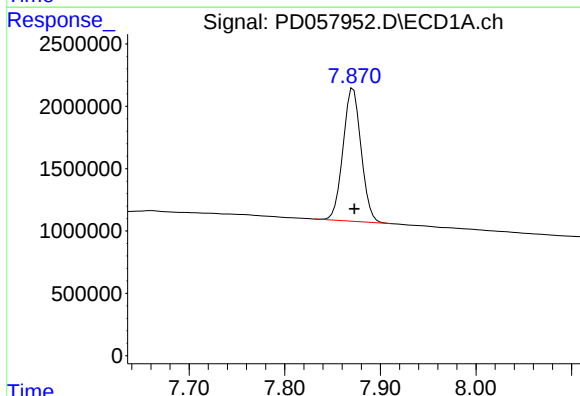

#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: -0.001 min
Response: 14030825
Conc: 15.57 ng/ml

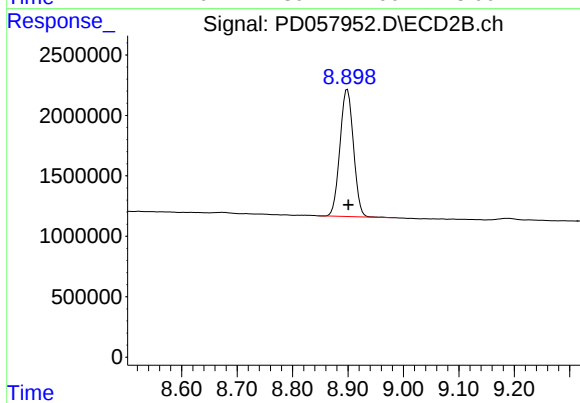

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: -0.002 min
Response: 17790654
Conc: 15.61 ng/ml