

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 09:42
 Operator : AJ\MA
 Sample : L2574-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HP-640

Manual Integrations
 APPROVED

mohammad
 5/14/2020 3:30:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 12:56:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.228	3.893	24318730	15489652	28.069m	13.168m#
28) SA Decachlor...	7.871	8.895	7183472	9209945	7.973	8.082m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 09:42
Operator : AJ\MA
Sample : L2574-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
HP-640


Manual Integrations
APPROVED

mohammad
5/14/2020 3:30:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 12:56:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

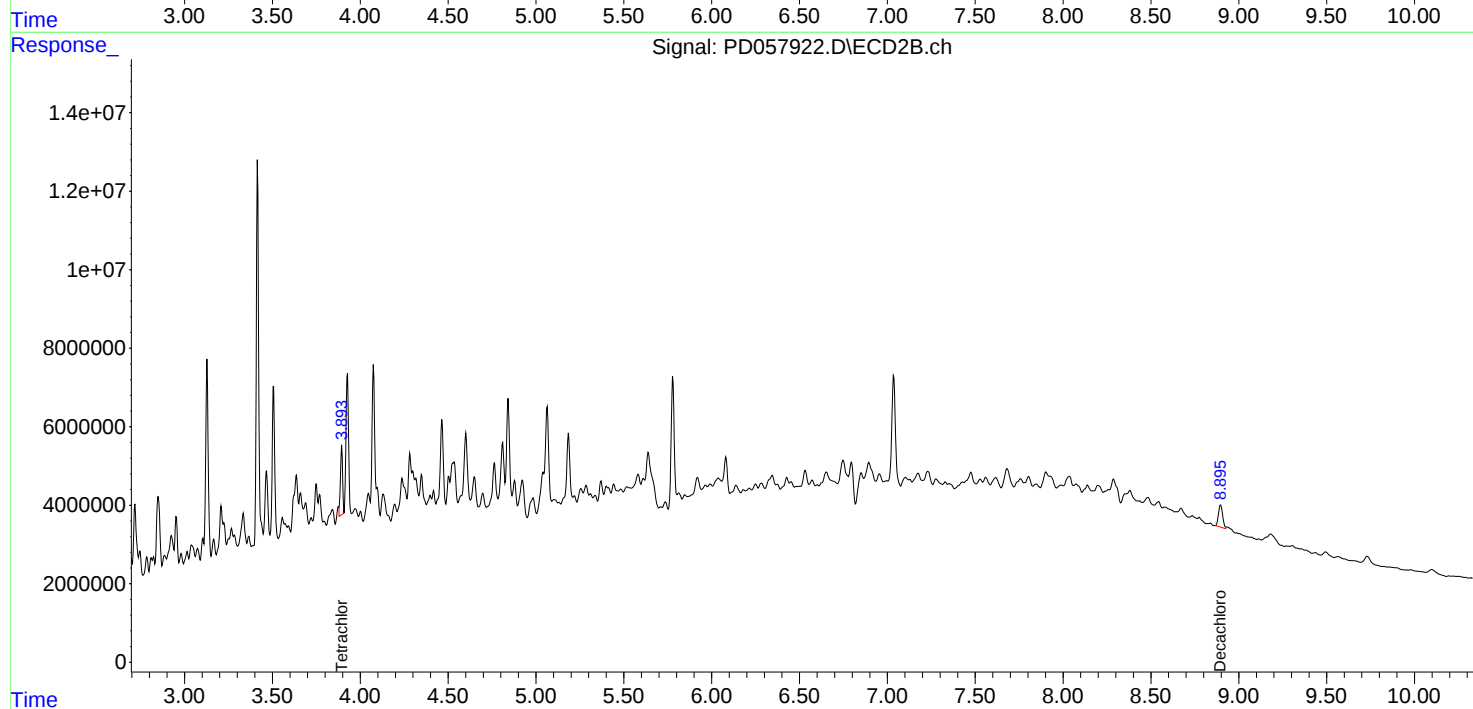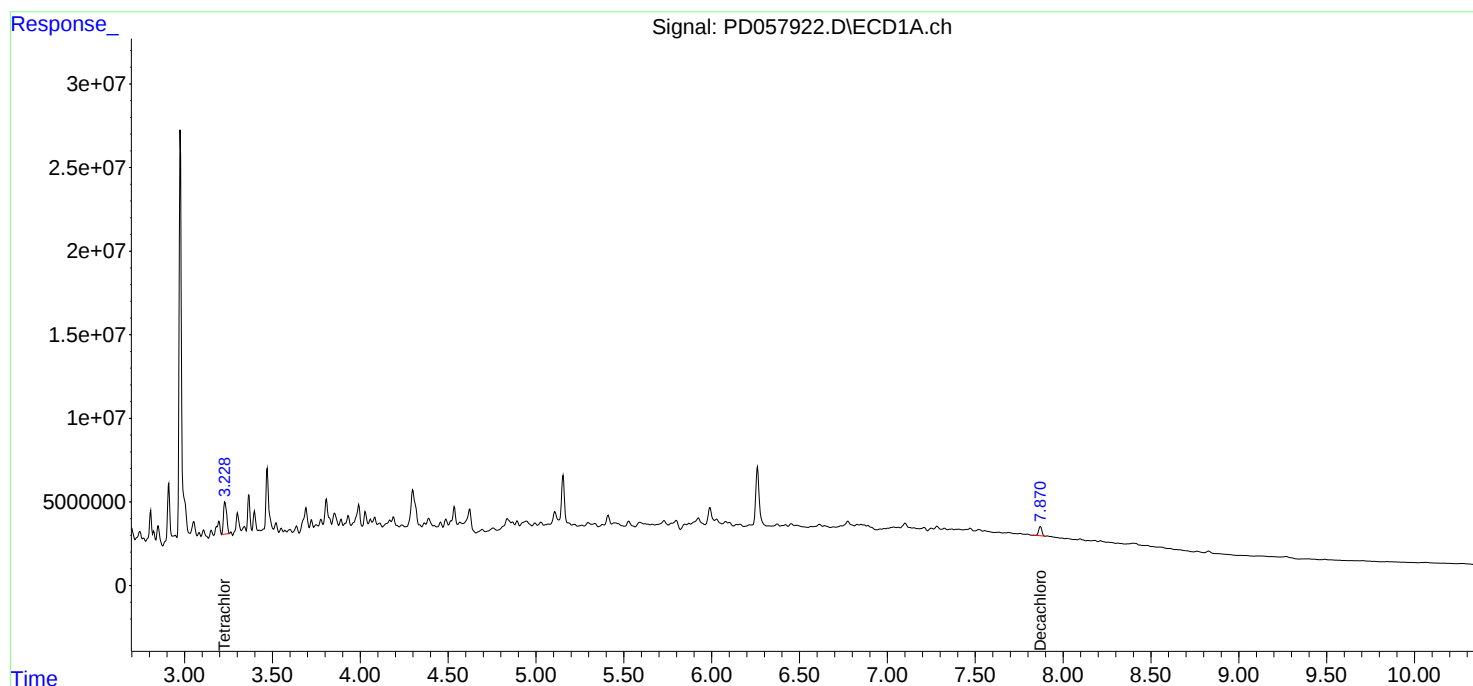

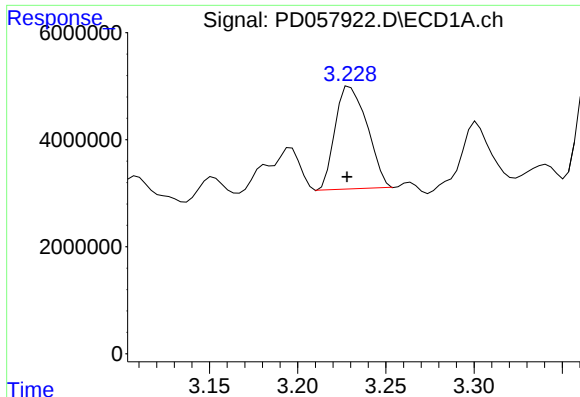


#1 Tetrachloro-m-xylene

R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 24318730
Conc: 28.07 ng/ml m

Instrument :
ECD_D
ClientSampleId :
HP-640


Manual Integrations
APPROVED

mohammad
5/14/2020 3:30:54 PM

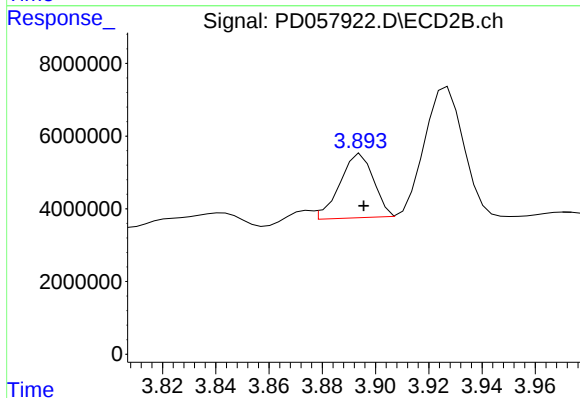


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.002 min
Response: 15489652
Conc: 13.17 ng/ml m

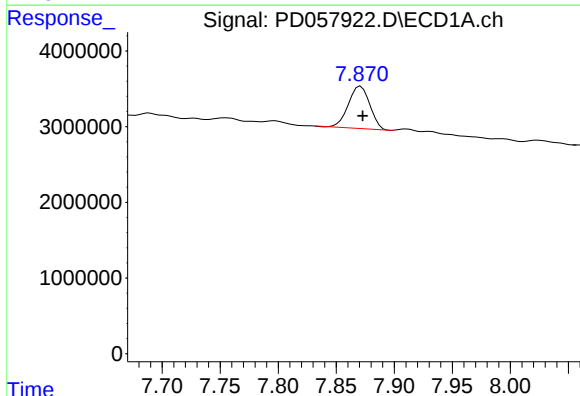

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: -0.002 min
Response: 7183472
Conc: 7.97 ng/ml

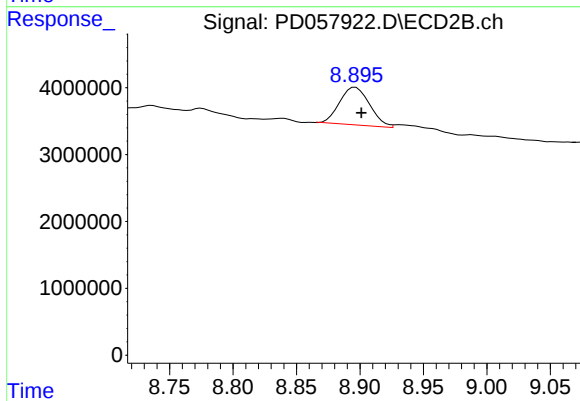

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: -0.006 min
Response: 9209945
Conc: 8.08 ng/ml m