

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 10:13
 Operator : AJ\MA
 Sample : L2502-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PL-01-050820

Manual Integrations
 APPROVED

mohammad
 5/14/2020 3:30:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 12:56:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.230	3.894	1891771	2009291	2.184	1.708
28) SA Decachlor...	7.873	8.896	2214797	5419839	2.458m	4.756m#
Target Compounds						
3) MA gamma-BHC...	3.931	4.540f	10245443	9903096	7.416	5.780

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 10:13
Operator : AJ\MA
Sample : L2502-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PL-01-050820


Manual Integrations
APPROVED

mohammad
5/14/2020 3:30:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 12:56:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

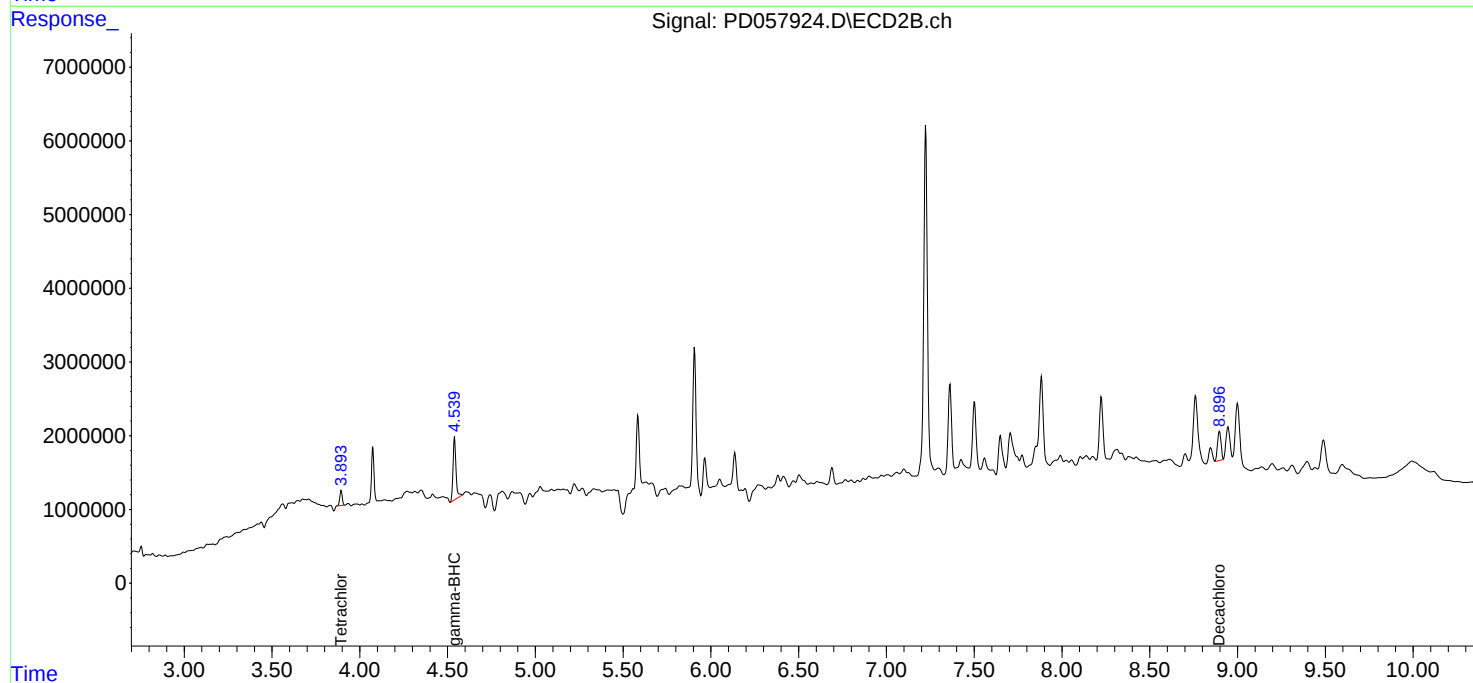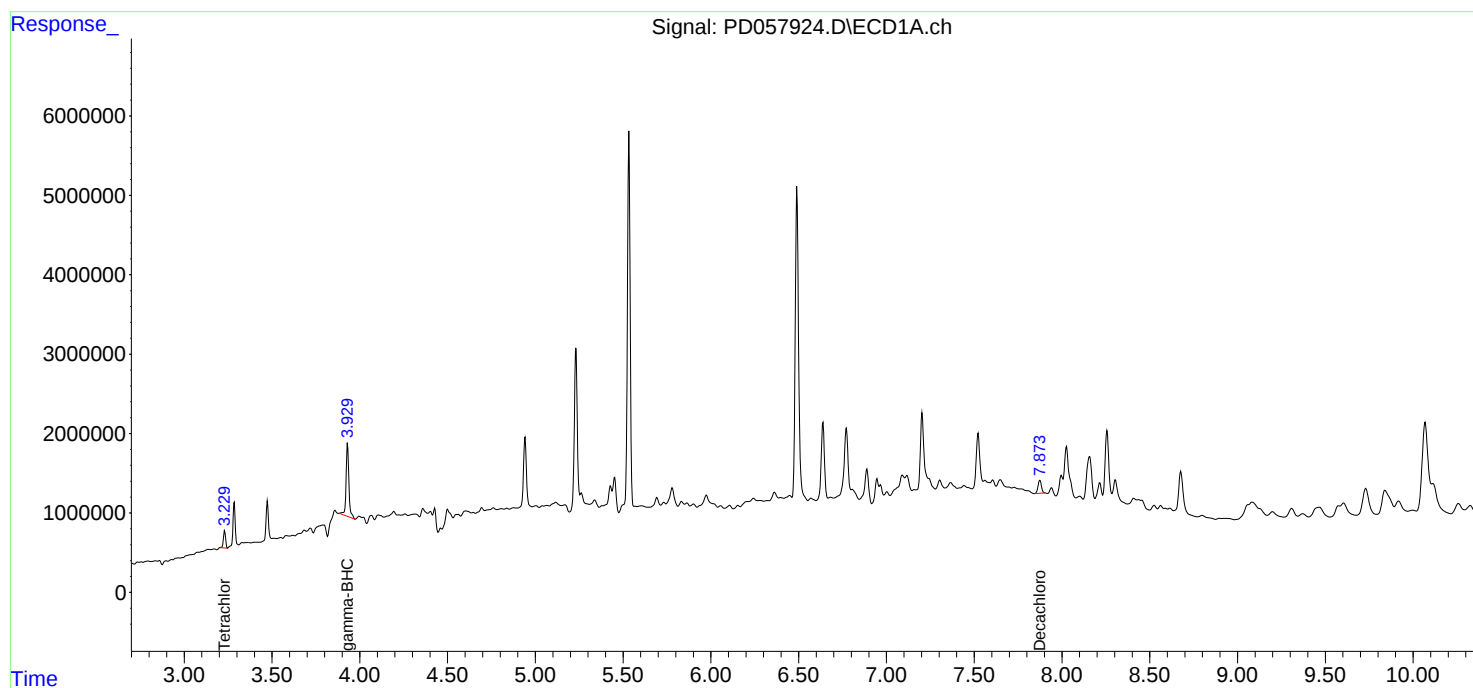

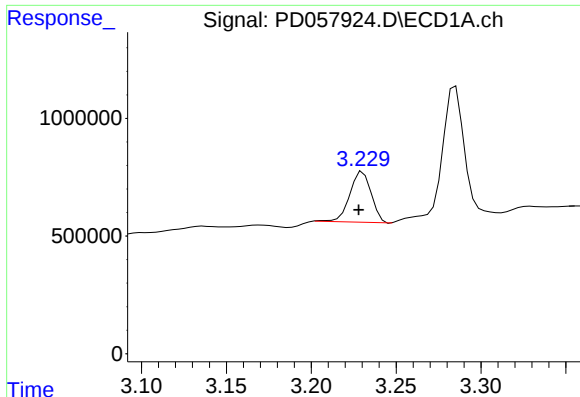


#1 Tetrachloro-m-xylene

R.T.: 3.230 min
Delta R.T.: 0.002 min
Response: 1891771
Conc: 2.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PL-01-050820


Manual Integrations
APPROVED

mohammad
5/14/2020 3:30:59 PM

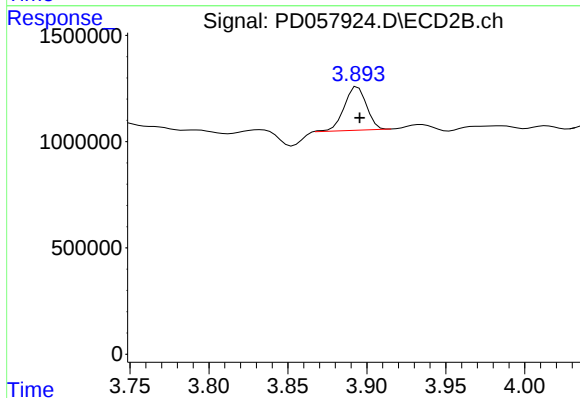


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.001 min
Response: 2009291
Conc: 1.71 ng/ml

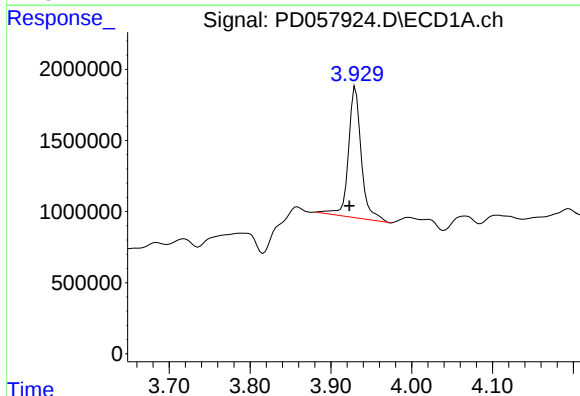


#3 gamma-BHC (Lindane)

R.T.: 3.931 min
Delta R.T.: 0.008 min
Response: 10245443
Conc: 7.42 ng/ml

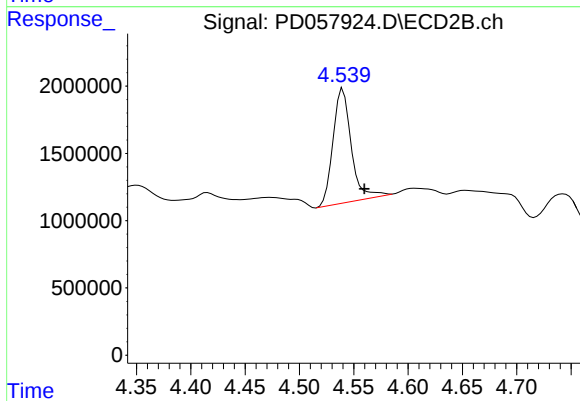

#3 gamma-BHC (Lindane)

R.T.: 4.540 min
Delta R.T.: -0.020 min
Response: 9903096
Conc: 5.78 ng/ml

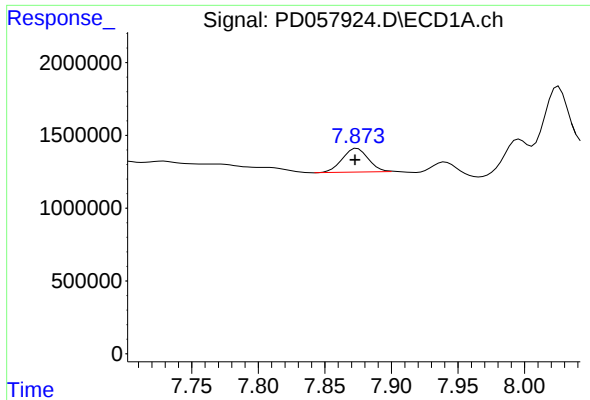


#28 Decachlorobiphenyl

R.T.: 7.873 min
Delta R.T.: 0.000 min
Response: 2214797
Conc: 2.46 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PL-01-050820

Manual Integrations
APPROVED

mohammad
5/14/2020 3:30:59 PM

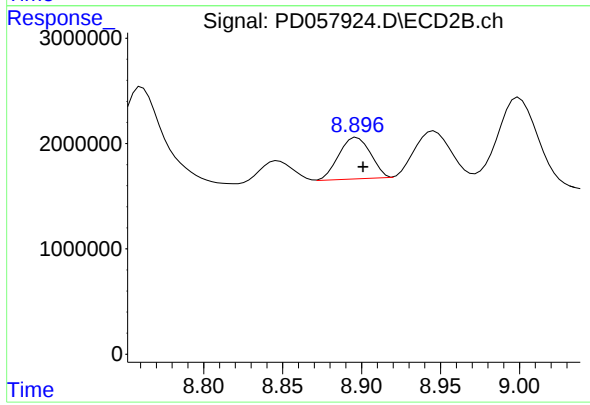

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: -0.005 min
Response: 5419839
Conc: 4.76 ng/ml m