

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
 Data File : PD057937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 15:40
 Operator : AJ\MA
 Sample : L2500-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-02-051220

Manual Integrations
 APPROVED

mohammad
 5/14/2020 3:31:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 07:25:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
 Quant Title : GC Extractables
 QLast Update : Tue May 12 12:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.895	10604324	14531648	12.240	12.353
28)	SA Decachlor...	7.872	8.899	9386619	14728237	10.418	12.925
Target Compounds							
10)	B gamma-Chl...	5.111f	5.975	255081	250445	0.228m	0.163m#
17)	MA 4,4'-DDT	6.057	6.993	1028835	1485531	1.260m	1.263

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051320\
Data File : PD057937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 15:40
Operator : AJ\MA
Sample : L2500-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OK-02-051220


Manual Integrations
APPROVED

mohammad
5/14/2020 3:31:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 07:25:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051220.M
Quant Title : GC Extractables
QLast Update : Tue May 12 12:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

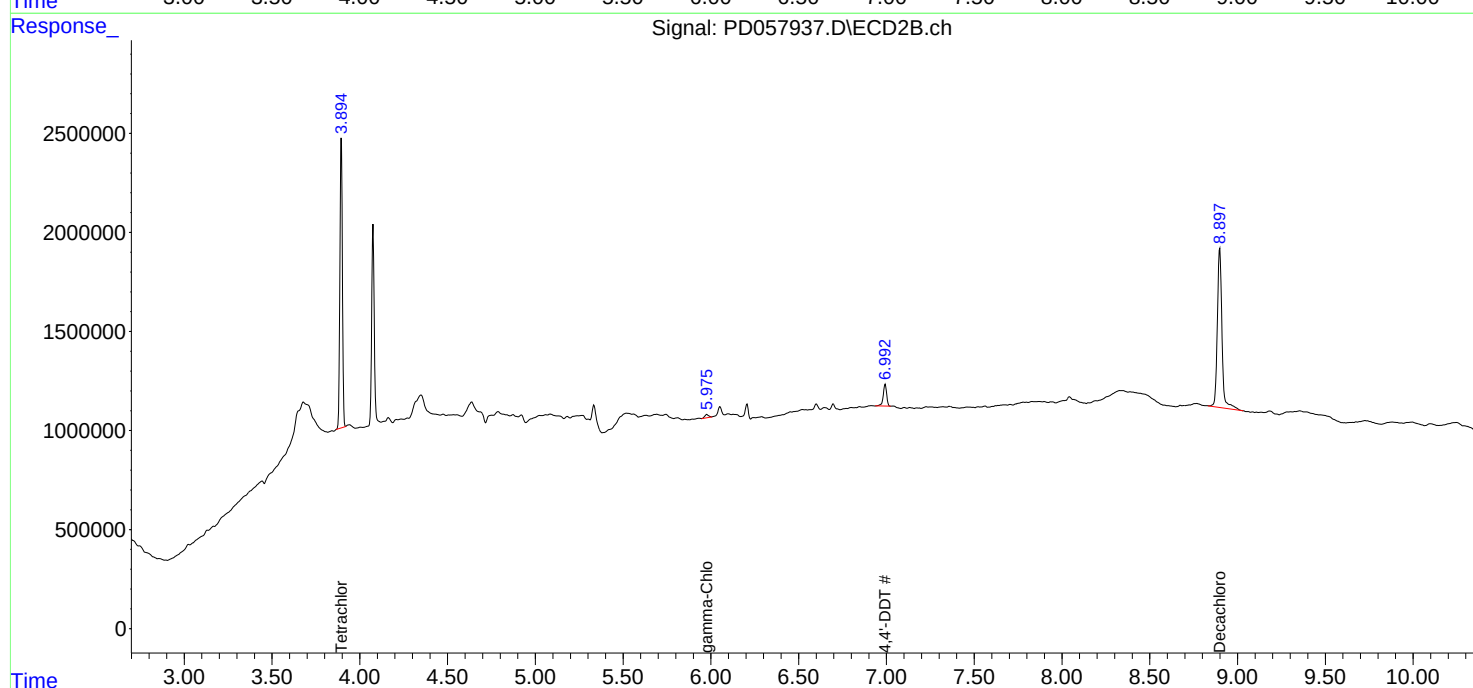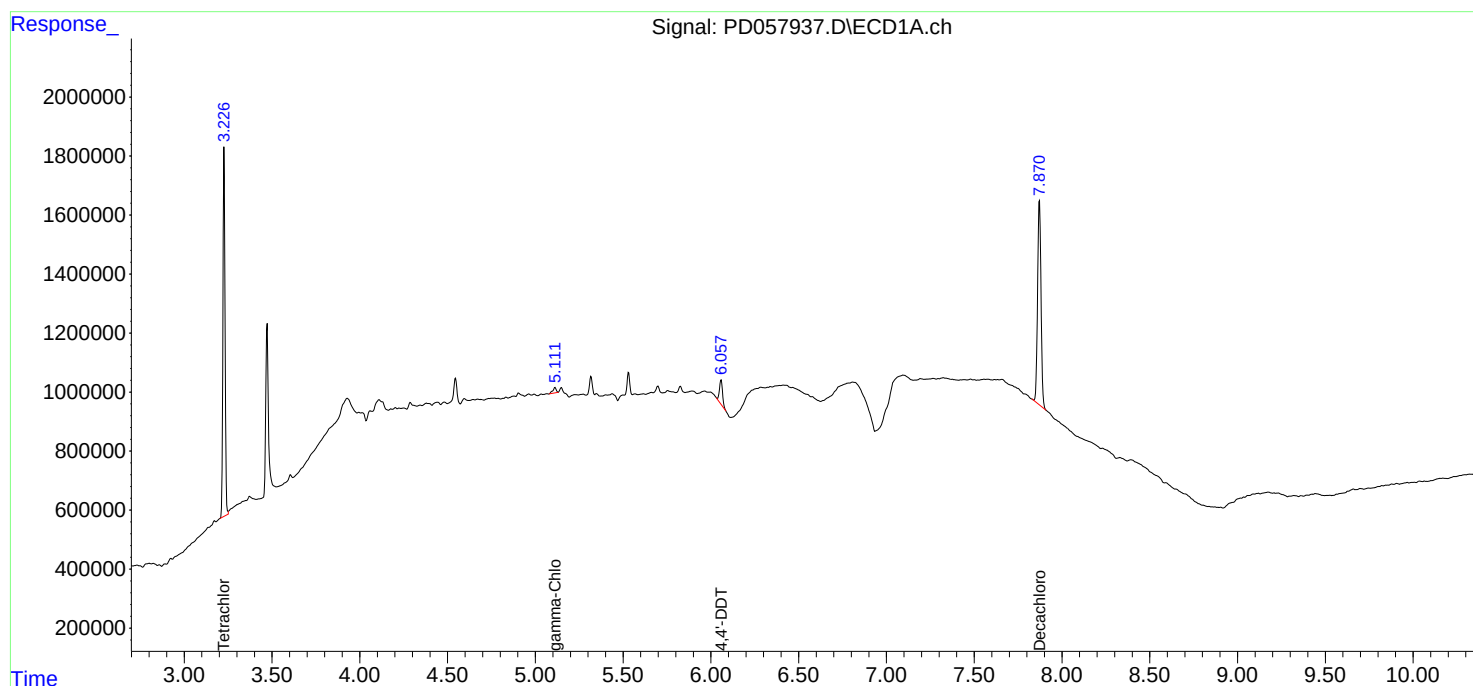

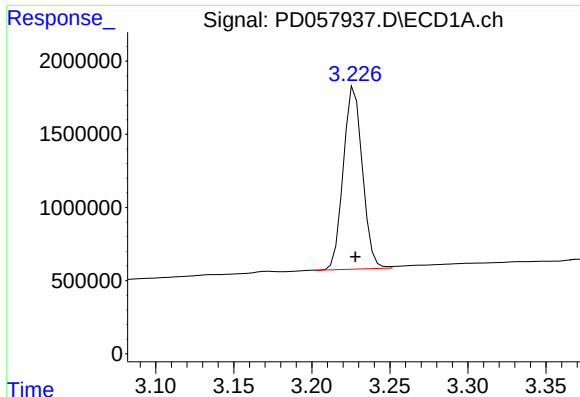


#1 Tetrachloro-m-xylene

R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 10604324
Conc: 12.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-02-051220


Manual Integrations
APPROVED

mohammad
5/14/2020 3:31:59 PM

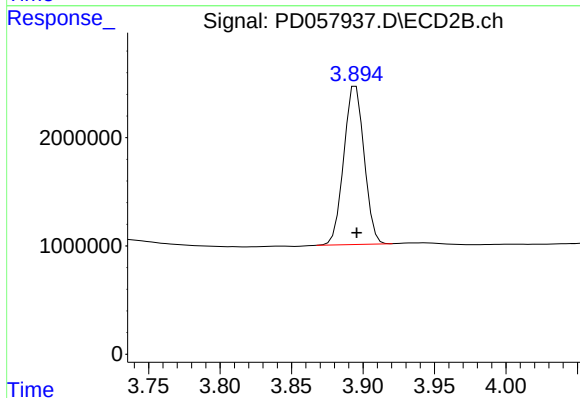


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 14531648
Conc: 12.35 ng/ml

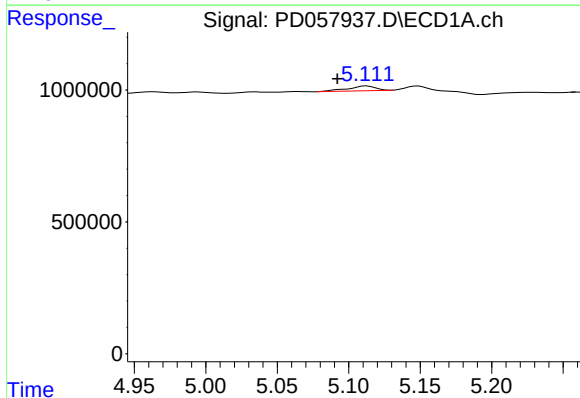


#10 gamma-Chlordane

R.T.: 5.111 min
Delta R.T.: 0.019 min
Response: 255081
Conc: 0.23 ng/ml m

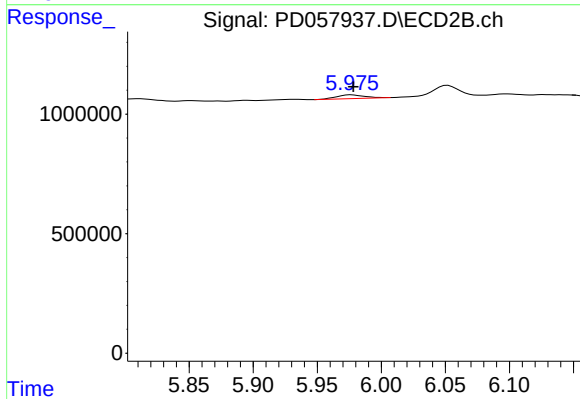

#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: -0.003 min
Response: 250445
Conc: 0.16 ng/ml m

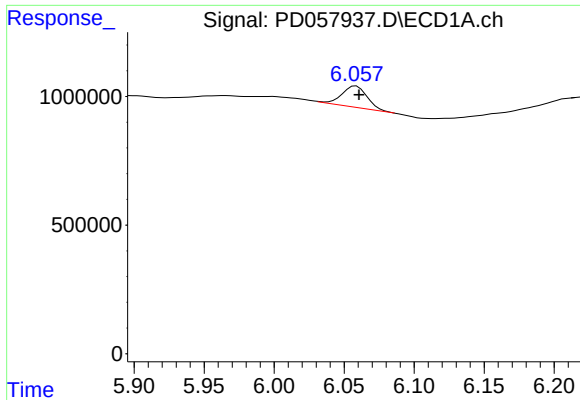


#17 4,4'-DDT

R.T.: 6.057 min
Delta R.T.: -0.003 min
Response: 1028835
Conc: 1.26 ng/ml m

Instrument :
ECD_D
ClientSampleId :
OK-02-051220


Manual Integrations
APPROVED

mohammad
5/14/2020 3:31:59 PM

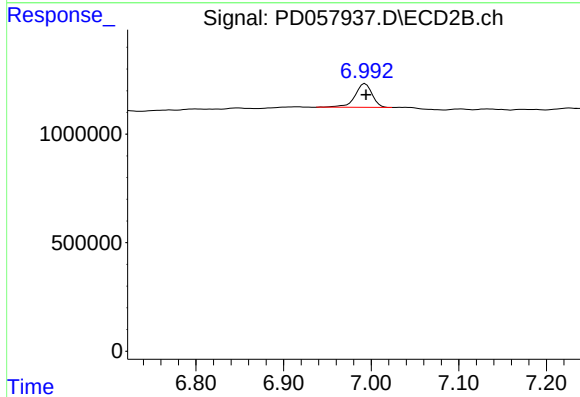


#17 4,4'-DDT

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 1485531
Conc: 1.26 ng/ml

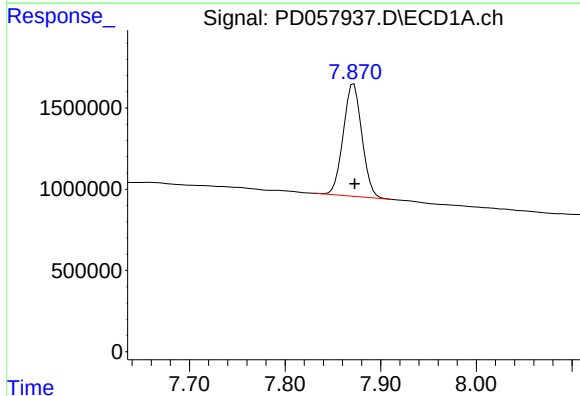

#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.000 min
Response: 9386619
Conc: 10.42 ng/ml

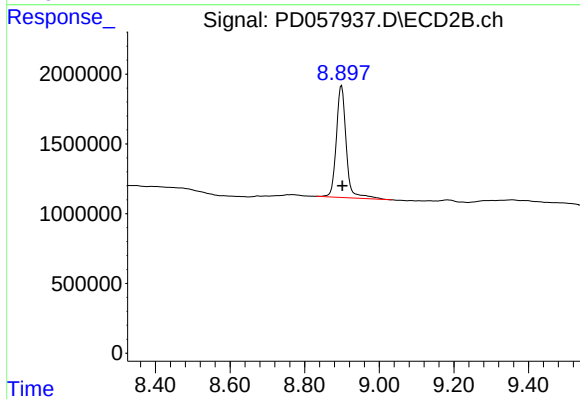

#28 Decachlorobiphenyl

R.T.: 8.899 min
Delta R.T.: -0.002 min
Response: 14728237
Conc: 12.92 ng/ml