

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051325\
 Data File : PD088534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2025 19:05
 Operator : AR\AJ
 Sample : Q2014-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MOO-25-0148

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/14/2025
 Supervised By : mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 22:47:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 06:32:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.576f	2.923f	11845439	67205232	5.930m	4.596m
28) SA Decachlor...	9.074	8.075	31037089	112.7E6	9.382	6.101 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051325\
Data File : PD088534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2025 19:05
Operator : AR\AJ
Sample : Q2014-05
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MOO-25-0148


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/14/2025
Supervised By : mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 22:47:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 06:32:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

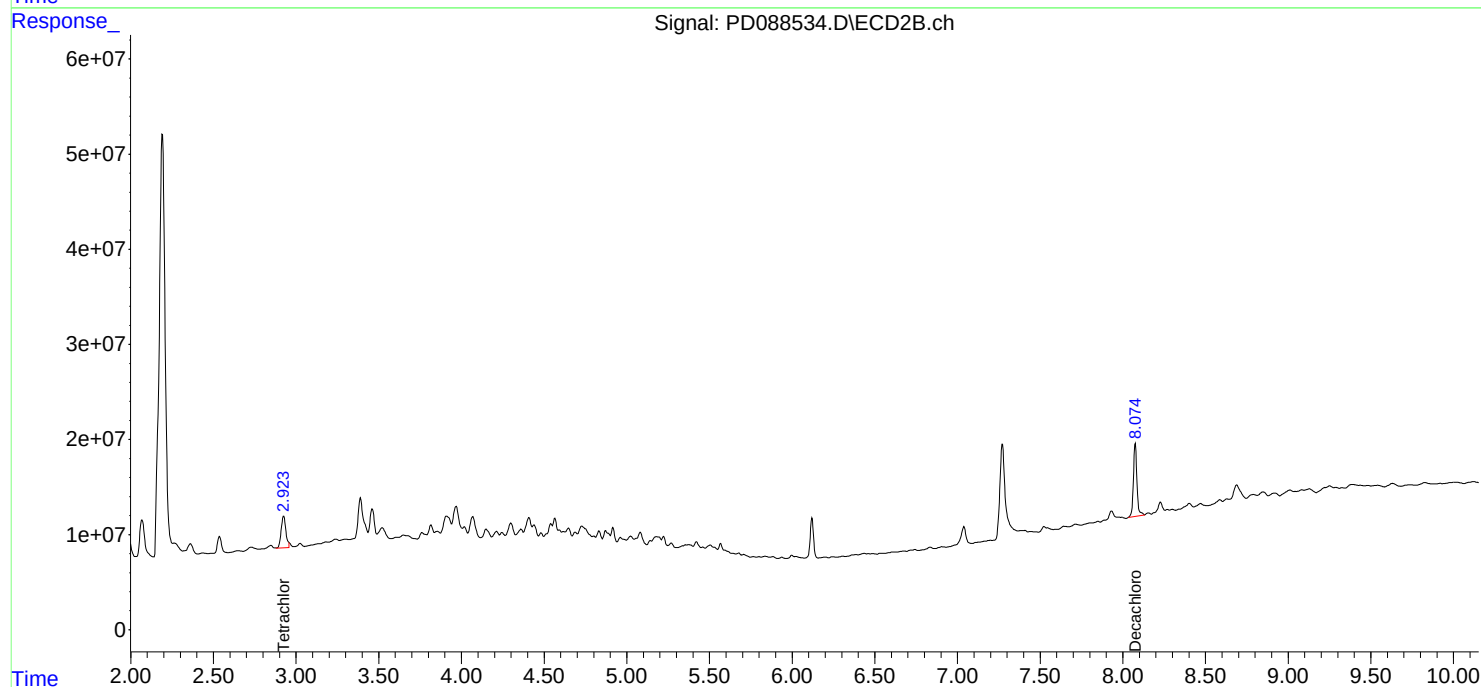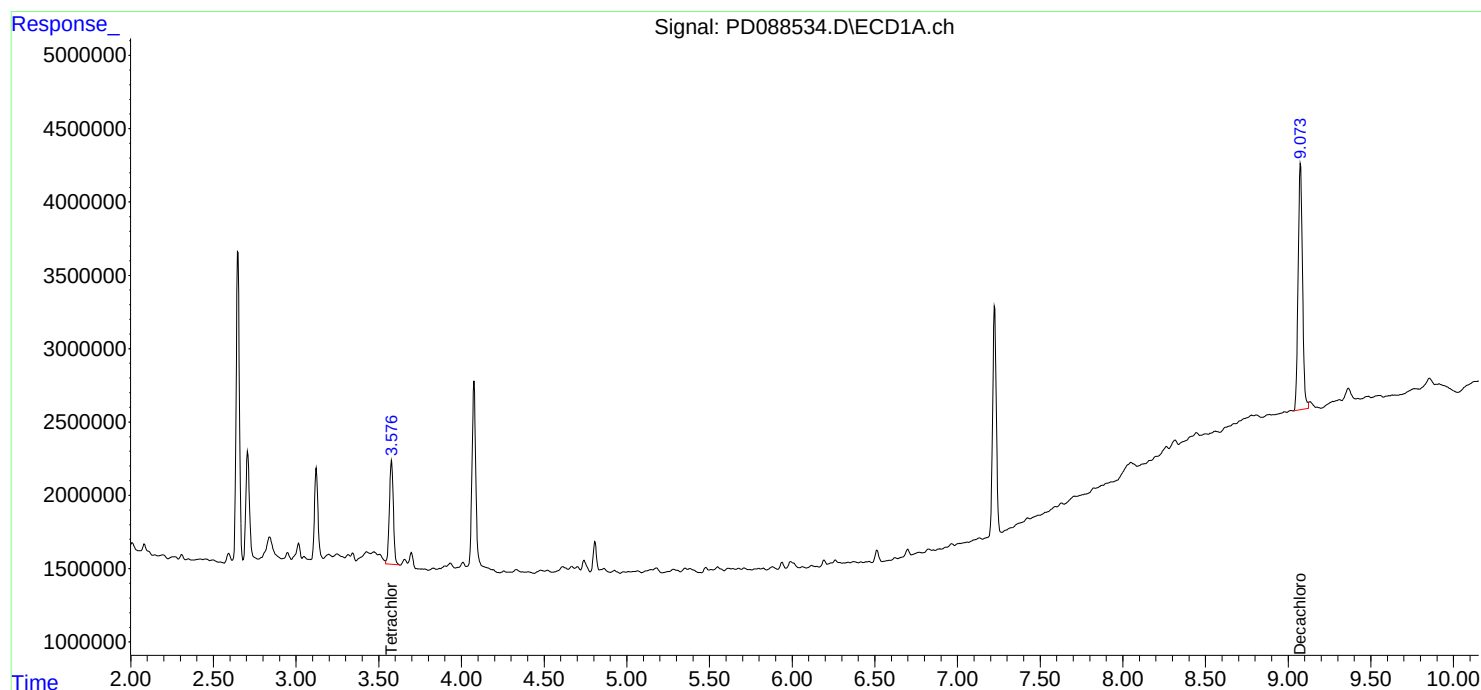

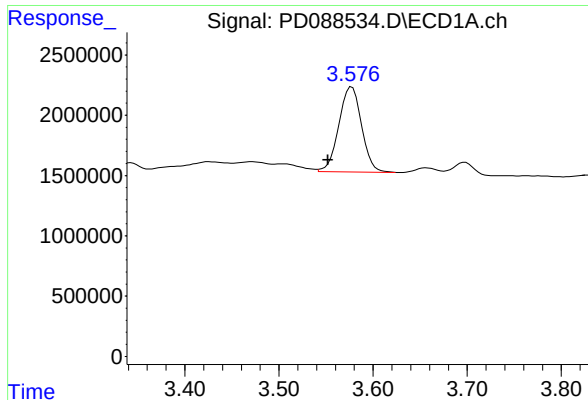


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: 0.024 min
Response: 11845439
Conc: 5.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
MOO-25-0148


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/14/2025
Supervised By :mohammad ahmed 05/20/2025

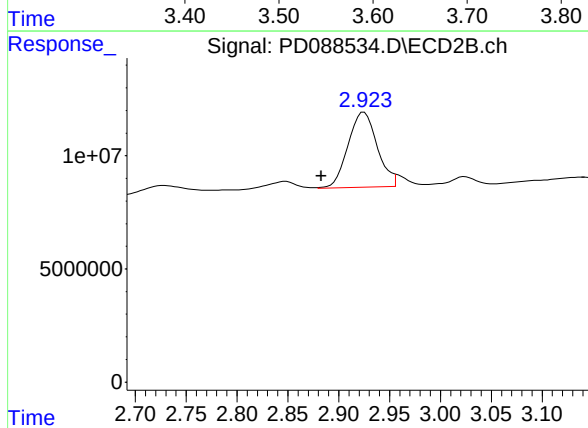


#1 Tetrachloro-m-xylene

R.T.: 2.923 min
Delta R.T.: 0.040 min
Response: 67205232
Conc: 4.60 ng/ml m

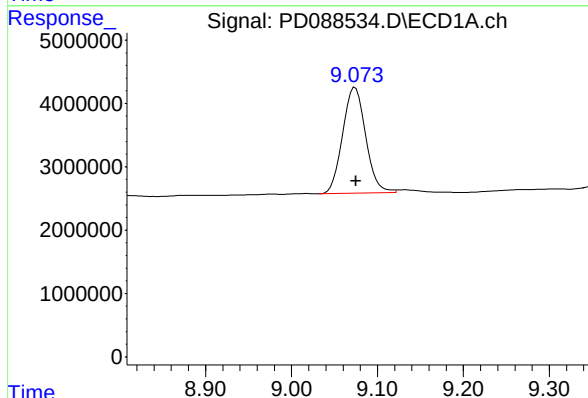

#28 Decachlorobiphenyl

R.T.: 9.074 min
Delta R.T.: 0.000 min
Response: 31037089
Conc: 9.38 ng/ml

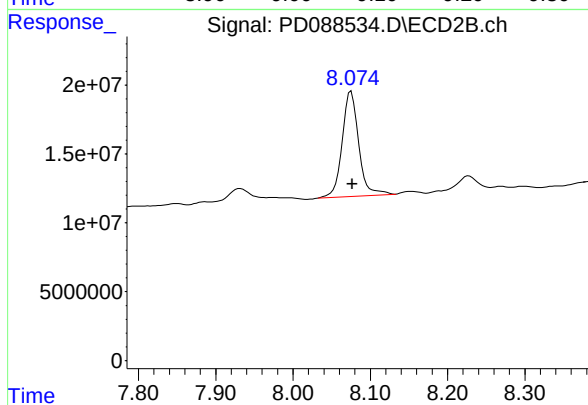

#28 Decachlorobiphenyl

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 112736984
Conc: 6.10 ng/ml