

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051421\
 Data File : PD062916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 13:30
 Operator : AR\AJ
 Sample : M2372-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CHRT-27051

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:20:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 16:02:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.970	9098584	73353451	10.232	6.336m#
28)	SA Decachlor...	8.198	9.026	18703484	173.0E6	17.666	14.991

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051421\
Data File : PD062916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 13:30
Operator : AR\AJ
Sample : M2372-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CHRT-27051


Manual Integrations
APPROVED

Ankita
5/14/2021 2:20:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 16:02:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

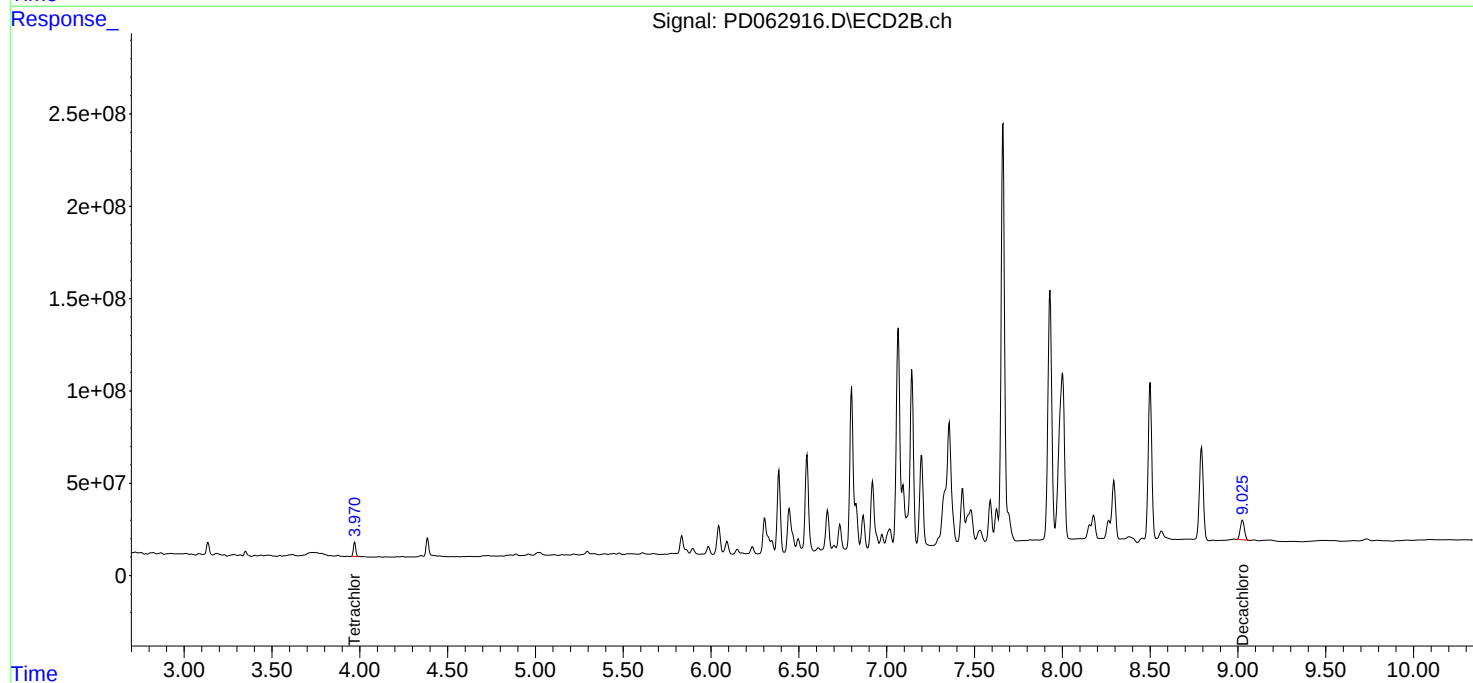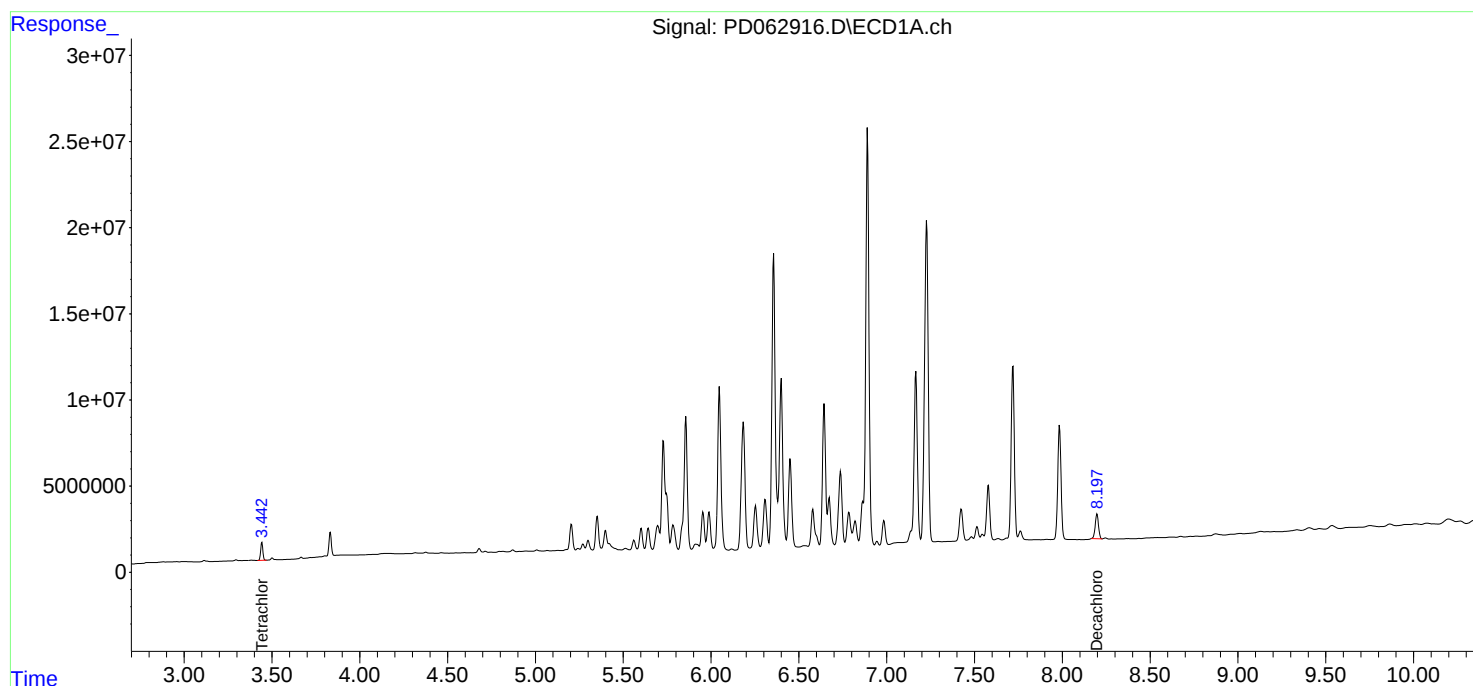

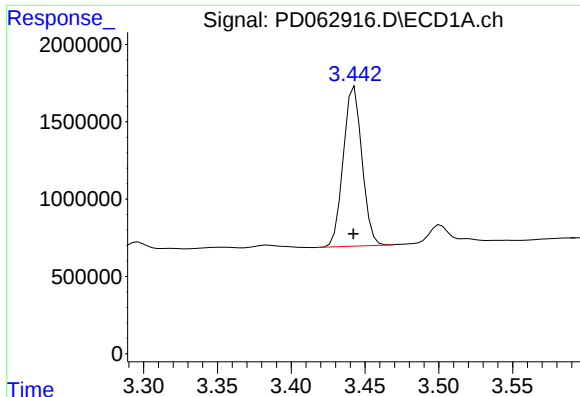


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 9098584
Conc: 10.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHRT-27051


Manual Integrations
APPROVED

Ankita
5/14/2021 2:20:08 PM

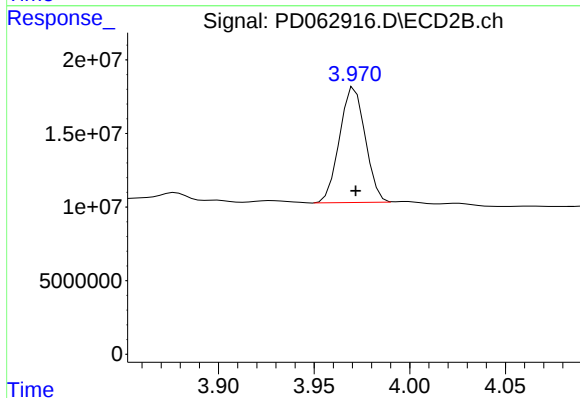


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.002 min
Response: 73353451
Conc: 6.34 ng/ml m

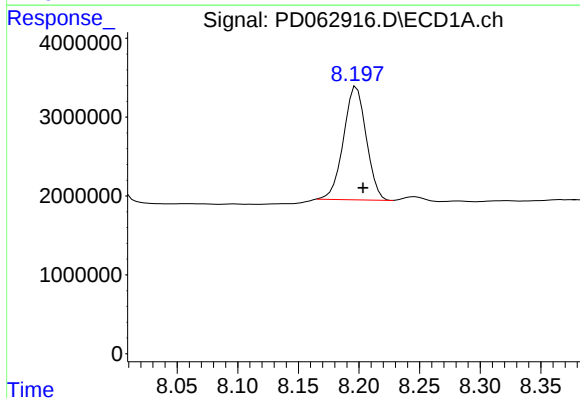

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: -0.005 min
Response: 18703484
Conc: 17.67 ng/ml

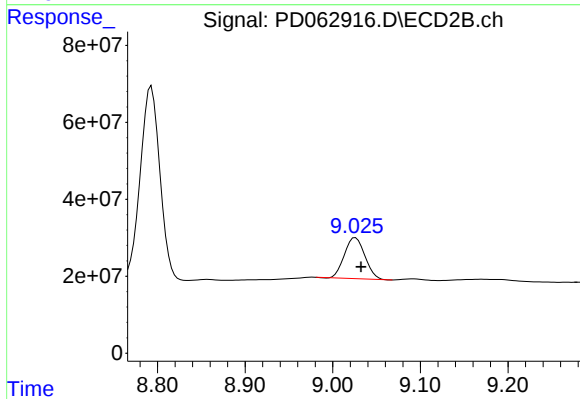

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.006 min
Response: 172977347
Conc: 14.99 ng/ml