

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051422\
 Data File : PD069620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 16:49
 Operator : AR\AJ
 Sample : N2714-03MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2X5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/19/2022
 Supervised By : mohammad ahmed 05/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 05:21:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.170	15428990	185.8E6	12.692	14.650
27)	SA Decachlor...	8.194	9.363	27865129	156.6E6	22.465	21.443
Target Compounds							
2)	A alpha-BHC	3.882	4.567	80345699	670.7E6	47.103	36.727
3)	MA gamma-BHC...	4.165	4.857	79325758	659.0E6	47.375	40.473
4)	MA Heptachlor	4.462	5.384	79687737	671.7E6	49.254	42.454
5)	MB Aldrin	4.709	5.696	80567447	660.2E6	54.905	45.998
6)	B beta-BHC	4.415	5.021	34532099	294.5E6	48.409	43.223
7)	B delta-BHC	4.619	5.245	18054644	147.5E6	11.962	13.018m
8)	B Heptachlo...	5.153	6.084	74764314	572.0E6	53.830	53.046
9)	A Endosulfan I	5.491	6.447	67274152	512.3E6	48.914	40.543
10)	B trans-Chl...	5.378	6.321	76305163	583.3E6	53.701	44.423
11)	B cis-Chlor...	5.437	6.396	73029858	551.8E6	52.421	43.292
12)	B 4,4'-DDE	5.602	6.546	151.2E6	1096.5E6	116.120	94.904
13)	MA Dieldrin	5.734	6.706	159.3E6	1135.2E6	107.456	89.168
14)	MA Endrin	5.992	6.925	136.8E6	906.7E6	105.035	89.654
15)	B Endosulfa...	6.266	7.130	133.4E6	899.2E6	114.398	93.976
16)	A 4,4'-DDD	6.119	7.037	121.8E6	868.1E6	103.945	87.709
17)	MA 4,4'-DDT	6.359	7.340	123.2E6	836.4E6	105.328	87.431
18)	B Endrin al...	6.436	7.255	107.9E6	725.8E6	103.813	87.883
19)	B Endosulfa...	6.648	7.480	103.5E6	680.2E6	84.439	72.707
20)	A Methoxychlor	6.909	7.793	323.8E6	1865.4E6	492.958	423.156
21)	B Endrin ke...	7.141	7.954	156.1E6	907.9E6	114.570	94.922

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051422\
Data File : PD069620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 16:49
Operator : AR\AJ
Sample : N2714-03MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 05:21:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

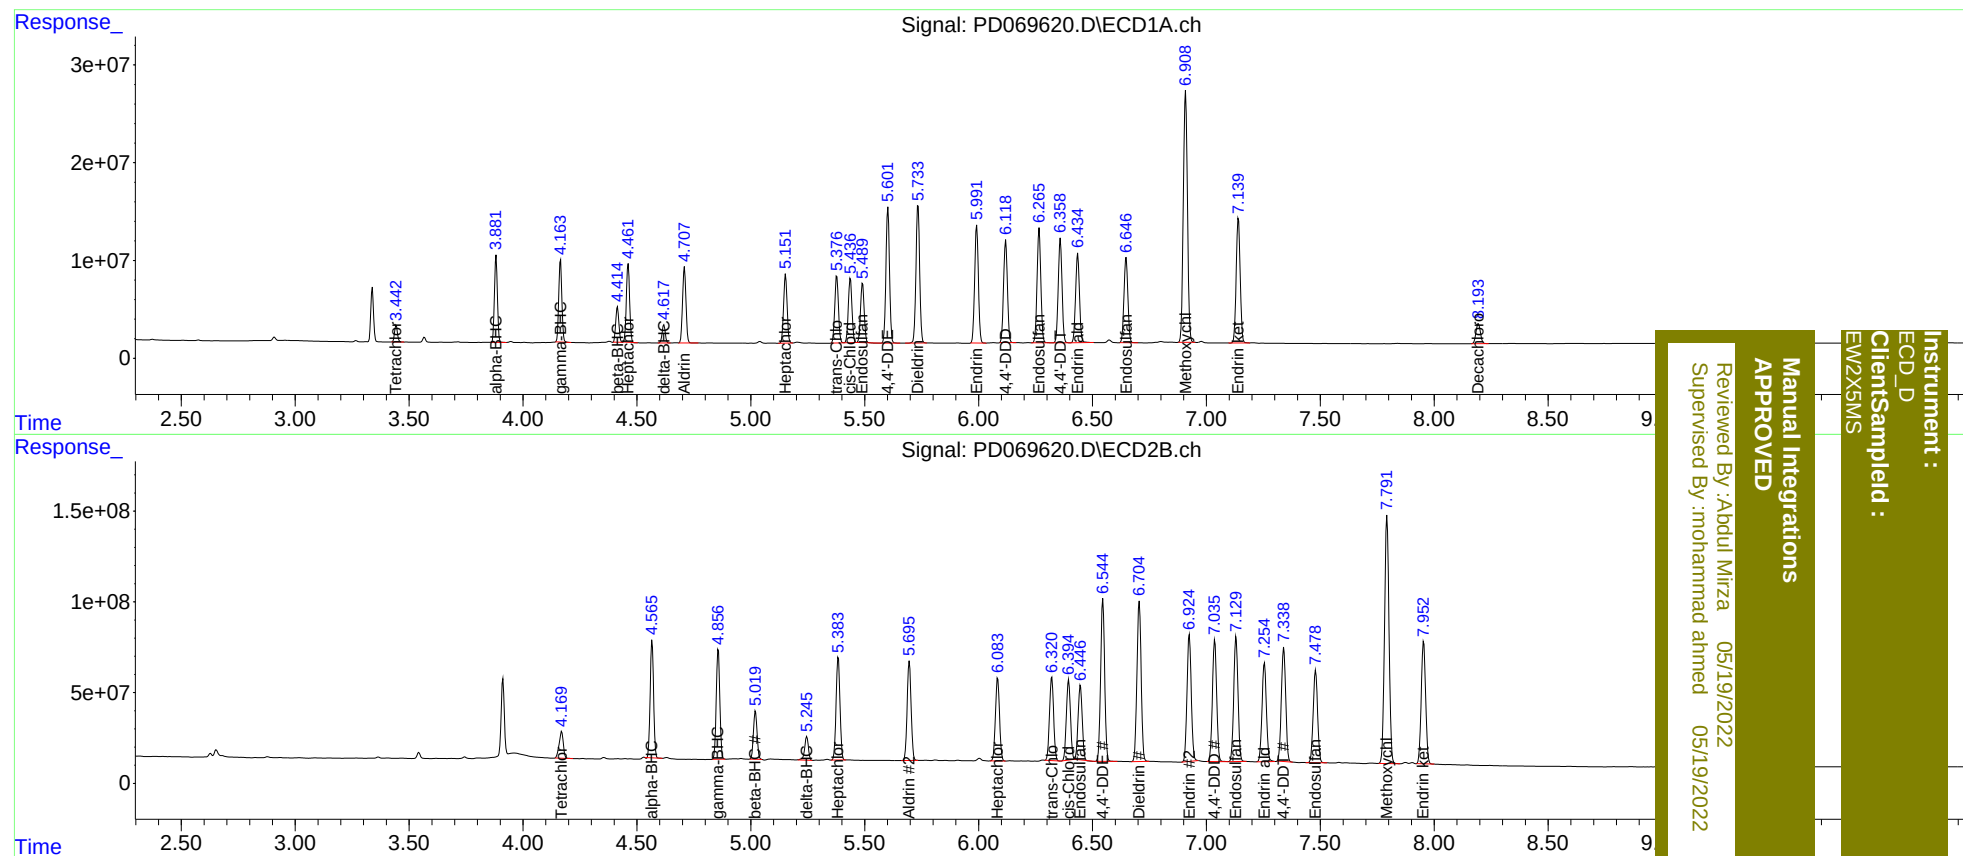

Reviewed By: Abdul Mirza 05/19/2022
Supervised By: mohammad ahmed 05/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW2X5MS