

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051521\
 Data File : PD062931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2021 11:05
 Operator : AR\AJ
 Sample : M2250-01
 Misc : TOX MDL 100 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2021-05

Manual Integrations
 APPROVED

Ankita
 5/17/2021 5:12:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 00:49:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	3.971	18081586	210.4E6	18.886m	17.324
27)	SA Decachlor...	8.205	9.029	43619582	395.1E6	40.637	36.199
Target Compounds							
22)	Toxaphene-1	5.703	6.356	777296	7363765	104.274m	110.830
23)	Toxaphene-2	5.865	6.645	650169	7757465	88.343	93.150
24)	Toxaphene-3	6.187	7.053	709188	10305221	86.306m	93.475
25)	Toxaphene-4	6.307	7.129	1669578	29099511	86.690	91.396
26)	Toxaphene-5	7.042	7.628	3032344	12392563	141.254	91.864 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051521\
Data File : PD062931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2021 11:05
Operator : AR\AJ
Sample : M2250-01
Misc : TOX MDL 100 PPB
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 00:49:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

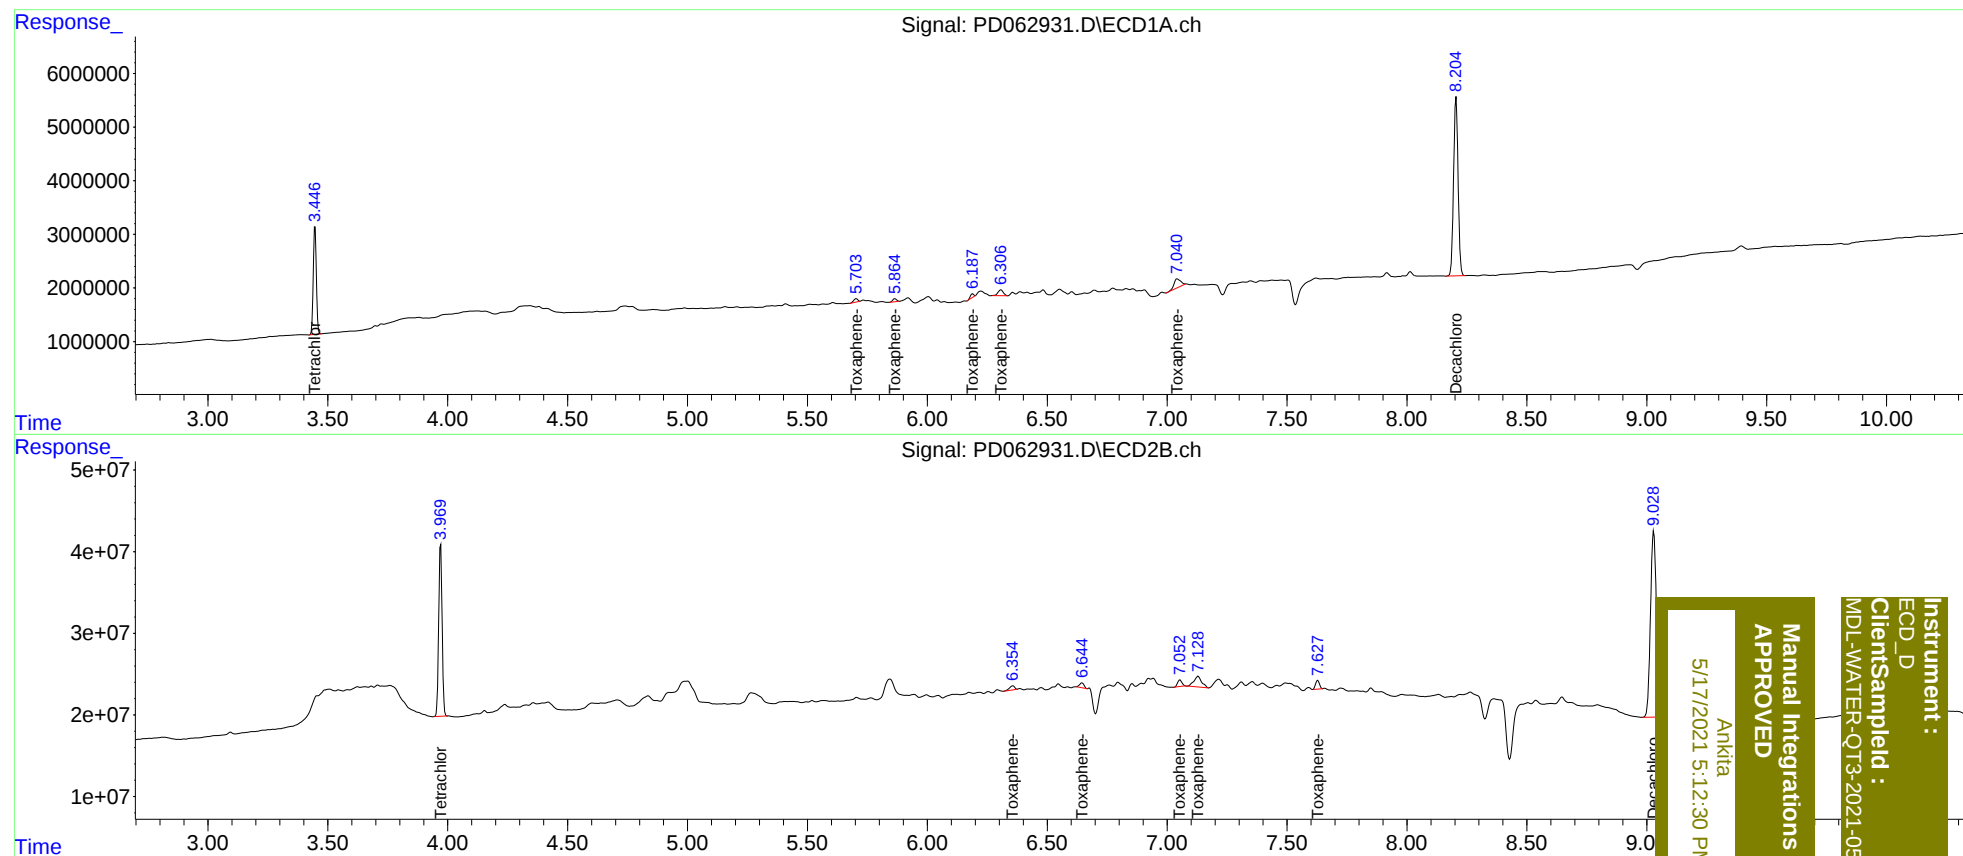

Manual Integrations
APPROVED

5/17/2021 5:12:30 PM
Ankita

Instrument :
ECD_D
Client Sampled :
MDL-WATER-QT3-2021-05