

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051521\
 Data File : PD062941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2021 13:52
 Operator : AR\AJ
 Sample : M2377-05MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG1Y7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:17:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	17746091	208.0E6	18.536	17.132
27)	SA Decachlor...	8.198	9.025	30981271	311.7E6	28.863	28.555
Target Compounds							
2)	A alpha-BHC	3.877	4.358	71422878	821.7E6	51.013	43.451
3)	MA gamma-BHC...	4.160	4.643	68079908	771.3E6	50.964	44.650
4)	MA Heptachlor	4.461	5.150	64650718	748.7E6	50.350	43.019
5)	MB Aldrin	4.709	5.455	61220022	727.5E6	46.999	42.056
6)	B beta-BHC	4.411	4.813	29091356	310.9E6	46.857	40.721
7)	B delta-BHC	4.615	5.029	68084835	684.4E6	50.037	36.891 #
8)	B Heptachlo...	5.152	5.840	58964504	638.5E6	48.116	39.812
9)	A Endosulfan I	5.491	6.197	54624851	648.1E6	48.851	44.186
10)	B trans-Chl...	5.379	6.074	59277378	691.2E6	47.283	42.204
11)	B cis-Chlor...	5.437	6.147	58179976	672.7E6	47.380	43.340
12)	B 4,4'-DDE	5.601	6.304	121.3E6	1361.8E6	98.044	86.905
13)	MA Dieldrin	5.734	6.454	126.4E6	1395.1E6	100.261	89.971
14)	MA Endrin	5.992	6.671	114.3E6	1190.6E6	107.987	95.468
15)	B Endosulfa...	6.266	6.880	106.8E6	1165.7E6	102.981	93.146
16)	A 4,4'-DDD	6.119	6.794	101.8E6	1148.0E6	102.199	92.367
17)	MA 4,4'-DDT	6.359	7.092	106.5E6	1155.5E6	113.697	97.321
18)	B Endrin al...	6.434	7.004	89717790	962.3E6	100.553	88.207
19)	B Endosulfa...	6.648	7.227	101.2E6	1150.3E6	101.192	90.136
20)	A Methoxychlor	6.906	7.551	284.0E6	2564.3E6	532.239	452.395
21)	B Endrin ke...	7.140	7.697	126.6E6	1110.9E6	108.014	90.270

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051521\
Data File : PD062941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2021 13:52
Operator : AR\AJ
Sample : M2377-05MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:17:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

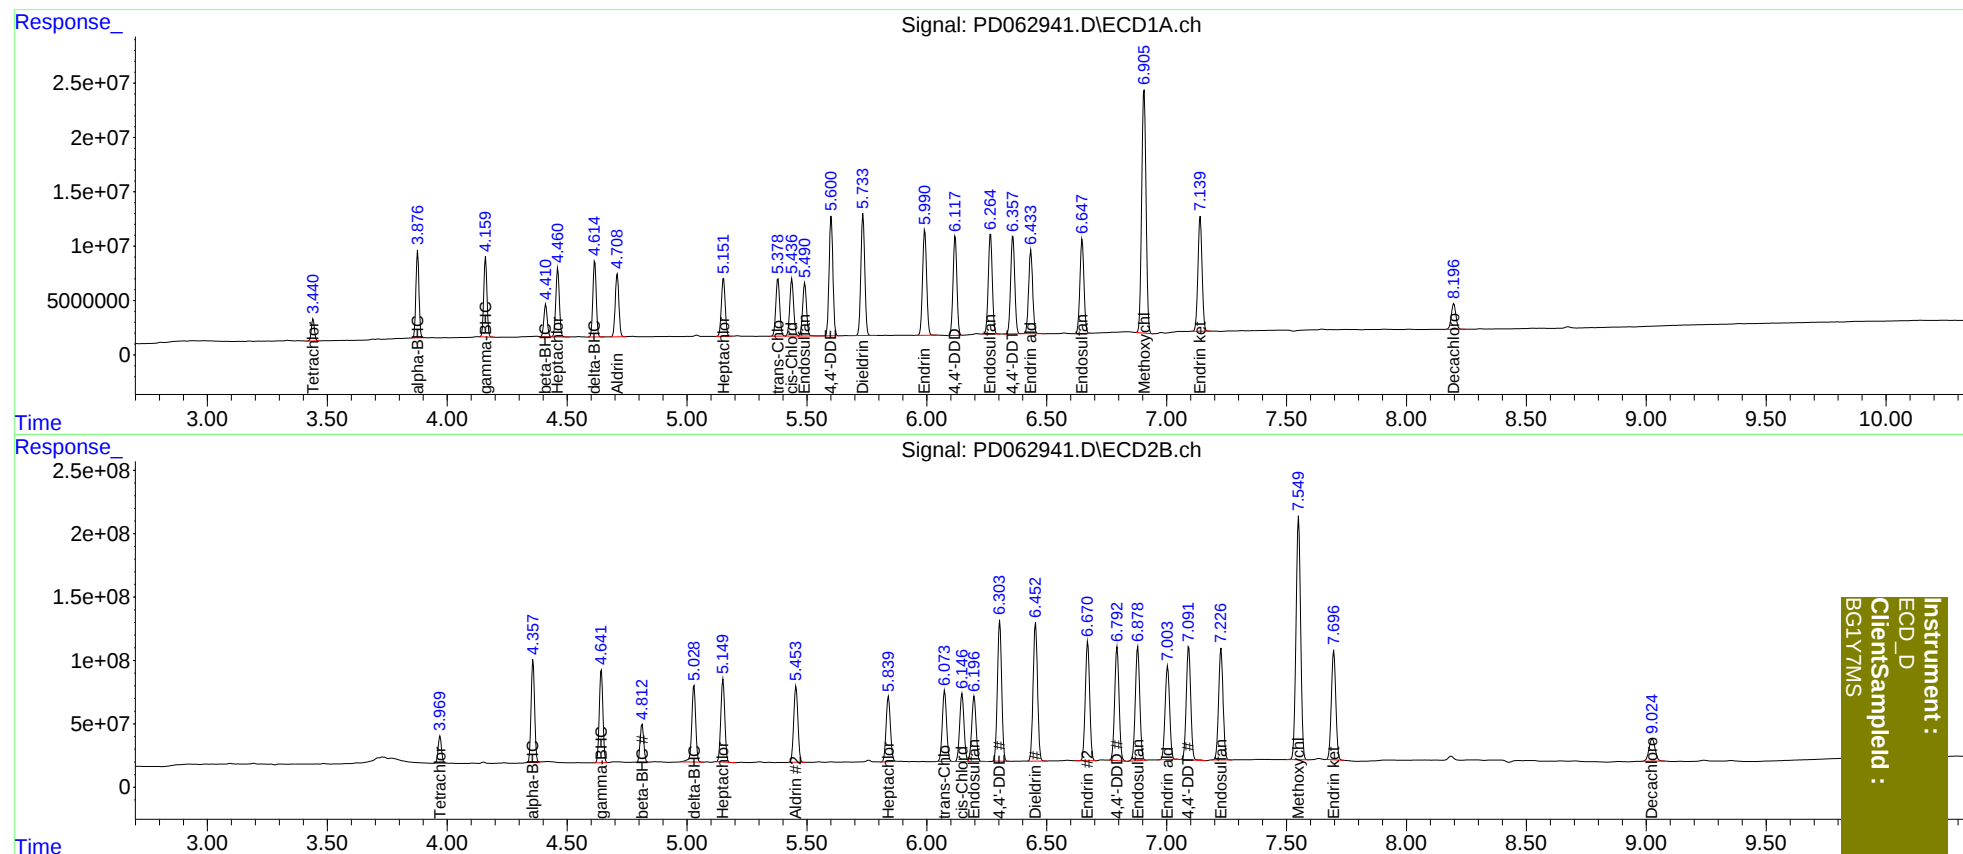

Instrument :
ECD_D
Client Sampled :
BG1YTMS