

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051522\
 Data File : PD069634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 16:10
 Operator : AR\AJ
 Sample : N2788-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:21:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.170	13026534	72422041	11.735m	6.755m#
28)	SA Decachlor...	8.198	9.363	13089259	64670800	10.483m	9.882m
Target Compounds							
12)	B 4,4'-DDE	5.609	6.542	8021033	34164324	6.339m	3.163m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051522\
Data File : PD069634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 16:10
Operator : AR\AJ
Sample : N2788-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:21:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

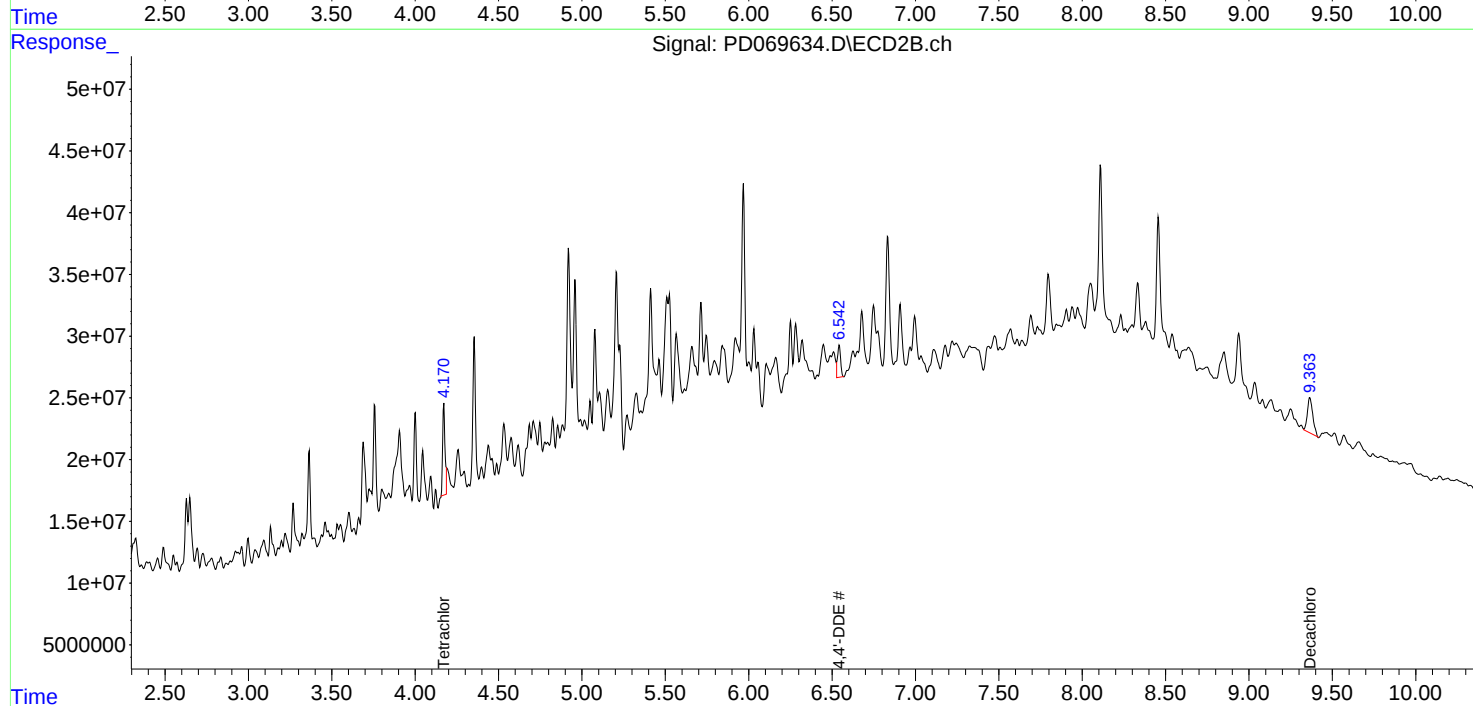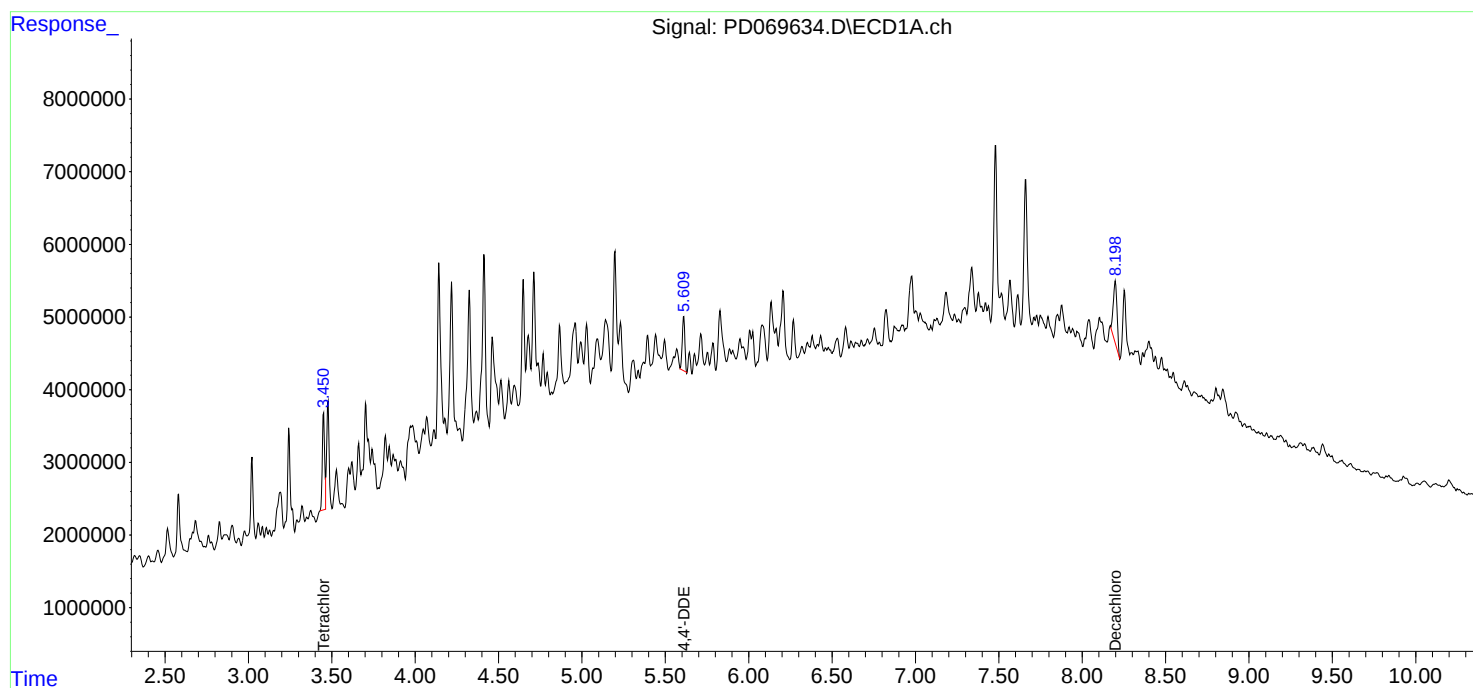


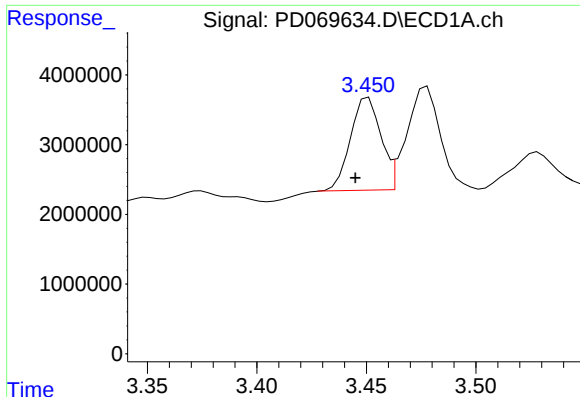

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.005 min
Response: 13026534
Conc: 11.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

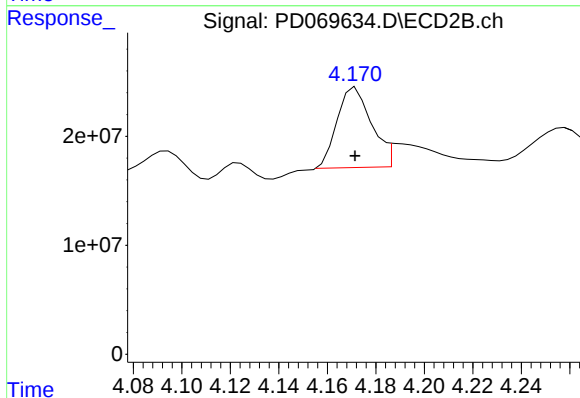


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: -0.001 min
Response: 72422041
Conc: 6.75 ng/ml m

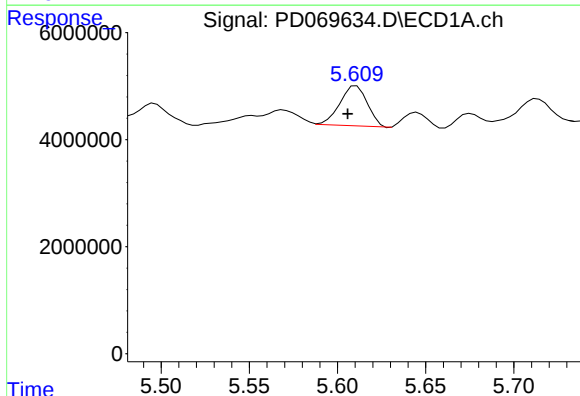


#12 4,4'-DDE

R.T.: 5.609 min
Delta R.T.: 0.004 min
Response: 8021033
Conc: 6.34 ng/ml m

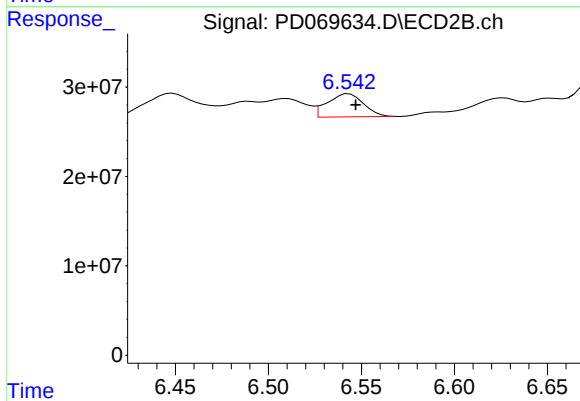

#12 4,4'-DDE


R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 34164324
Conc: 3.16 ng/ml m

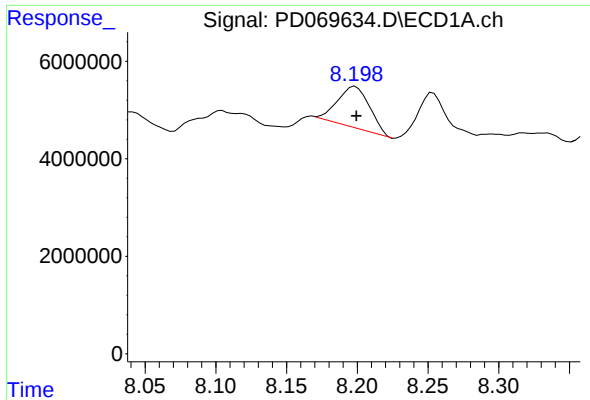

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: -0.002 min
Response: 13089259
Conc: 10.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

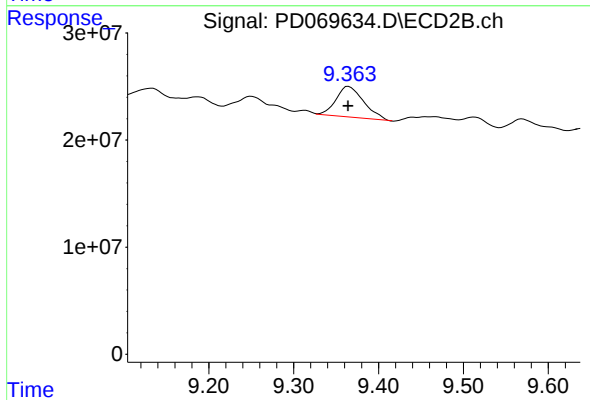

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: -0.001 min
Response: 64670800
Conc: 9.88 ng/ml m