

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051523\
 Data File : PD075483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2023 16:13
 Operator : AR\AJ
 Sample : 02612-03MSD
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JREG4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/16/2023
 Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 22:09:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	22253700	11287432	9.757	10.702
27)	SA Decachlor...	9.090	7.916	32741707	14357988	13.230	15.204
Target Compounds							
2)	A alpha-BHC	4.003	3.272	132.5E6	60256744	34.462m	38.900
3)	MA gamma-BHC...	4.338	3.602	117.4E6	54568887	32.659	37.123
4)	MA Heptachlor	4.930	3.942	118.5E6	53181024	31.788	36.396
5)	MB Aldrin	5.272	4.223	127.9E6	56286956	35.063	37.952
6)	B beta-BHC	4.534	3.899	51896121	24289209	31.615	33.357
7)	B delta-BHC	4.782	4.129	95856267	43246308	28.359	27.369
8)	B Heptachlo...	5.699	4.725	111.0E6	48012183	32.738	34.423
9)	A Endosulfan I	6.086	5.096	101.5E6	44251597	33.652	36.871
10)	B trans-Chl...	5.956	4.976	106.8E6	48010348	32.603	35.184
11)	B cis-Chlor...	6.036	5.040	110.4E6	48707648	32.388	34.901
12)	B 4,4'-DDE	6.208	5.229	218.1E6	92296060	66.776	71.794
13)	MA Dieldrin	6.362	5.360	237.7E6	101.6E6	69.512	74.443
14)	MA Endrin	6.593	5.636	193.3E6	86691562	66.832	71.274
15)	B Endosulfa...	6.811	5.931	206.1E6	84662775	64.014	66.170
16)	A 4,4'-DDD	6.726	5.784	176.3E6	76067963	72.963	76.729
17)	MA 4,4'-DDT	7.041	6.035	179.5E6	73338797	70.735	72.766
18)	B Endrin al...	6.942	6.110	141.9E6	62681069	59.972	61.726
19)	B Endosulfa...	7.177	6.332	171.2E6	76287442	62.248	65.594
20)	A Methoxychlor	7.517	6.611	487.6E6	194.4E6	331.951	339.356
21)	B Endrin ke...	7.663	6.839	205.8E6	93368493	67.884	70.808

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051523\
Data File : PD075483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2023 16:13
Operator : AR\AJ
Sample : 02612-03MSD
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 22:09:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

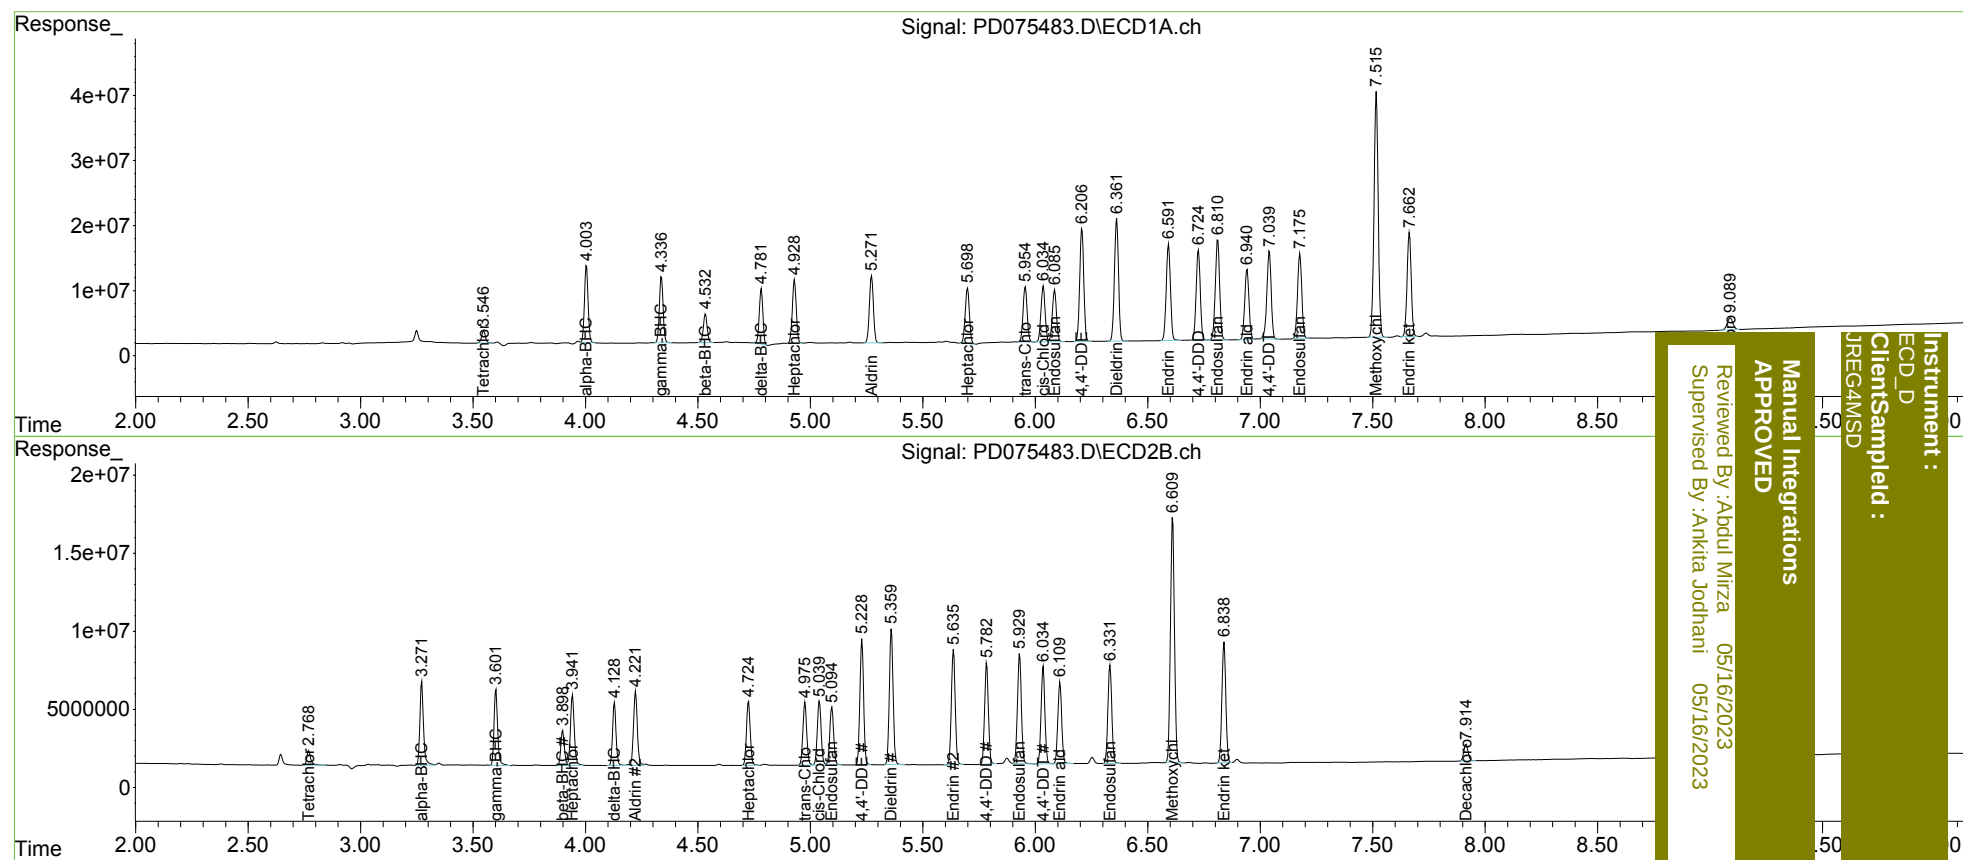

Instrument :
ECD_D
ClientSampled :
JREG4MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 05/16/2023
Supervised By: Ankita Jodhani 05/16/2023