

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051524\
 Data File : PD082815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 10:17
 Operator : AR\AJ
 Sample : PB160843BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB160843BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/17/2024
 Supervised By : Ankita Jodhani 05/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 05:47:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
 Quant Title : GC Extractables
 QLast Update : Mon May 13 15:39:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.776	32425642	79457223	20.944m	20.049
28) SA Decachlor...	9.122	7.906	42253076	84366212	21.159	21.826

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051524\
Data File : PD082815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 10:17
Operator : AR\AJ
Sample : PB160843BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PB160843BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/17/2024
Supervised By : Ankita Jodhani 05/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 05:47:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 15:39:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

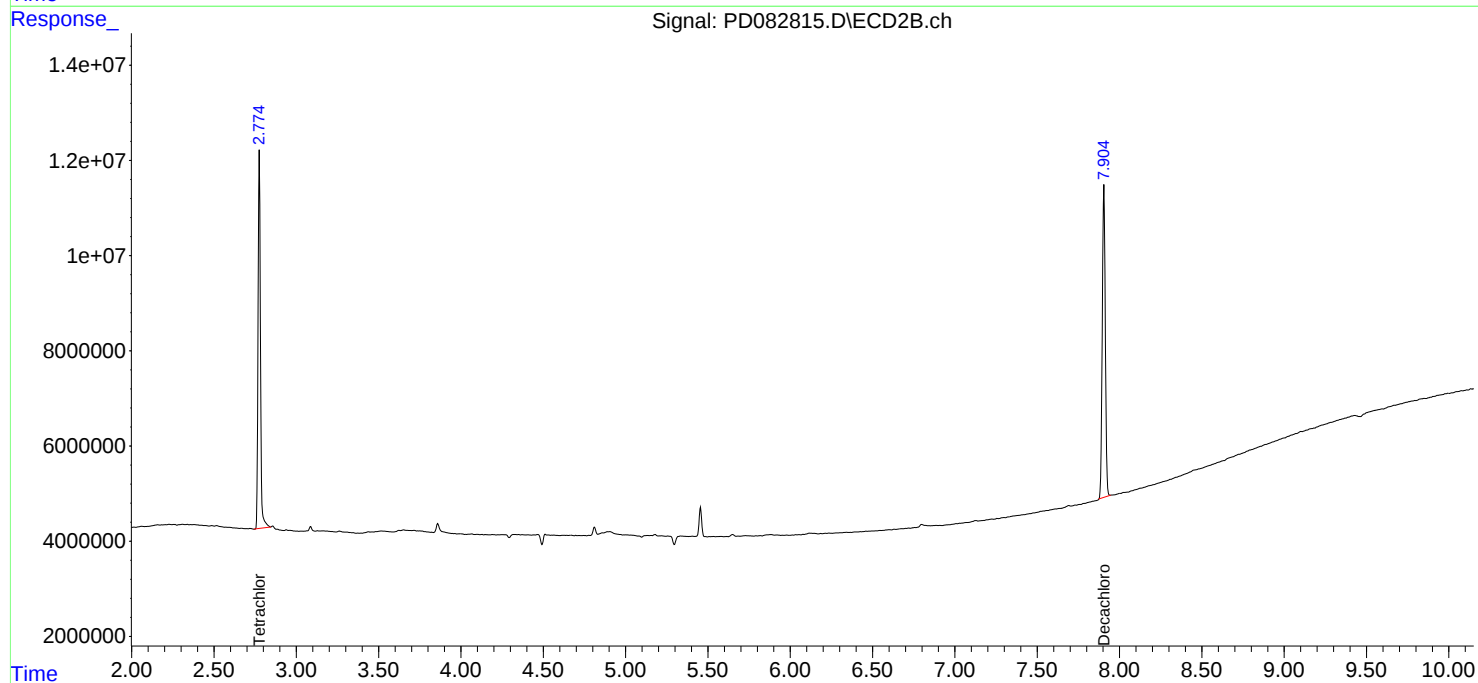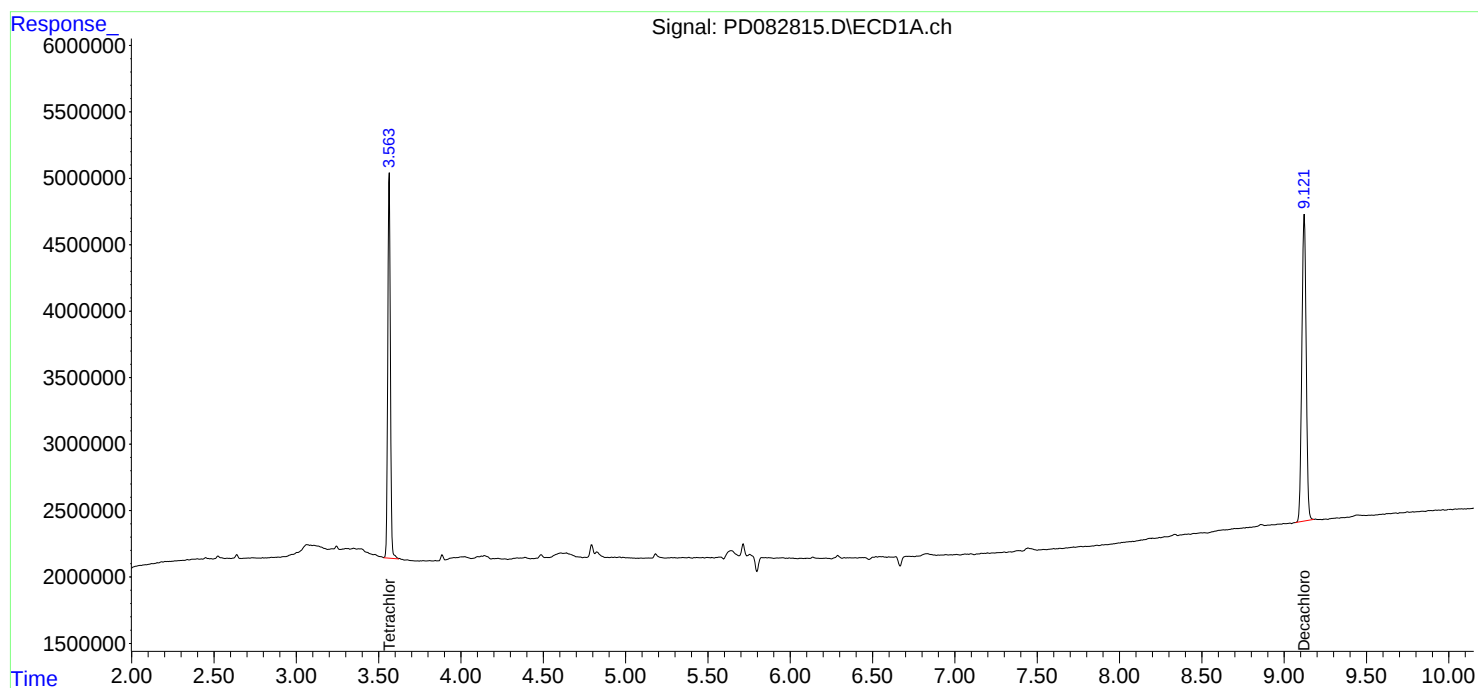

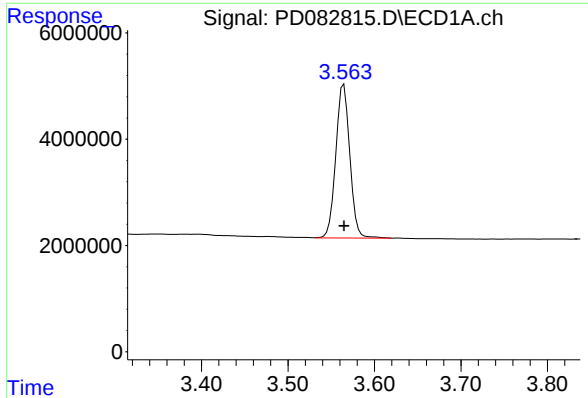

#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.002 min
Response: 32425642
Conc: 20.94 ng/ml

Instrument :

ECD_D


ClientSampleId :

PB160843BL

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 05/17/2024
Supervised By :Ankita Jodhani 05/17/2024

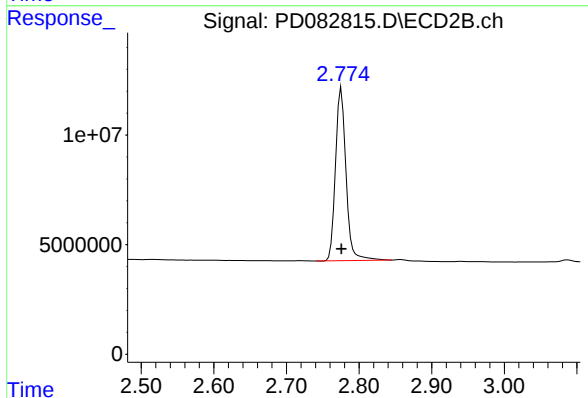


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 79457223
Conc: 20.05 ng/ml

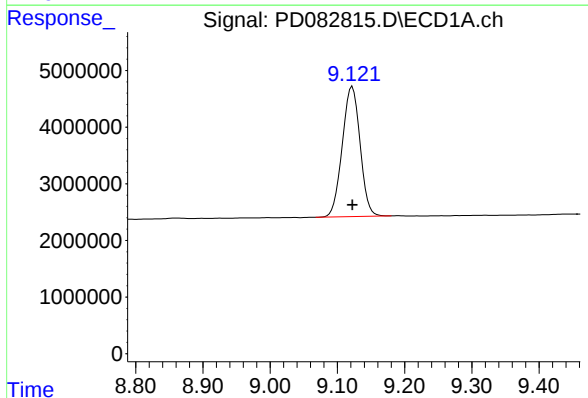

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.000 min
Response: 42253076
Conc: 21.16 ng/ml

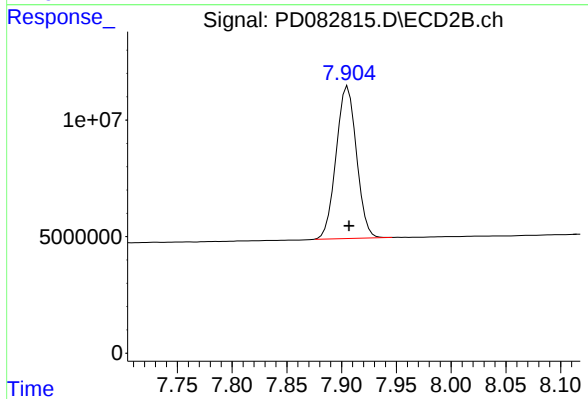

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.001 min
Response: 84366212
Conc: 21.83 ng/ml