

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051623\
 Data File : PD075530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 19:11
 Operator : AR\AJ
 Sample : 02689-08MSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JREM0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/17/2023
 Supervised By : Ankita Jodhani 05/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 21:48:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.769	12373222	6677070	5.425m	6.331m
2)	SA Decachlor...	9.091	7.915	17762532	9215384	7.178m	9.758m#
Target Compounds							
2)	A alpha-BHC	4.005	3.273	176.5E6	74906694	45.898	48.358
3)	MA gamma-BHC...	4.337	3.601	171.3E6	68734475	47.654m	46.760m
4)	MA Heptachlor	4.930	3.942	164.6E6	92850846	44.152	63.544 #
5)	MB Aldrin	5.274	4.223	173.7E6	71549686	47.622	48.244
6)	B beta-BHC	4.534	3.899	64804364	29302578	39.479	40.243
7)	B delta-BHC	4.784	4.130	184.4E6	54837537	54.548	34.705 #
8)	B Heptachlo...	5.700	4.726	150.4E6	58754563	44.373	42.125
9)	A Endosulfan I	6.087	5.097	136.3E6	53406778	45.173	44.500
10)	B trans-Chl...	5.957	4.977	135.1E6	58368236	41.240	42.775
11)	B cis-Chlor...	6.037	5.041	143.6E6	60082192	42.135	43.052
12)	B 4,4'-DDE	6.209	5.230	289.2E6	113.2E6	88.557	88.089
13)	MA Dieldrin	6.363	5.362	317.2E6	130.9E6	92.757	95.953
14)	MA Endrin	6.594	5.638	263.8E6	111.6E6	91.222	91.719
15)	B Endosulfa...	6.813	5.932	269.4E6	103.7E6	83.668	81.077
16)	A 4,4'-DDD	6.728	5.786	244.7E6	94797313	101.273	95.622
17)	MA 4,4'-DDT	7.043	6.037	247.8E6	95799171	97.624	95.051
18)	B Endrin al...	6.944	6.111	183.2E6	72632772	77.425	71.526
19)	B Endosulfa...	7.179	6.335	224.3E6	96241552	81.559	82.751
20)	A Methoxychlor	7.518	6.613	644.7E6	240.1E6	438.924	419.209
21)	B Endrin ke...	7.666	6.842	293.1E6	112.3E6	96.678	85.196

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051623\
Data File : PD075530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 19:11
Operator : AR\AJ
Sample : 02689-08MSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 21:48:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

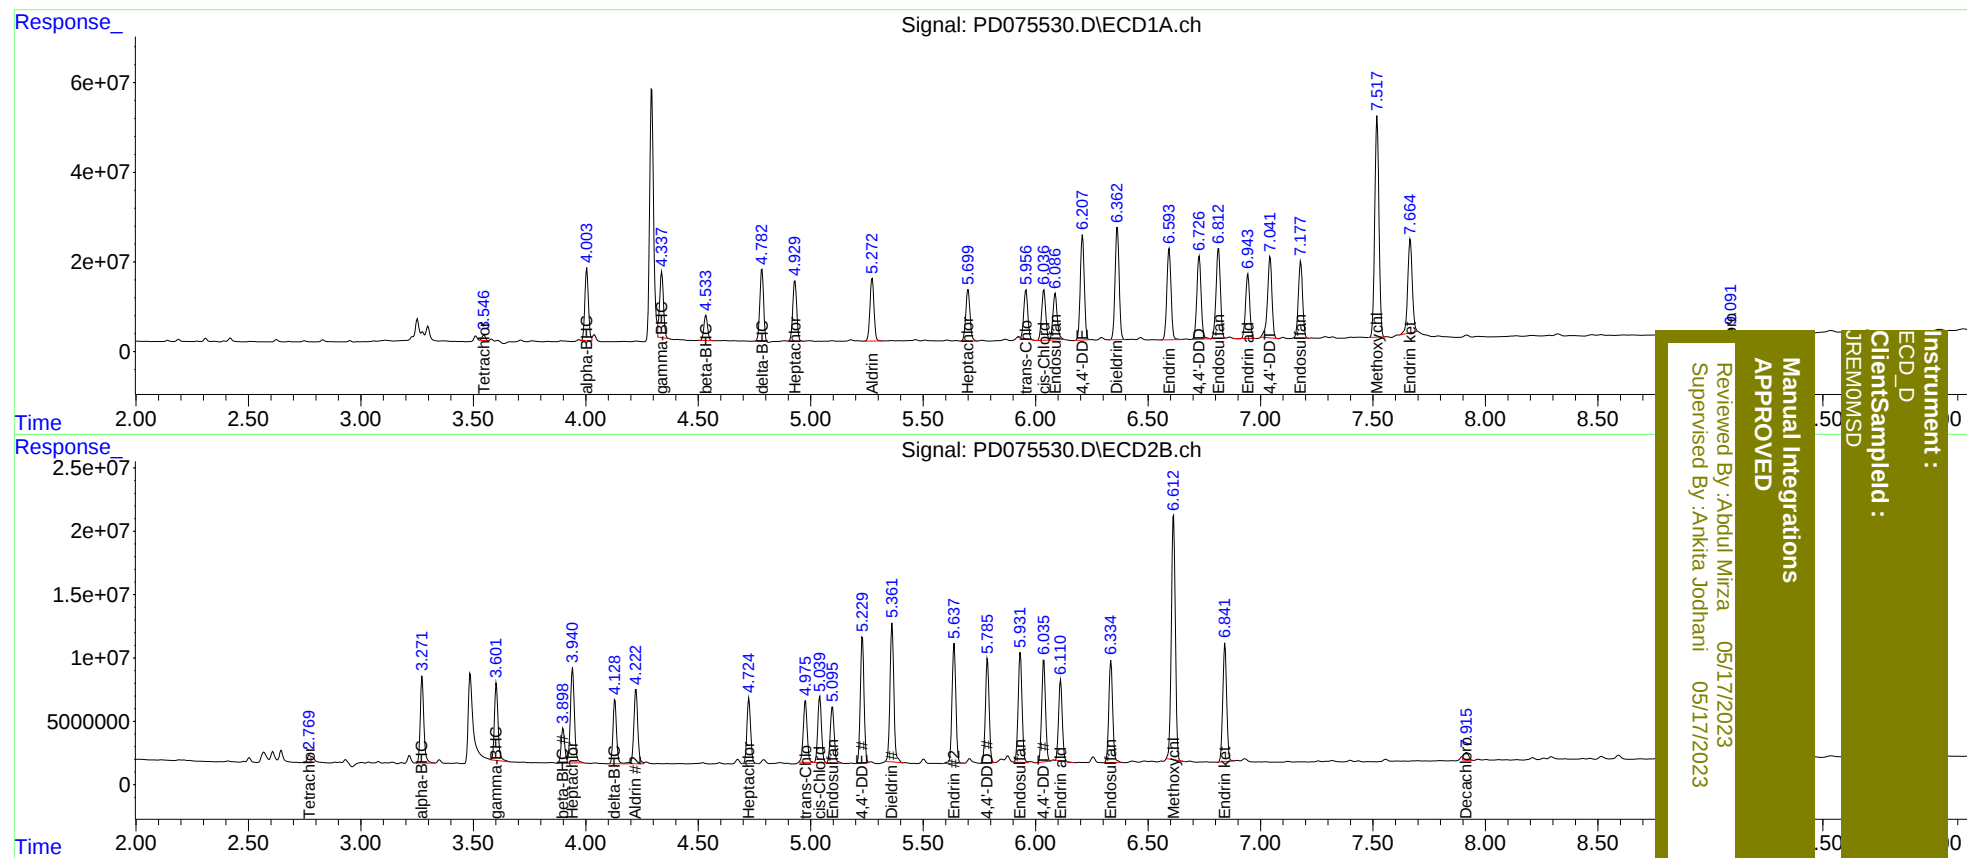

Instrument :
ECD_D
ClientSampled :
JREMOMSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/17/2023
Supervised By :Ankita Jodhani 05/17/2023