

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
 Data File : PD062991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2021 12:11
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 15:07:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Mon May 17 15:06:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	3.970	60699711	541.3E6	50.000	50.000
28)	SA Decachlor...	8.201	9.027	61159413	498.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.314	4.962	18273118	334.6E6	500.000	500.000
24)	Chlordane-2	4.815	5.430	22986248	243.7E6	500.000	500.000
25)	Chlordane-3	5.385	6.075	71815823	1025.1E6	500.000	500.000
26)	Chlordane-4	5.443	6.150	58996577	1176.1E6	500.000	500.000
27)	Chlordane-5	6.279	6.953	22964536	213.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
Data File : PD062991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2021 12:11
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 15:07:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Mon May 17 15:06:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

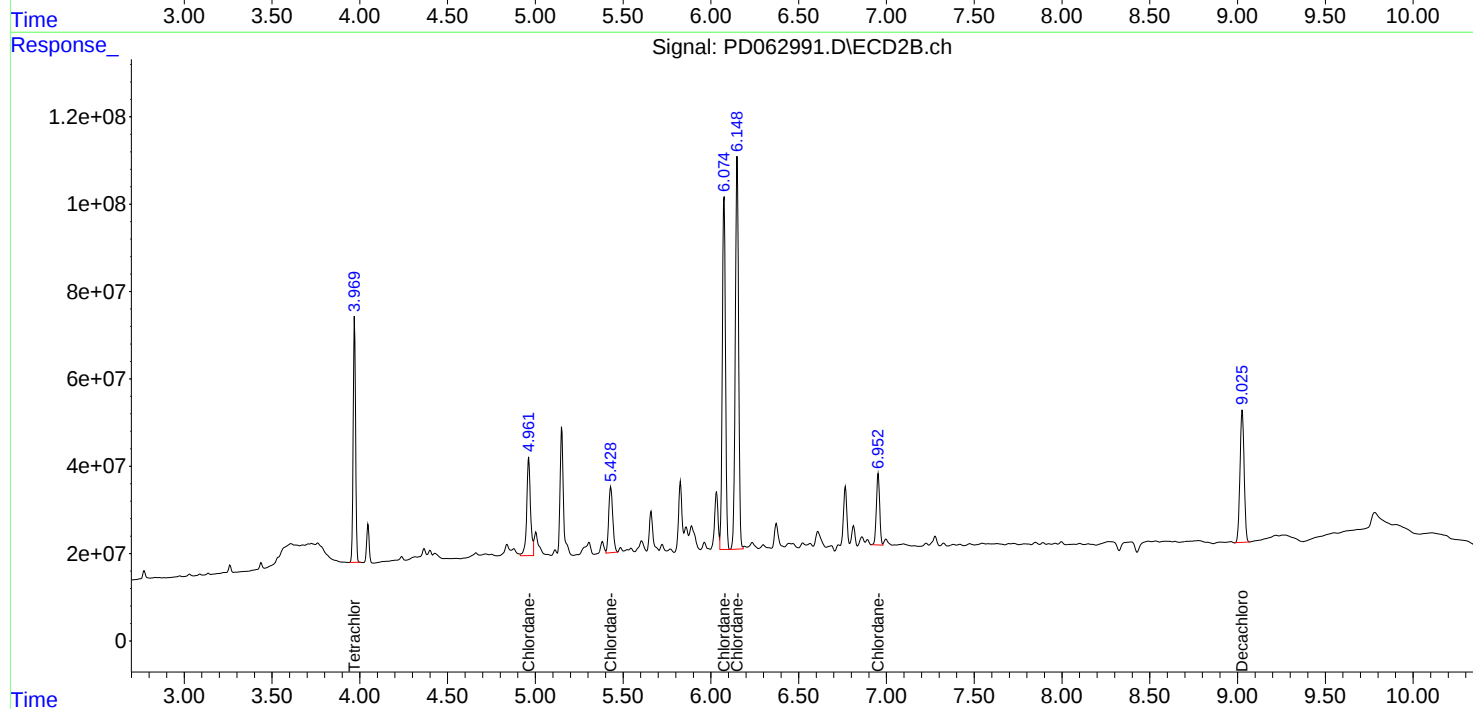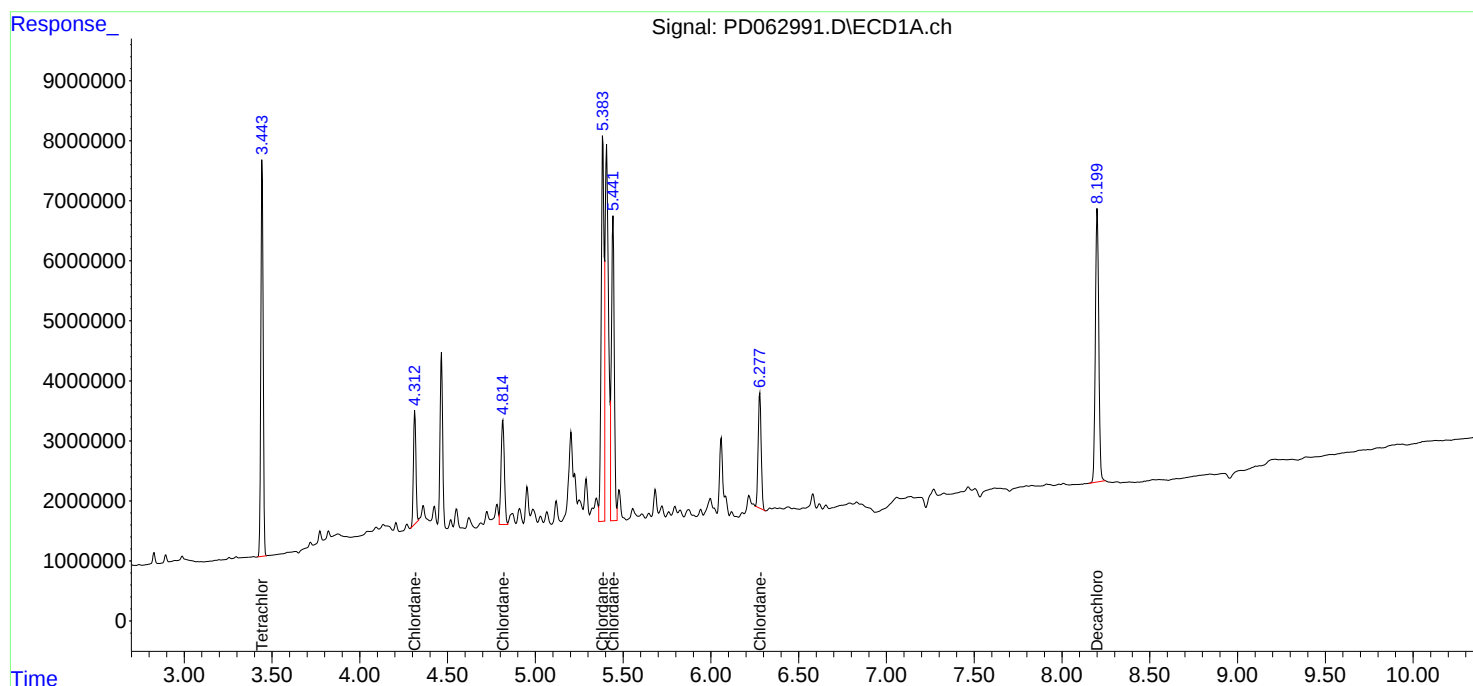


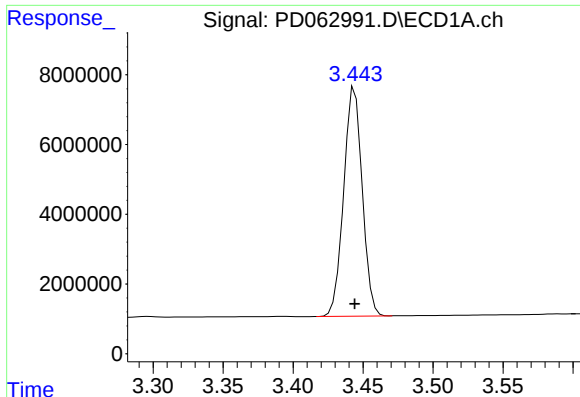

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 60699711
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

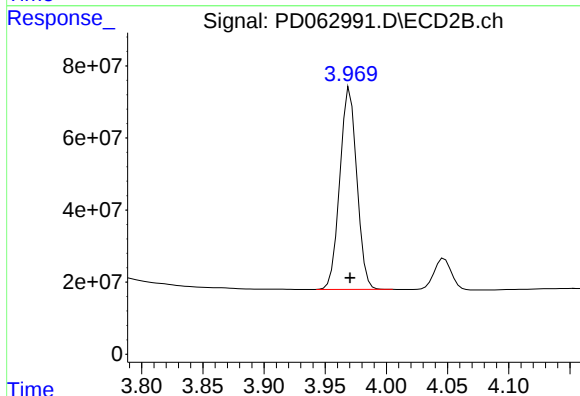


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 541328942
Conc: 50.00 ng/ml

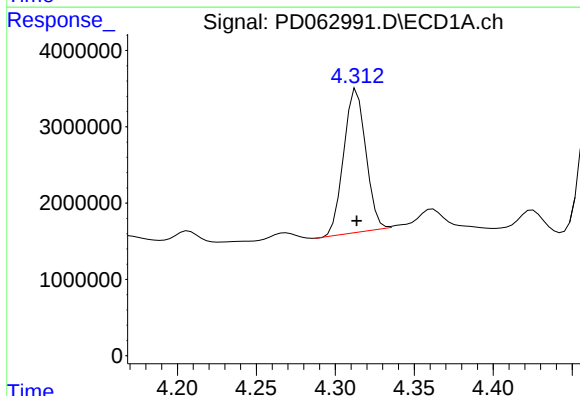


#23 Chlordane-1

R.T.: 4.314 min
Delta R.T.: 0.000 min
Response: 18273118
Conc: 500.00 ng/ml

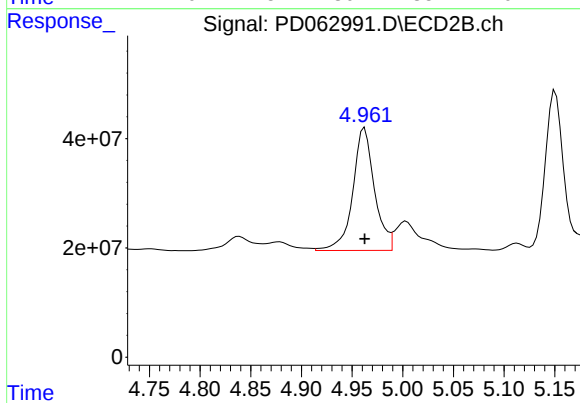

#23 Chlordane-1


R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 334635745
Conc: 500.00 ng/ml

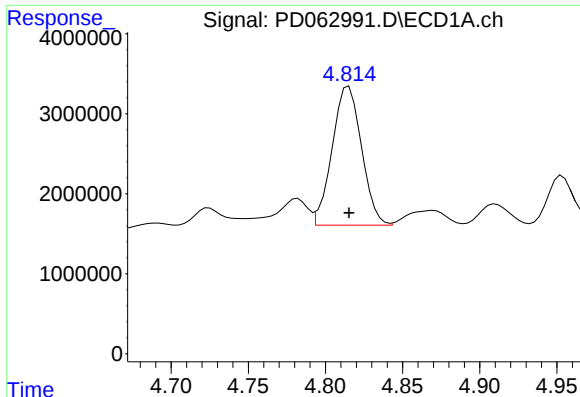

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.000 min
Response: 22986248
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

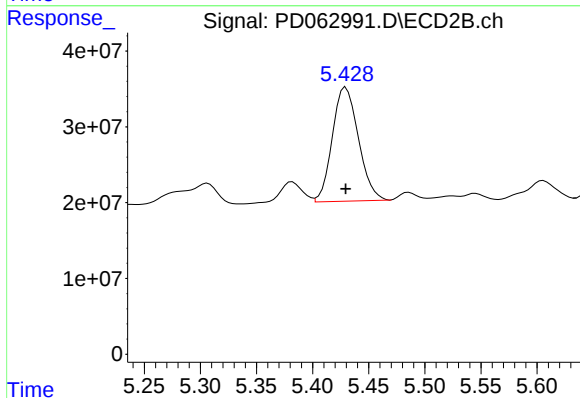


#24 Chlordane-2

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 243702362
Conc: 500.00 ng/ml

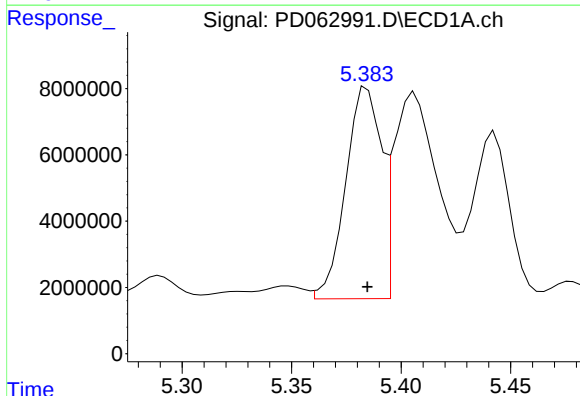


#25 Chlordane-3

R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 71815823
Conc: 500.00 ng/ml

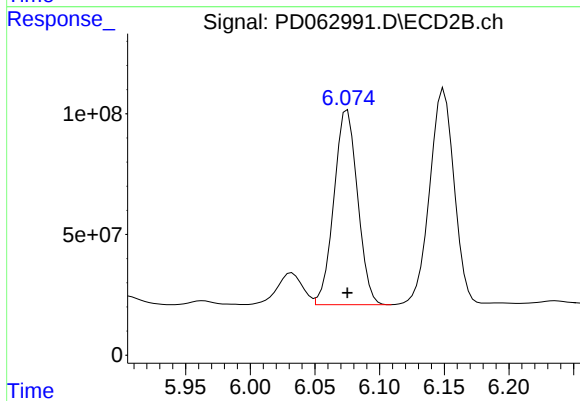

#25 Chlordane-3


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 1025105226
Conc: 500.00 ng/ml

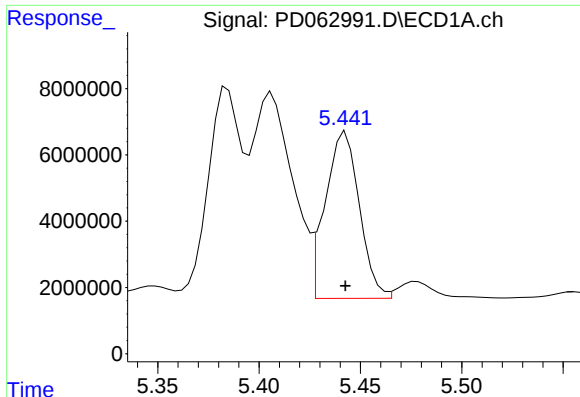

#26 Chlordane-4


R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 58996577
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

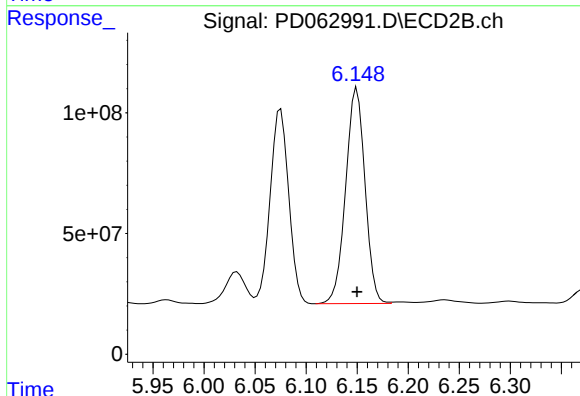


#26 Chlordane-4

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 1176144529
Conc: 500.00 ng/ml

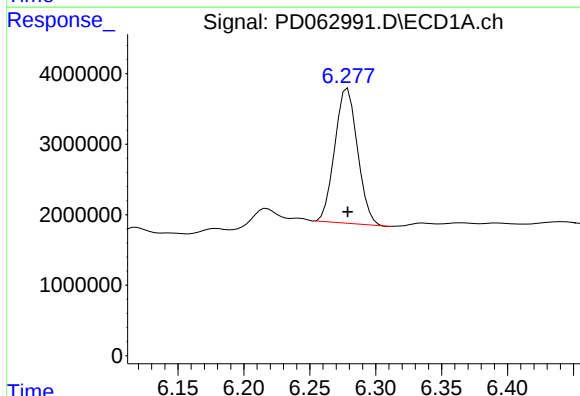


#27 Chlordane-5

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 22964536
Conc: 500.00 ng/ml

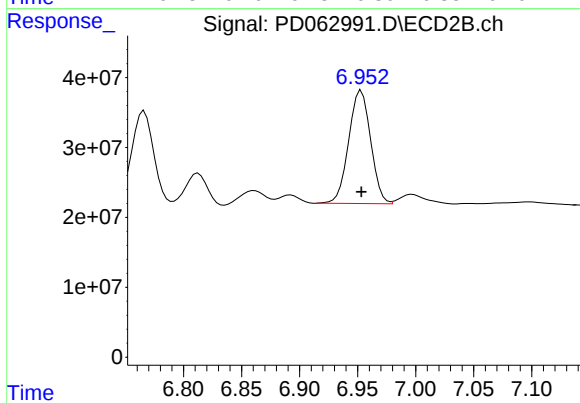

#27 Chlordane-5


R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 213216381
Conc: 500.00 ng/ml

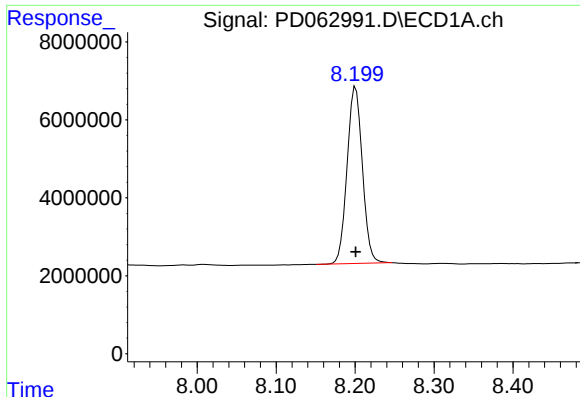

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 61159413
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

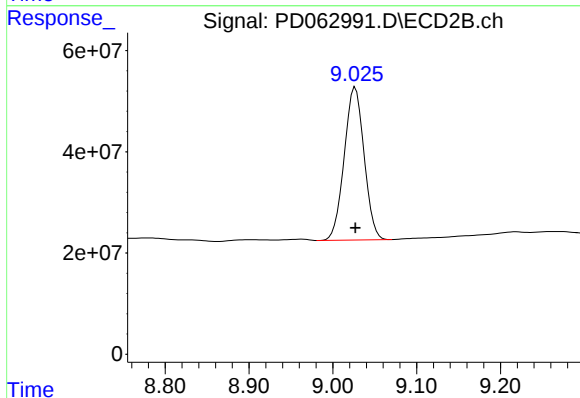

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.000 min
Response: 498044596
Conc: 50.00 ng/ml