

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
 Data File : PD063021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2021 19:12
 Operator : AR\AJ
 Sample : PB136391BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB136391BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 07:20:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	20631630	216.7E6	18.730	18.702
28)	SA Decachlor...	8.195	9.024	25947536	207.8E6	20.617	20.372
Target Compounds							
7)	B delta-BHC	0.000	5.002f	0 66863329	N.D.	4.786	#
8)	B Heptachlo...	0.000	5.851	0 7003558	N.D.	0.458	#
9)	A Endosulfan I	5.498	0.000	3826869	0	2.820	N.D. #
13)	MA Dieldrin	0.000	6.434f	0 2753488	N.D.	0.182	#
14)	MA Endrin	0.000	6.685	0 1312834	N.D.	0.103	#
16)	A 4,4'-DDD	0.000	6.809f	0 20612371	N.D.	1.699	#
17)	MA 4,4'-DDT	0.000	7.104	0 68611384	N.D.	6.085	#
18)	B Endrin al...	6.448	0.000	3550873	0	3.341	N.D. #
20)	A Methoxychlor	0.000	7.556	0 26009471	N.D.	4.534	#
21)	B Endrin ke...	0.000	7.707	0 76135546	N.D.	6.347	#
24)	Chlordane-2	0.000	5.401f	0 129051	N.D.	0.265	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
Data File : PD063021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2021 19:12
Operator : AR\AJ
Sample : PB136391BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB136391BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 07:20:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

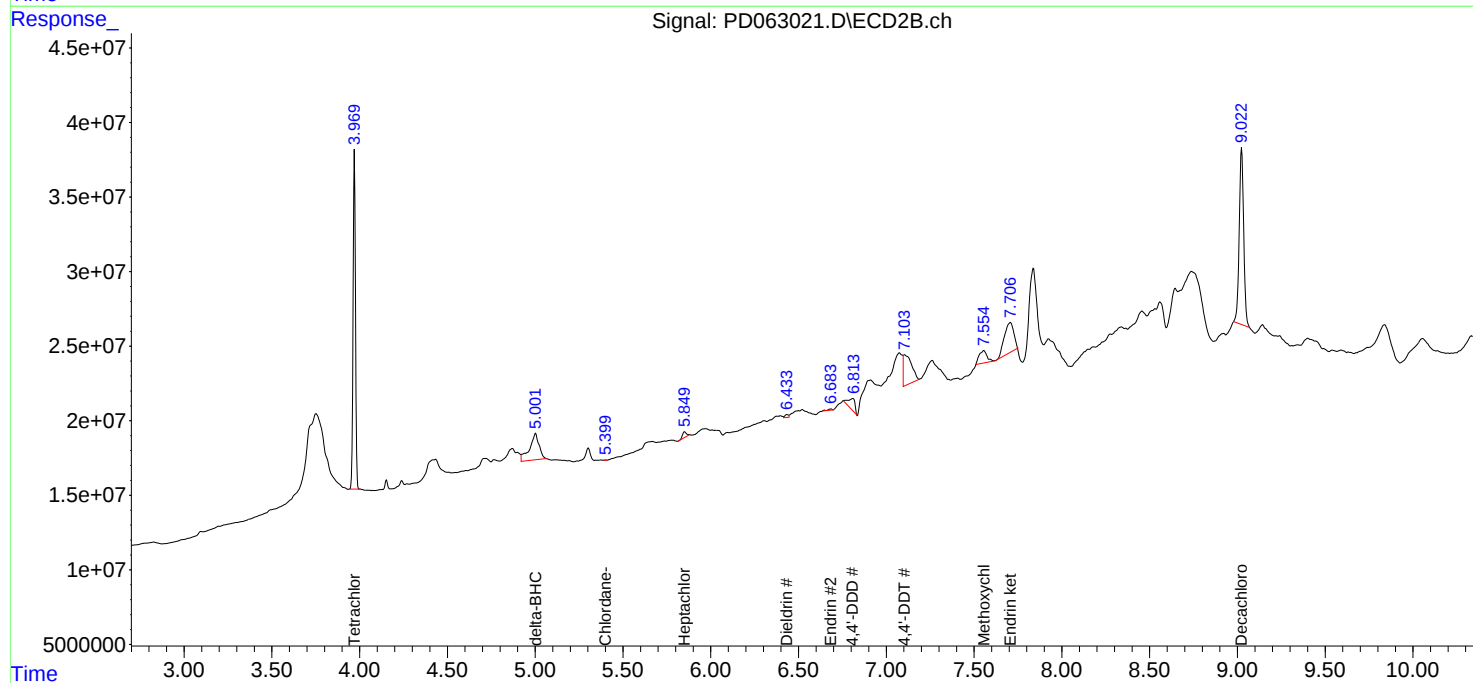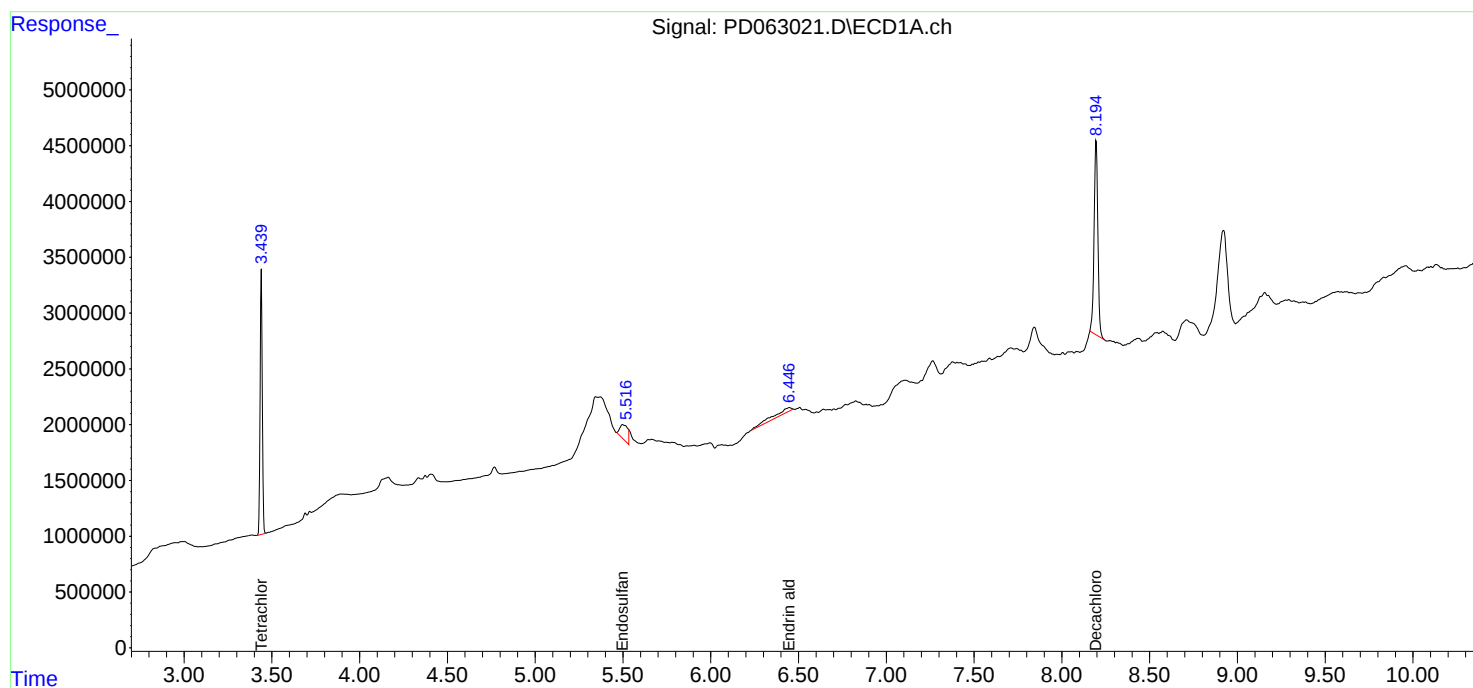


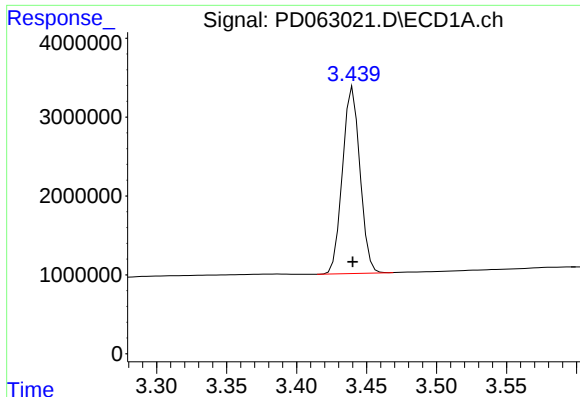

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 20631630
Conc: 18.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136391BL

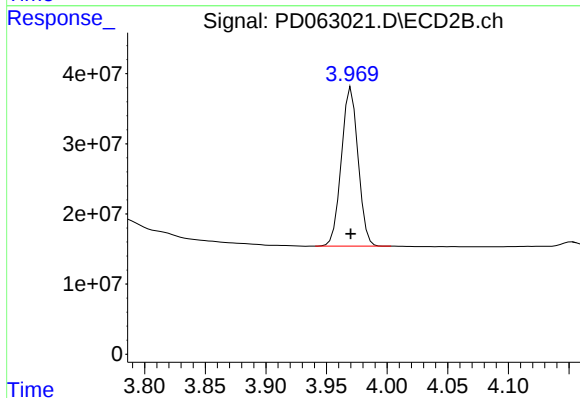


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 216717937
Conc: 18.70 ng/ml

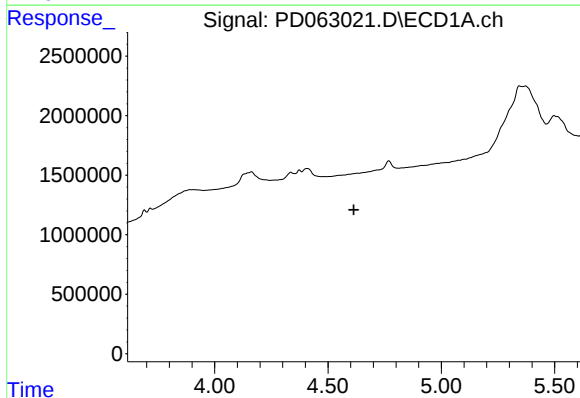


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.614 min
Response: 0
Conc: N.D.

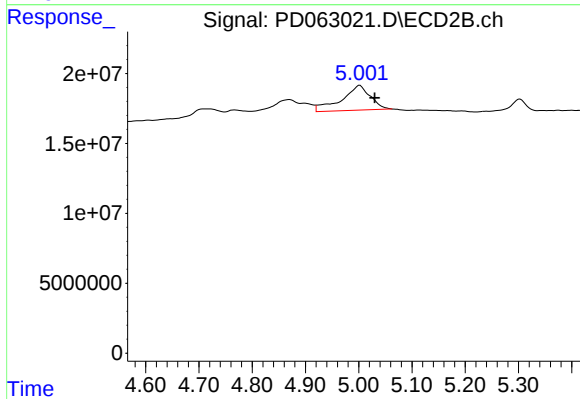

#7 delta-BHC


R.T.: 5.002 min
Delta R.T.: -0.028 min
Response: 66863329
Conc: 4.79 ng/ml

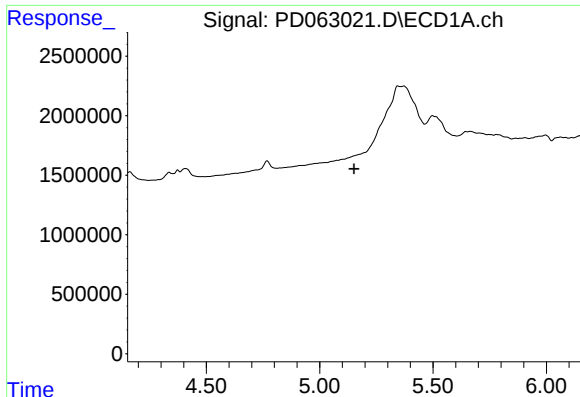

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136391BL

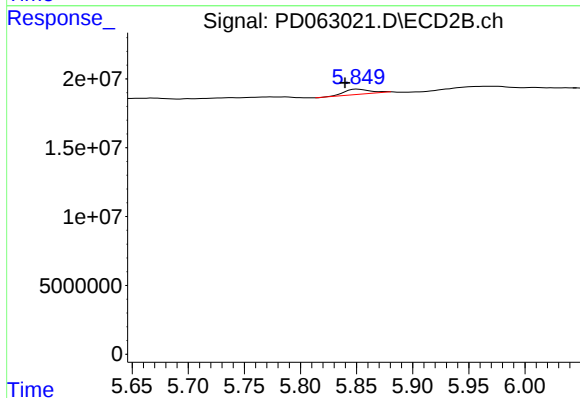


#8 Heptachlor epoxide

R.T.: 5.851 min
Delta R.T.: 0.011 min
Response: 7003558
Conc: 0.46 ng/ml

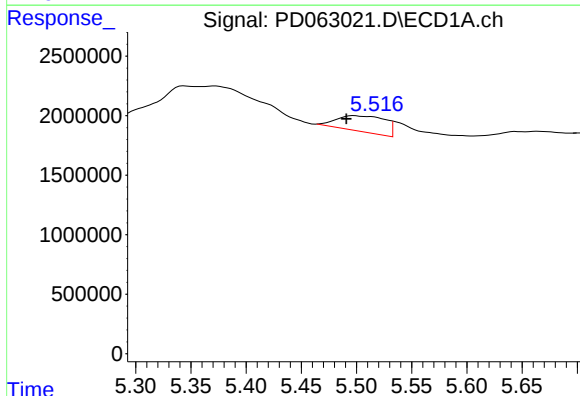


#9 Endosulfan I

R.T.: 5.498 min
Delta R.T.: 0.007 min
Response: 3826869
Conc: 2.82 ng/ml

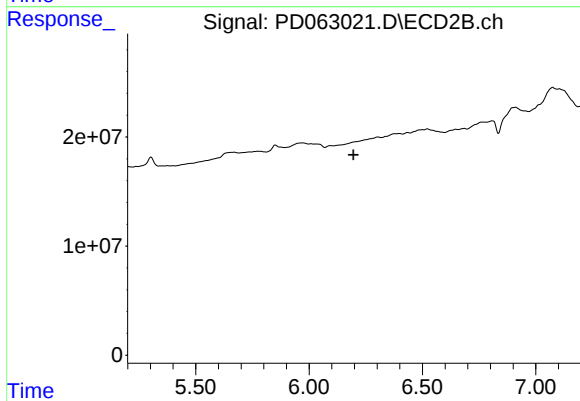

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

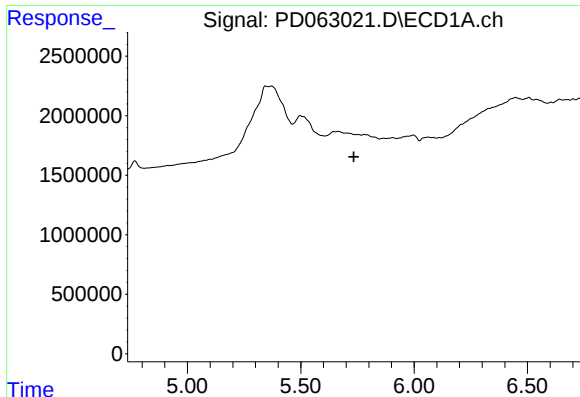

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136391BL

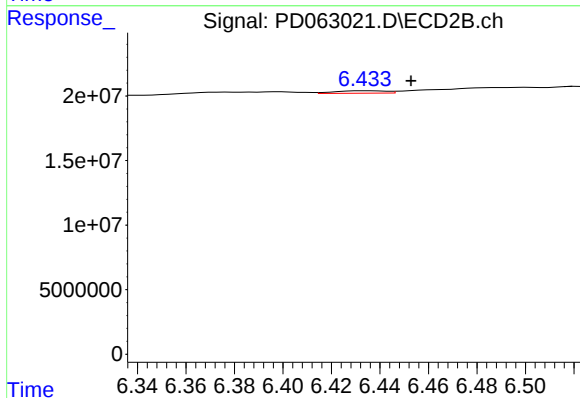


#13 Dieldrin

R.T.: 6.434 min
Delta R.T.: -0.018 min
Response: 2753488
Conc: 0.18 ng/ml

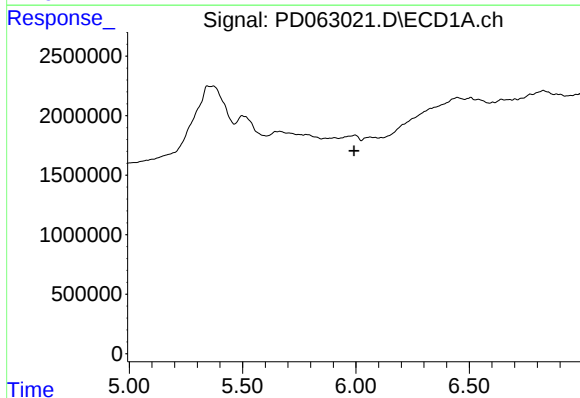


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.991 min
Response: 0
Conc: N.D.

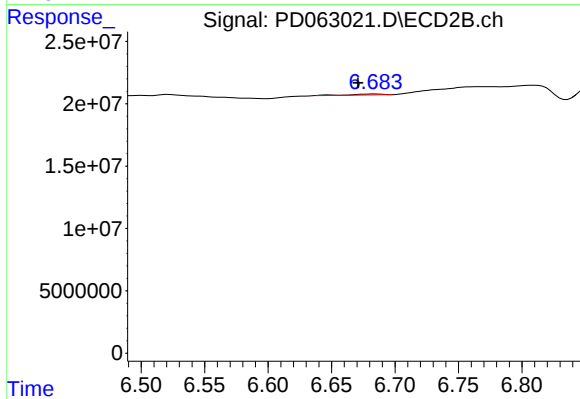

#14 Endrin


R.T.: 6.685 min
Delta R.T.: 0.014 min
Response: 1312834
Conc: 0.10 ng/ml

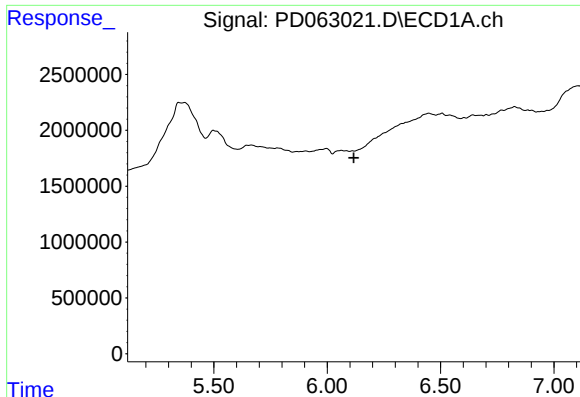

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136391BL

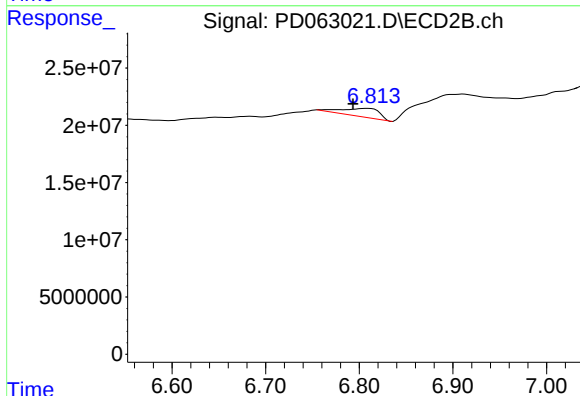


#16 4,4'-DDD

R.T.: 6.809 min
Delta R.T.: 0.016 min
Response: 20612371
Conc: 1.70 ng/ml

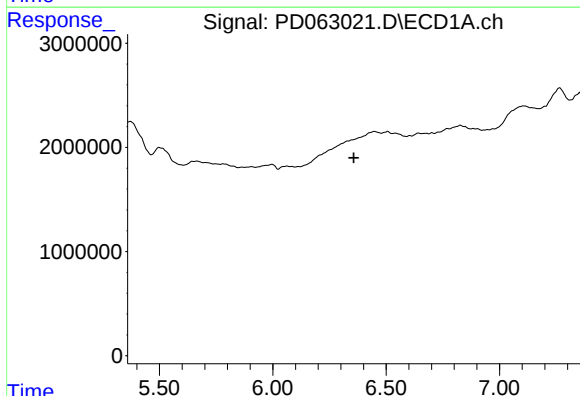


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

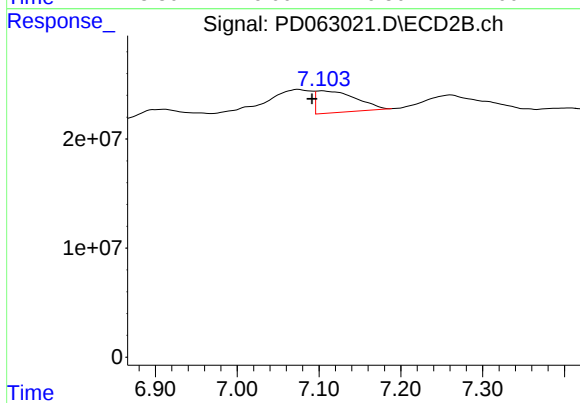

#17 4,4'-DDT


R.T.: 7.104 min
Delta R.T.: 0.013 min
Response: 68611384
Conc: 6.08 ng/ml

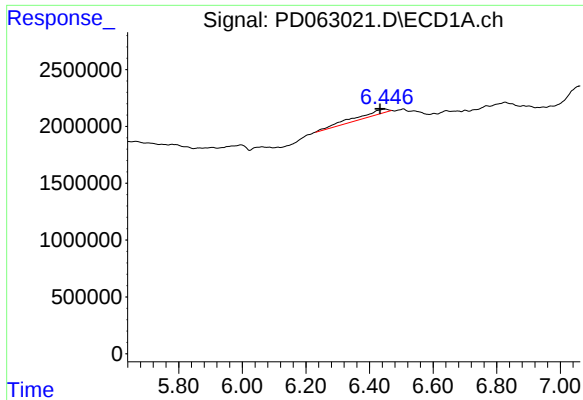

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: 0.015 min
Response: 3550873
Conc: 3.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136391BL

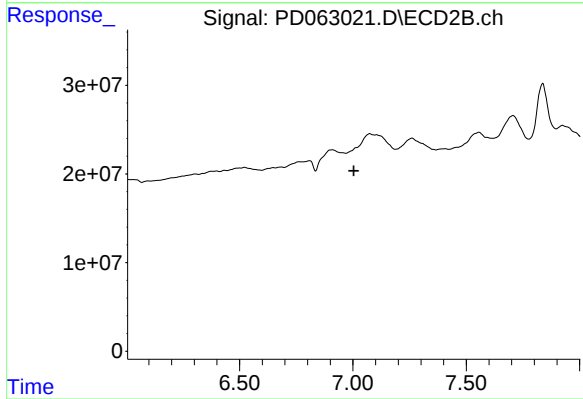


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.004 min
Response: 0
Conc: N.D.

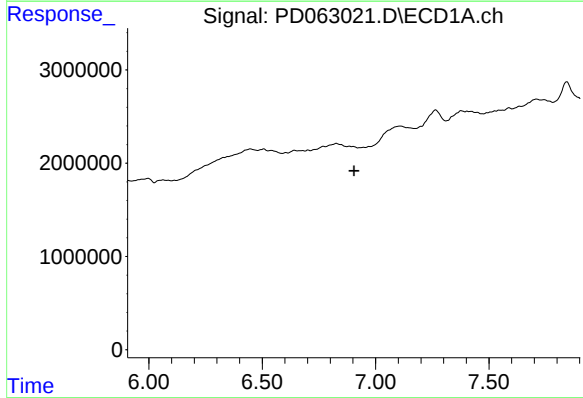


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.905 min
Response: 0
Conc: N.D.

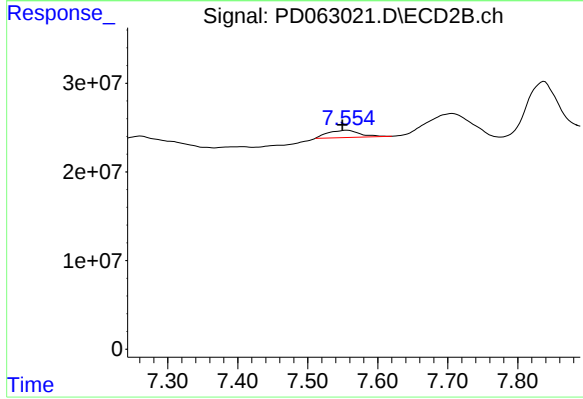

#20 Methoxychlor


R.T.: 7.556 min
Delta R.T.: 0.006 min
Response: 26009471
Conc: 4.53 ng/ml

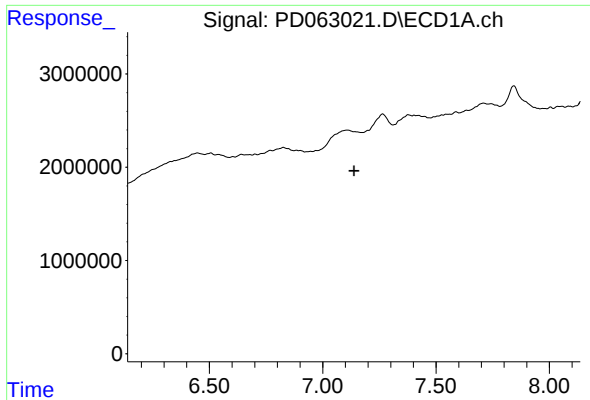

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB136391BL

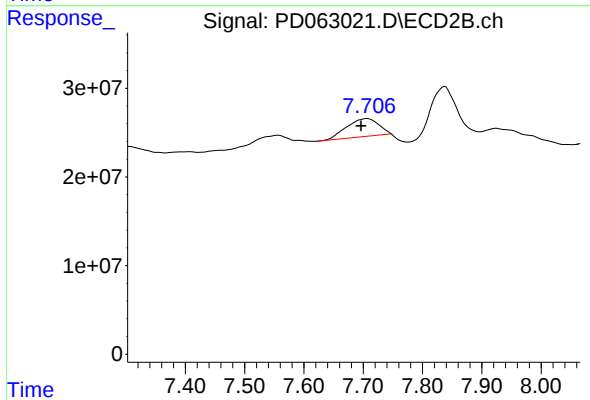


#21 Endrin ketone

R.T.: 7.707 min
Delta R.T.: 0.010 min
Response: 76135546
Conc: 6.35 ng/ml

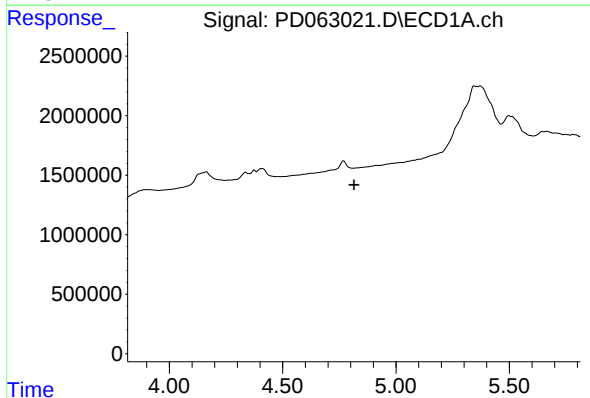


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.815 min
Response: 0
Conc: N.D.

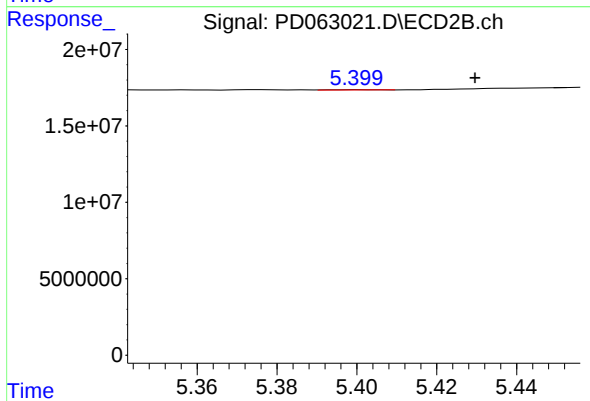

#24 Chlordane-2


R.T.: 5.401 min
Delta R.T.: -0.029 min
Response: 129051
Conc: 0.26 ng/ml

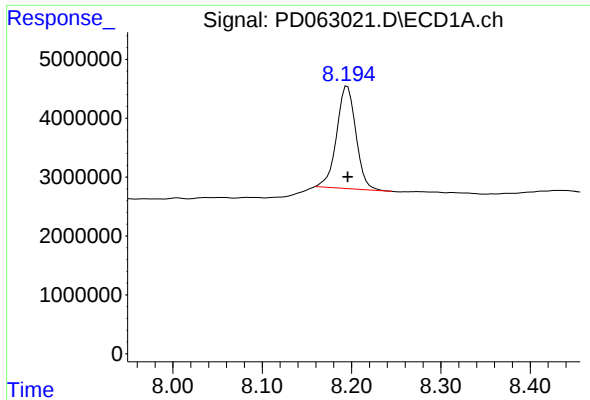

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 25947536
Conc: 20.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB136391BL

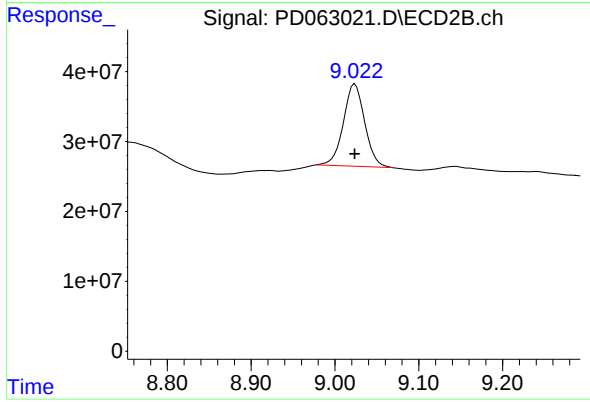

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 207836579
Conc: 20.37 ng/ml