

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
 Data File : PD063024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2021 19:54
 Operator : AR\AJ
 Sample : M2383-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 KTW-02

Manual Integrations
 APPROVED

Ankita
 5/20/2021 1:34:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 08:39:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.967	29691195	586.6E6	26.955	50.621m#
28)	SA Decachlor...	8.195	9.025	18453604	141.1E6	14.663	13.827m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051721\
Data File : PD063024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2021 19:54
Operator : AR\AJ
Sample : M2383-08
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
KTW-02


Manual Integrations
APPROVED

Ankita
5/20/2021 1:34:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 08:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

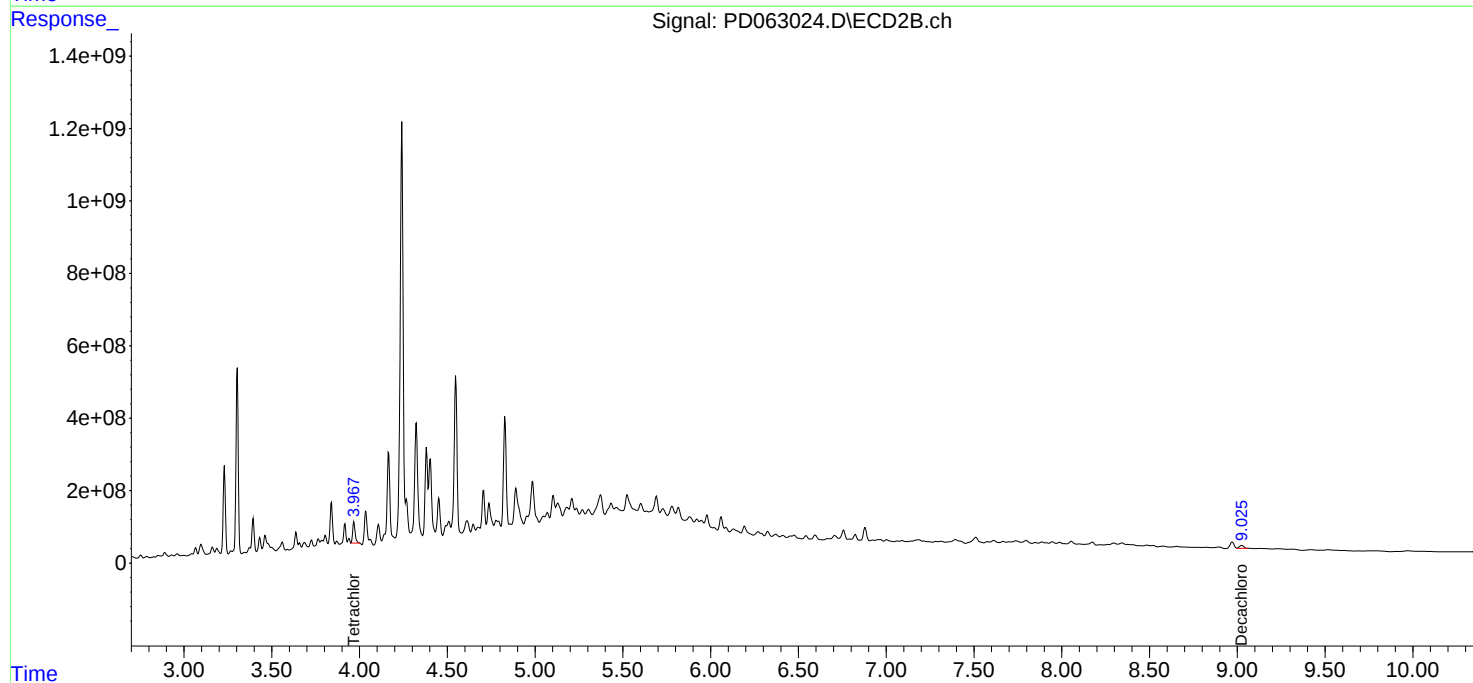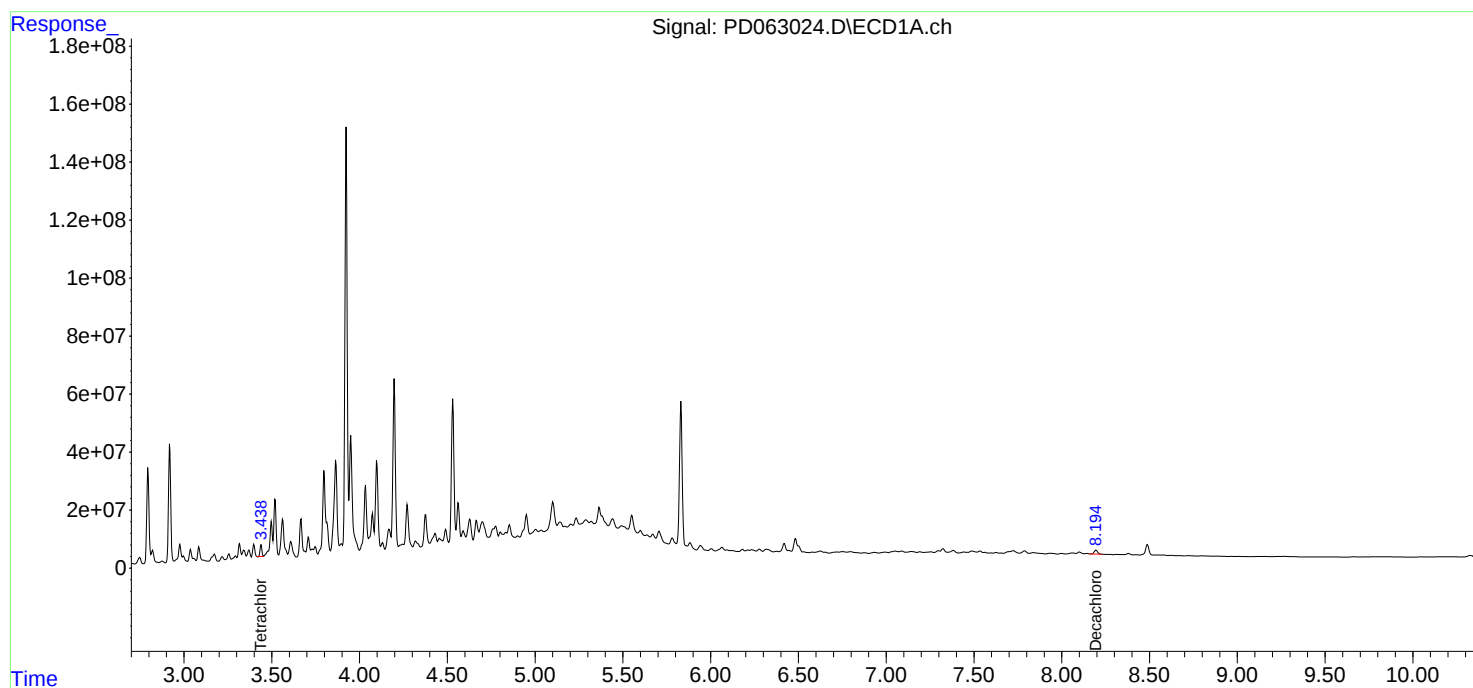

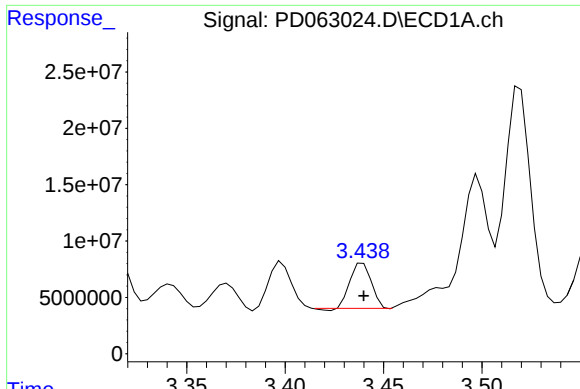


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 29691195
Conc: 26.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
KTW-02


Manual Integrations
APPROVED

Ankita
5/20/2021 1:34:01 PM

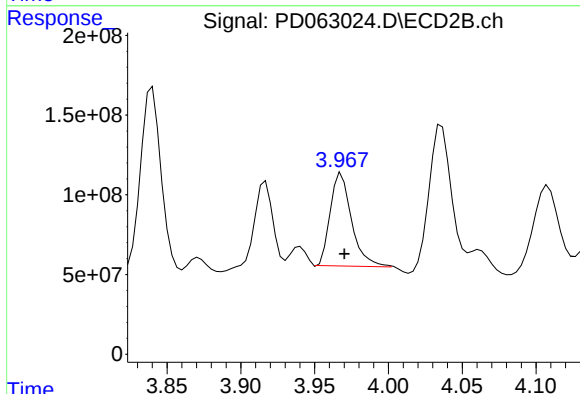


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.003 min
Response: 586602277
Conc: 50.62 ng/ml m

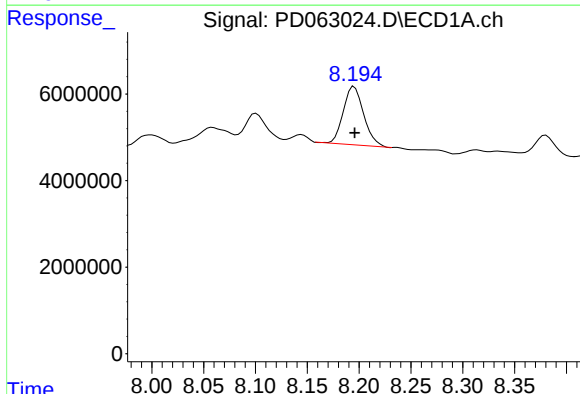

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 18453604
Conc: 14.66 ng/ml

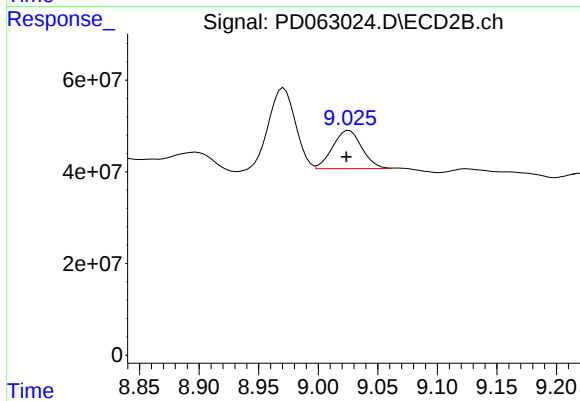

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 141066910
Conc: 13.83 ng/ml m