

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051722\
 Data File : PD069668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2022 16:12
 Operator : AR\AJ
 Sample : N2766-24MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4H1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/20/2022
 Supervised By : mohammad ahmed 05/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 06:01:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	11681405	144.6E6	9.609	11.404
27)	SA Decachlor...	8.200	9.368	21041128	127.8E6	16.964	17.504
Target Compounds							
2)	A alpha-BHC	3.883	4.567	61506598	530.8E6	36.058	29.064m
3)	MA gamma-BHC...	4.166	4.859	62751441	514.1E6	37.476	31.573
4)	MA Heptachlor	4.464	5.387	62974499	528.2E6	38.924	33.382
5)	MB Aldrin	4.711	5.699	61853305	511.3E6	42.152	35.626
6)	B beta-BHC	4.415	5.023	27597590	232.2E6	38.688m	34.083
7)	B delta-BHC	4.620	5.248	10811048	75779061	7.163	6.688
8)	B Heptachlo...	5.155	6.087	56763060	438.1E6	40.869	40.623
9)	A Endosulfan I	5.493	6.450	50836763	390.4E6	36.963	30.898
10)	B trans-Chl...	5.381	6.324	57664609	434.7E6	40.583	33.106
11)	B cis-Chlor...	5.440	6.399	55290388	414.8E6	39.688	32.543
12)	B 4,4'-DDE	5.605	6.549	113.1E6	823.2E6	86.835	71.251
13)	MA Dieldrin	5.737	6.708	118.9E6	852.4E6	80.150	66.959
14)	MA Endrin	5.995	6.929	103.8E6	693.5E6	79.710	68.570
15)	B Endosulfa...	6.267	7.134	97164632	673.8E6	83.325m	70.417
16)	A 4,4'-DDD	6.122	7.040	89842530	654.1E6	76.659	66.088
17)	MA 4,4'-DDT	6.363	7.343	89293921	637.0E6	76.362	66.582
18)	B Endrin al...	6.439	7.258	77491321	539.8E6	74.539	65.356
19)	B Endosulfa...	6.651	7.483	72476971	491.4E6	59.141	52.524
20)	A Methoxychlor	6.913	7.797	245.9E6	1485.5E6	374.291	336.969
21)	B Endrin ke...	7.145	7.958	110.0E6	669.5E6	80.755	69.993

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051722\
Data File : PD069668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2022 16:12
Operator : AR\AJ
Sample : N2766-24MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 06:01:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

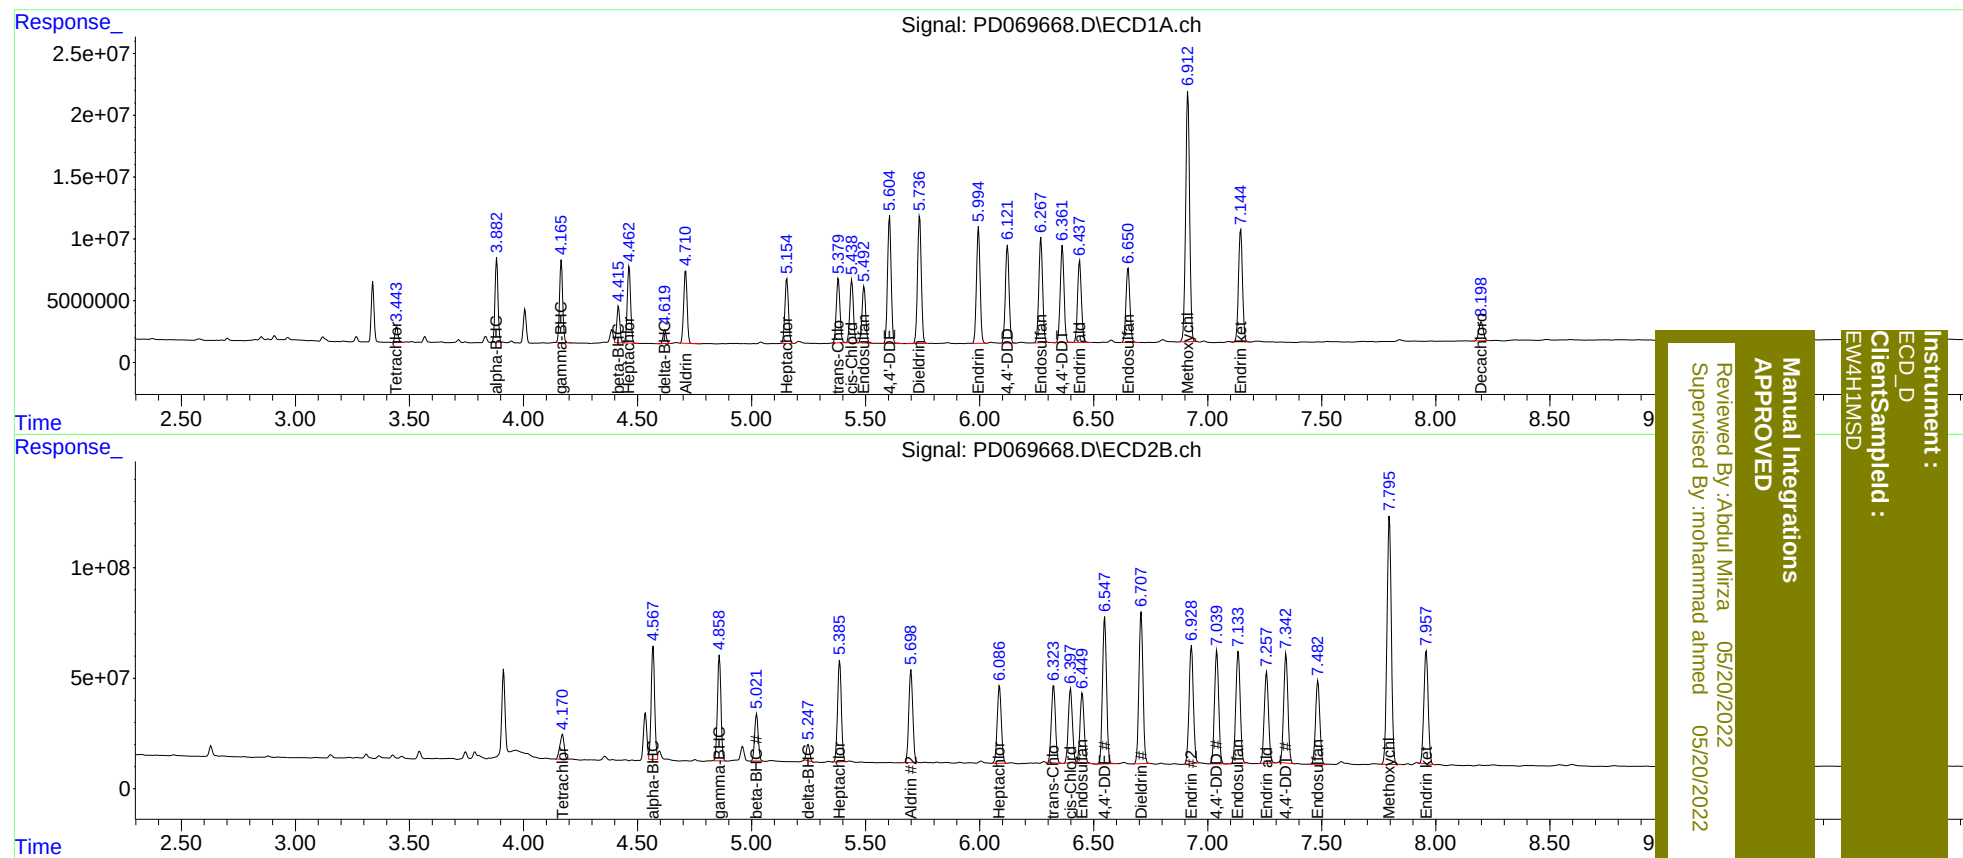

Reviewed By: Abdul Mirza 05/20/2022
Supervised By: mohammad ahmed 05/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW4H1MSD