

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051722\
 Data File : PD069667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2022 15:58
 Operator : AR\AJ
 Sample : N2766-23MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4H1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/20/2022
 Supervised By : mohammad ahmed 05/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 06:00:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	11612524	144.9E6	9.553	11.429
27)	SA Decachlor...	8.200	9.369	21179114	128.8E6	17.075	17.641
Target Compounds							
2)	A alpha-BHC	3.884	4.567	61580181	520.0E6	36.101	28.470m
3)	MA gamma-BHC...	4.167	4.859	62987988	519.1E6	37.618	31.882
4)	MA Heptachlor	4.464	5.387	63374160	531.3E6	39.171	33.579
5)	MB Aldrin	4.712	5.699	62176781	515.5E6	42.372	35.916
6)	B beta-BHC	4.416	5.023	27485609	233.7E6	38.531m	34.300
7)	B delta-BHC	4.621	5.248	10978469	79940225	7.274	7.055
8)	B Heptachlo...	5.156	6.087	57093147	448.7E6	41.107	41.610
9)	A Endosulfan I	5.494	6.451	50894622	394.7E6	37.005	31.234
10)	B trans-Chl...	5.381	6.324	58086183	438.6E6	40.879	33.405
11)	B cis-Chlor...	5.440	6.399	55433554	420.7E6	39.791	33.002
12)	B 4,4'-DDE	5.606	6.550	112.8E6	834.4E6	86.601	72.220
13)	MA Dieldrin	5.738	6.710	119.6E6	863.5E6	80.622	67.825
14)	MA Endrin	5.996	6.930	104.2E6	699.4E6	79.989	69.159
15)	B Endosulfa...	6.268	7.135	98334428	679.0E6	84.328m	70.964
16)	A 4,4'-DDD	6.123	7.041	90607542	660.8E6	77.312	66.763
17)	MA 4,4'-DDT	6.363	7.344	90075961	641.7E6	77.031	67.074
18)	B Endrin al...	6.439	7.259	78052421	546.4E6	75.078	66.157
19)	B Endosulfa...	6.652	7.484	73167373	495.6E6	59.705	52.974
20)	A Methoxychlor	6.913	7.798	247.3E6	1496.3E6	376.400	339.437
21)	B Endrin ke...	7.146	7.959	110.8E6	678.1E6	81.315	70.891

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051722\
Data File : PD069667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2022 15:58
Operator : AR\AJ
Sample : N2766-23MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 06:00:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

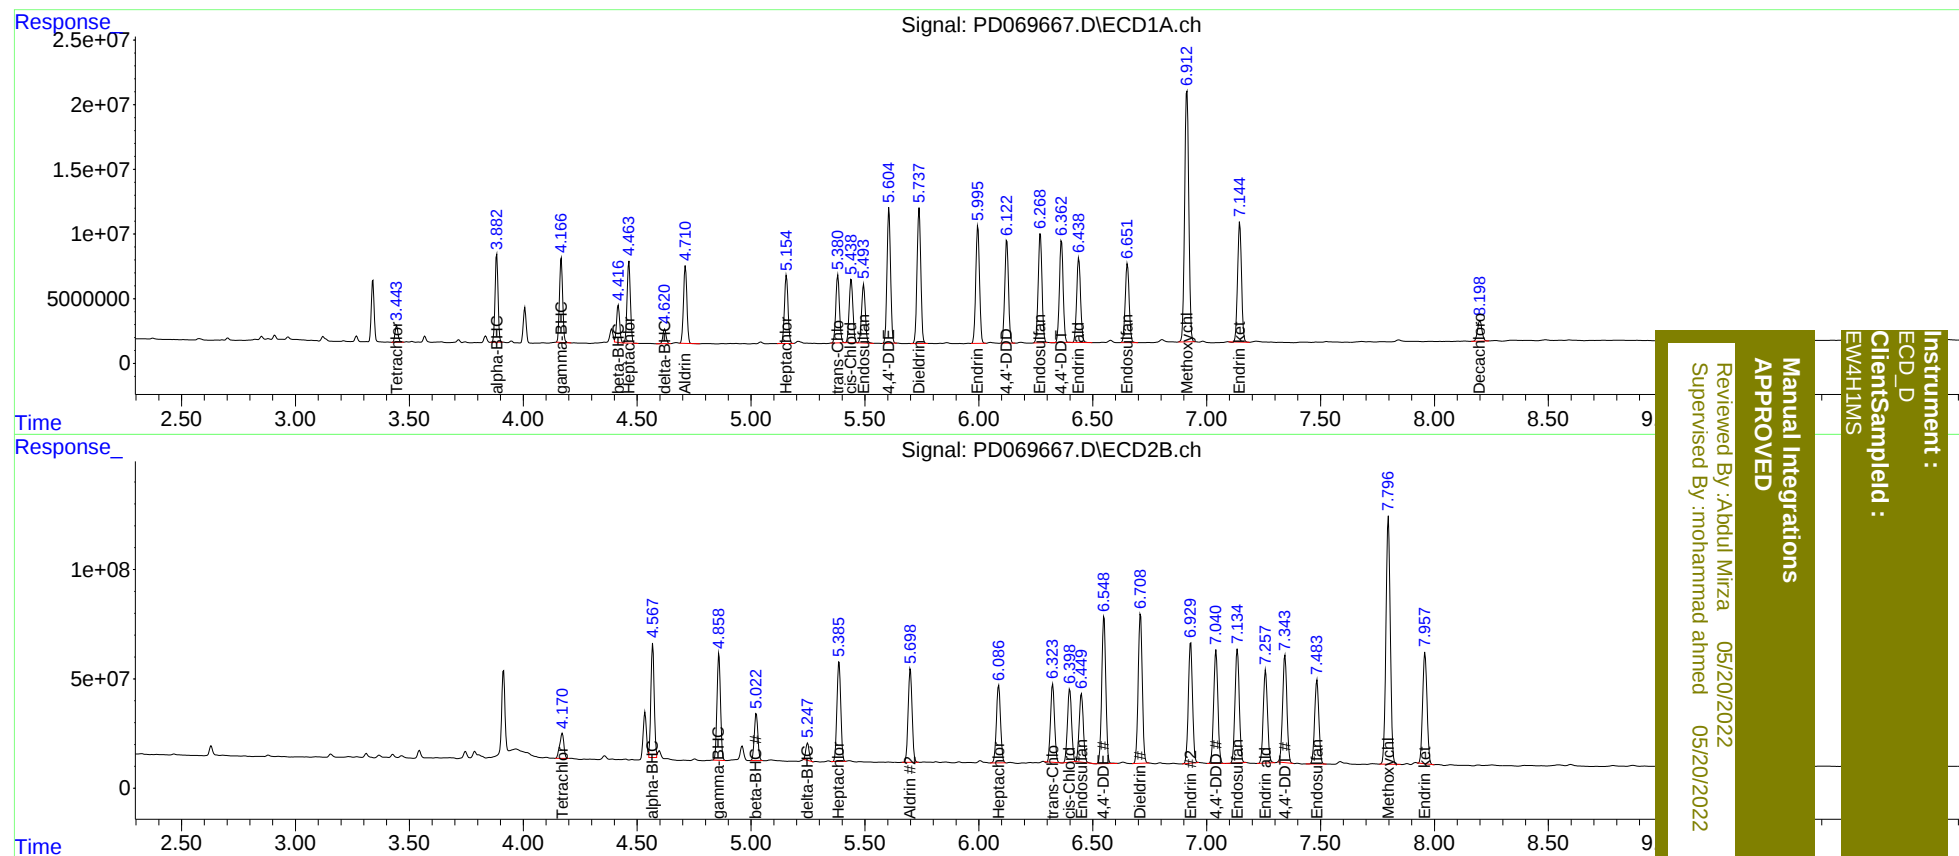

Reviewed By: Abdul Miza 05/20/2022
Supervised By: mohammad ahmed 05/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client/Sampled :
EW4/H1MS