

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051822\
 Data File : PD069687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 14:21
 Operator : AR\AJ
 Sample : N2843-04MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4H4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/19/2022
 Supervised By : mohammad ahmed 05/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:04:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.170	12123835	143.7E6	9.973	11.331
27)	SA Decachlor...	8.199	9.365	17608936	99236201	14.197	13.589
Target Compounds							
2)	A alpha-BHC	3.883	4.566	62585892	503.5E6	36.691	27.568m
3)	MA gamma-BHC...	4.166	4.858	64940332	494.6E6	38.784	30.376
4)	MA Heptachlor	4.463	5.385	64714713	492.1E6	40.000	31.100
5)	MB Aldrin	4.710	5.698	62523450	467.9E6	42.609	32.604
6)	B beta-BHC	4.417	5.021	27781414	194.2E6	38.946	28.495 #
7)	B delta-BHC	4.620	5.248	11135771	55789581	7.378	4.924 #
8)	B Heptachlo...	5.155	6.087	56117957	383.5E6	40.405	35.558
9)	A Endosulfan I	5.493	6.449	46845434	346.2E6	34.061	27.395
10)	B trans-Chl...	5.380	6.323	56190768	394.9E6	39.546	30.076
11)	B cis-Chlor...	5.439	6.398	52877904	368.4E6	37.956	28.902
12)	B 4,4'-DDE	5.605	6.548	108.4E6	702.5E6	83.275	60.807 #
13)	MA Dieldrin	5.737	6.708	121.8E6	729.0E6	82.146	57.264 #
14)	MA Endrin	5.995	6.928	96959856	591.3E6	74.465	58.465
15)	B Endosulfa...	6.269	7.133	89464260	567.3E6	76.721	59.291
16)	A 4,4'-DDD	6.122	7.038	81949418	551.6E6	69.924	55.732
17)	MA 4,4'-DDT	6.362	7.340	82970285	558.5E6	70.954	58.379m
18)	B Endrin al...	6.439	7.257	68547654	448.7E6	65.936	54.323
19)	B Endosulfa...	6.651	7.481	66677819	396.6E6	54.409	42.396
20)	A Methoxychlor	6.913	7.795	224.1E6	1270.5E6	341.172	288.201
21)	B Endrin ke...	7.143	7.955	93487009	553.2E6	68.633m	57.839m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051822\
Data File : PD069687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 14:21
Operator : AR\AJ
Sample : N2843-04MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:04:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

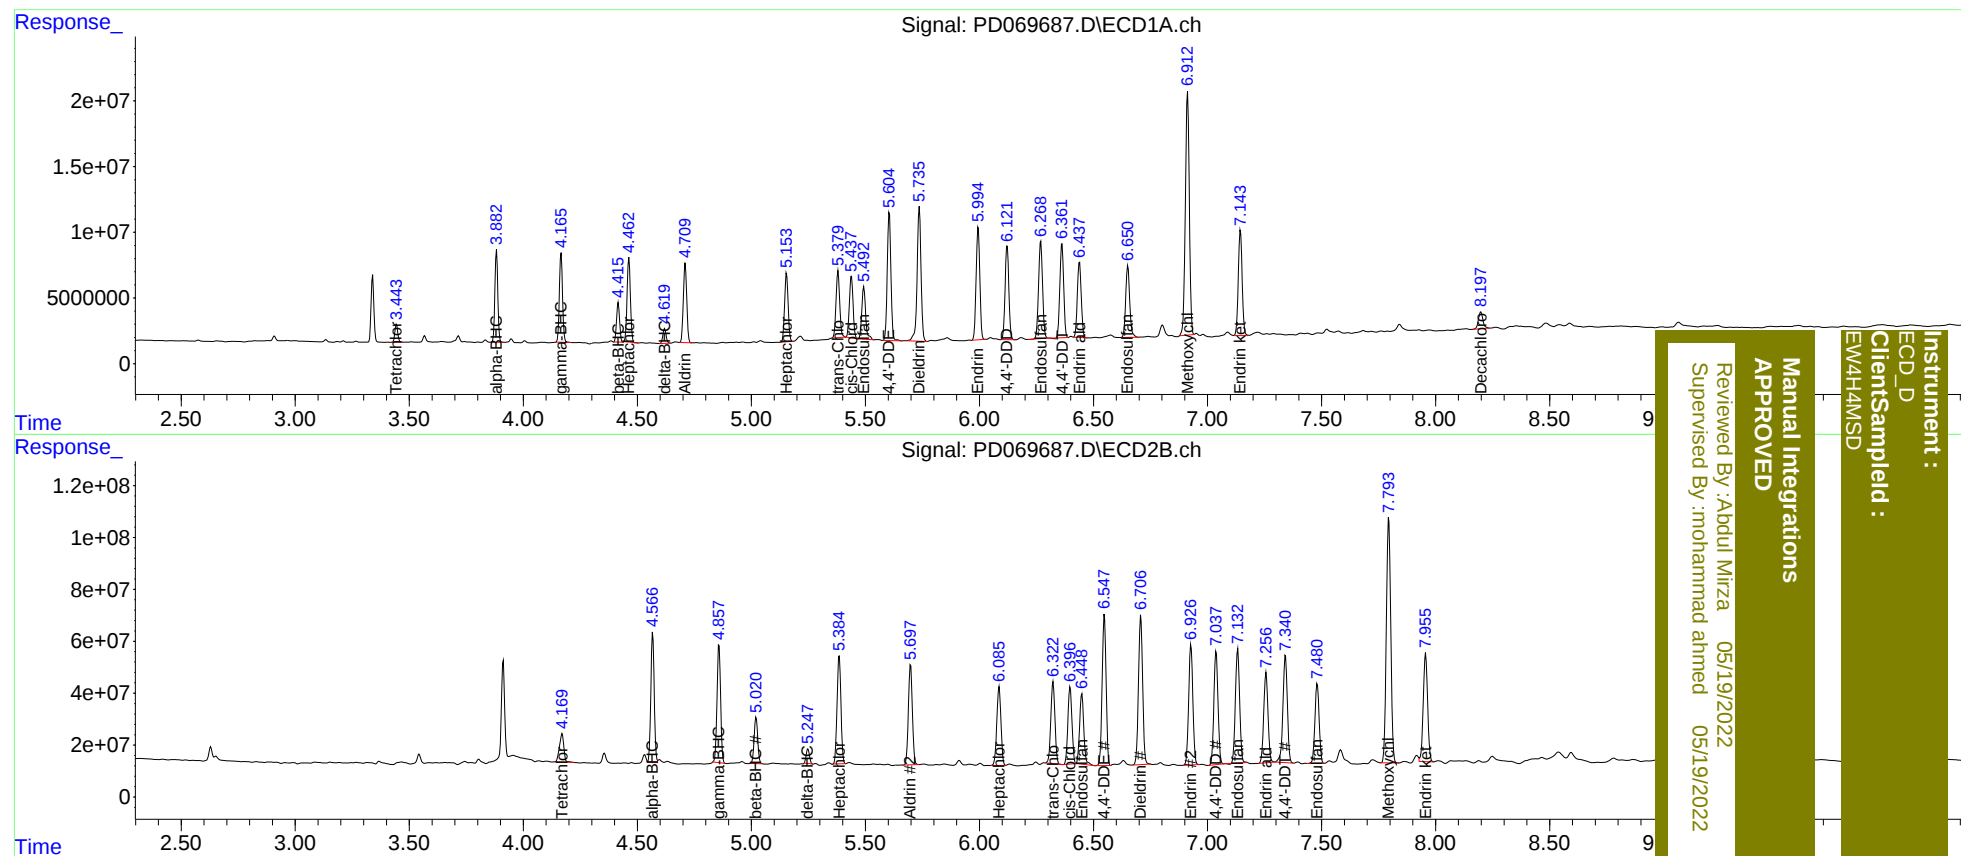

Reviewed By: Abdul Miza 05/19/2022
Supervised By: mohammad ahmed 05/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW4H4MSD