

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051822\
 Data File : PD069688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 14:35
 Operator : AR\AJ
 Sample : N2843-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4H7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/19/2022
 Supervised By : mohammad ahmed 05/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 03:04:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.444	4.171	10699208	81383929	8.801	6.418m#
2) SA Decachlor...	8.198	9.366	13749515	78935724	11.085	10.809
Target Compounds						
10) B trans-Chl...	5.380	6.323	2092182	72221742	1.472m	5.501 #
11) B cis-Chlor...	5.437	6.400	2533393	30750856	1.818m	2.412 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051822\
Data File : PD069688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 14:35
Operator : AR\AJ
Sample : N2843-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 03:04:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

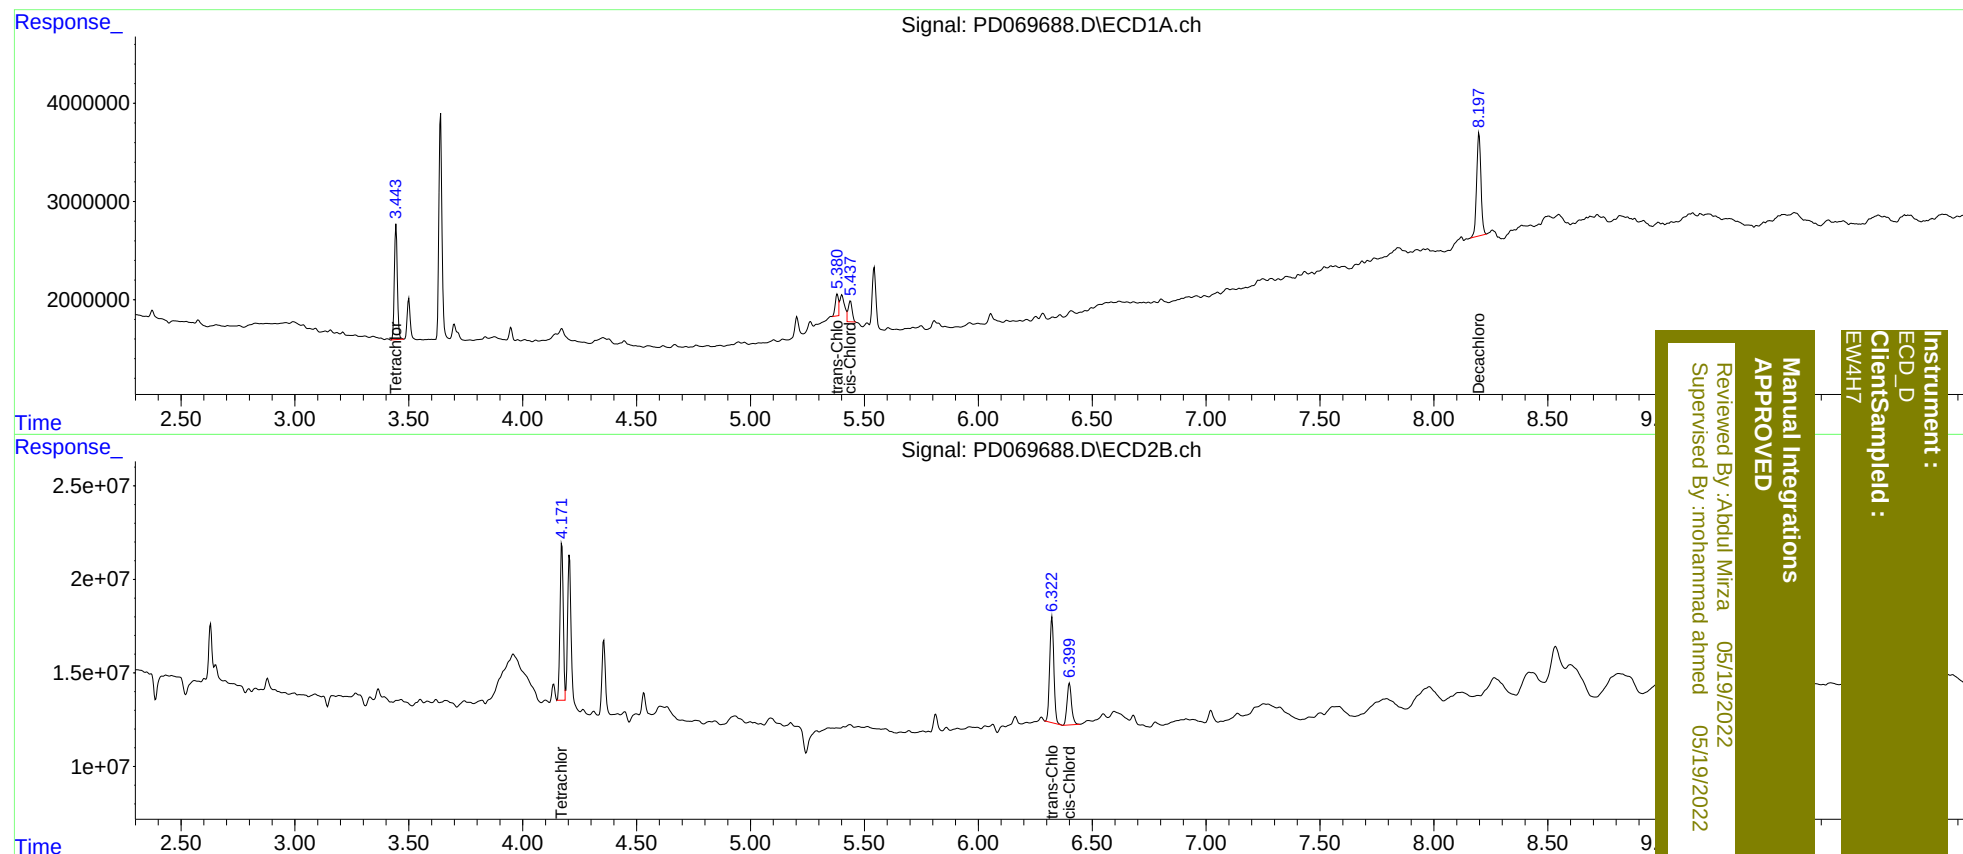

Reviewed By : Abdul Mirza 05/19/2022
Supervised By : mohammad ahmed 05/19/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/4H7