

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
 Data File : PD063067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 16:49
 Operator : AR\AJ
 Sample : M2435-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VAN-REIPEN-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 04:50:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	24238506	258.4E6	22.005	22.303
28)	SA Decachlor...	8.196	9.026	21907638	193.9E6	17.407	19.004
Target Compounds							
2)	A alpha-BHC	3.873	0.000	326141	0	0.188	N.D. #
3)	MA gamma-BHC...	4.160	0.000	1024658	0	0.630	N.D. #
5)	MB Aldrin	4.691f	5.467	6137177	8366150	4.006	0.501 #
9)	A Endosulfan I	0.000	6.222f	0	2492059	N.D.	0.175 #
15)	B Endosulfa...	0.000	6.893	0	17359573	N.D.	1.448 #
20)	A Methoxychlor	0.000	7.538	0	1178321	N.D.	0.205 #
21)	B Endrin ke...	0.000	7.696	0	12393576	N.D.	1.033 #
24)	Chlordane-2	0.000	5.426	0	19027131	N.D.	39.038 #
27)	Chlordane-5	0.000	6.949	0	1596997	N.D.	3.745 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
Data File : PD063067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 16:49
Operator : AR\AJ
Sample : M2435-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 04:50:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

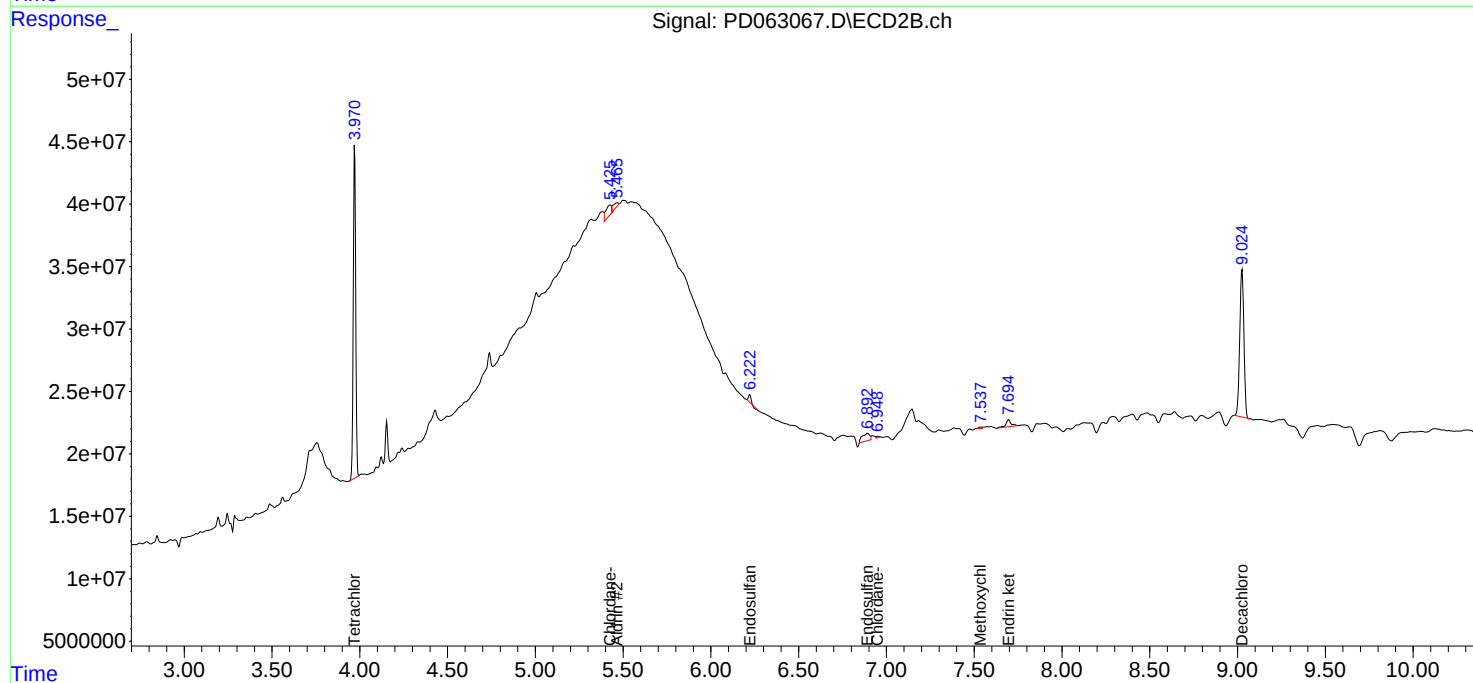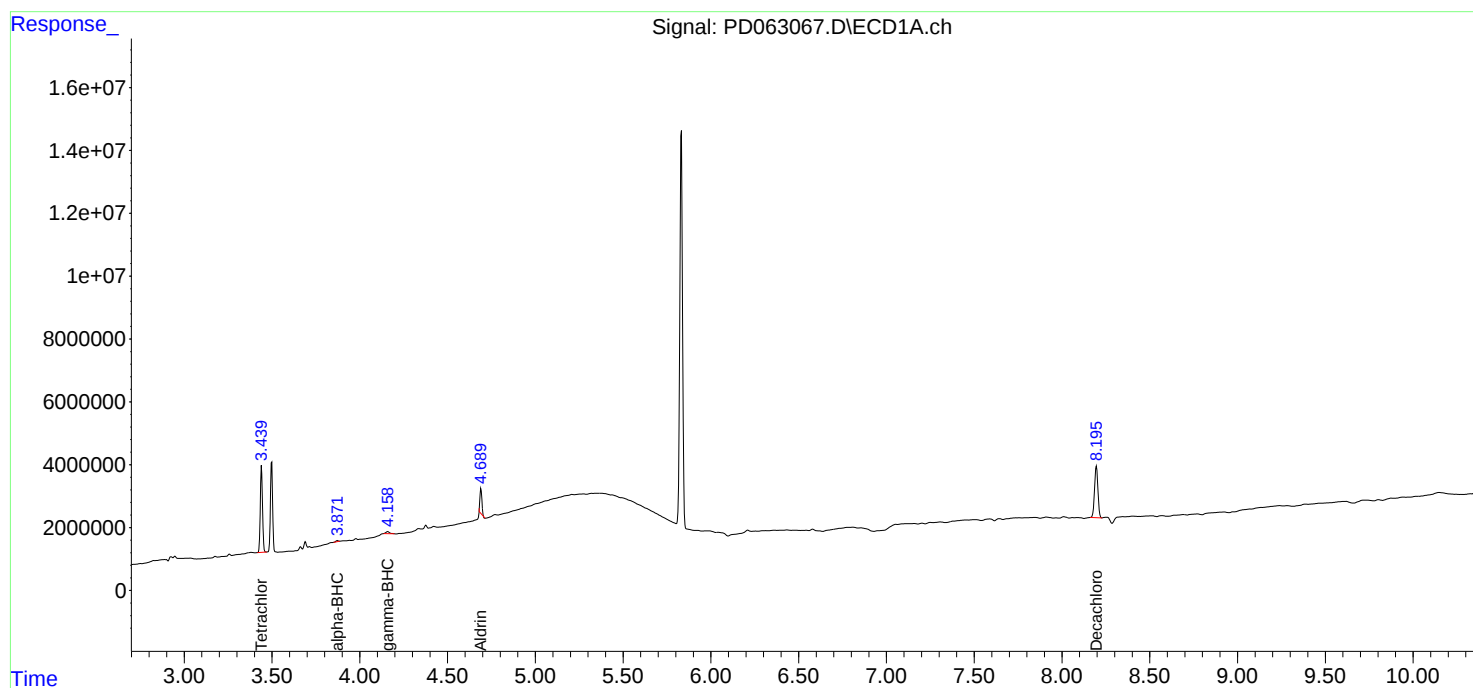


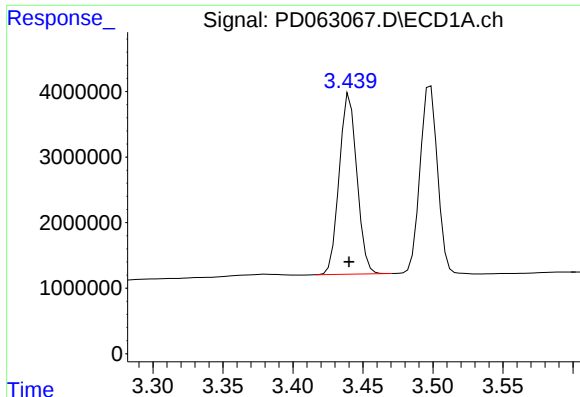

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 24238506
Conc: 22.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

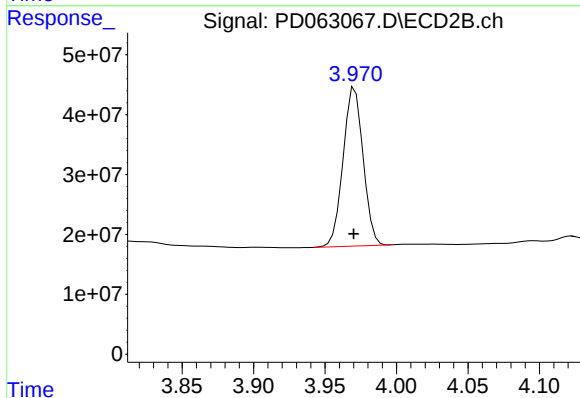


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 258447629
Conc: 22.30 ng/ml

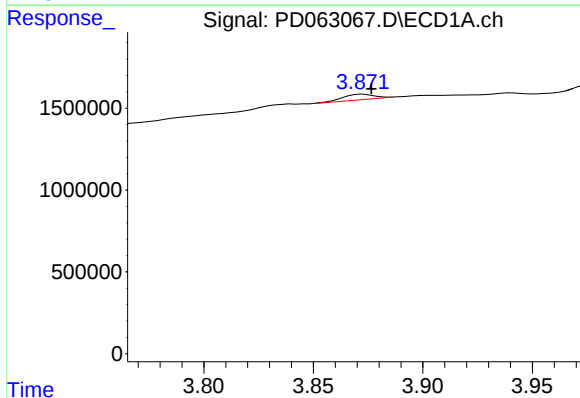


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: -0.004 min
Response: 326141
Conc: 0.19 ng/ml

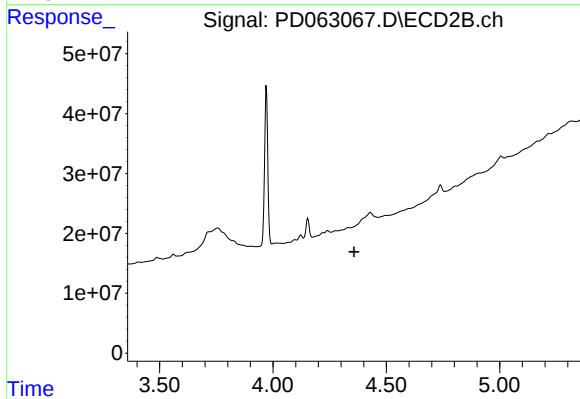

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.358 min
Response: 0
Conc: N.D.

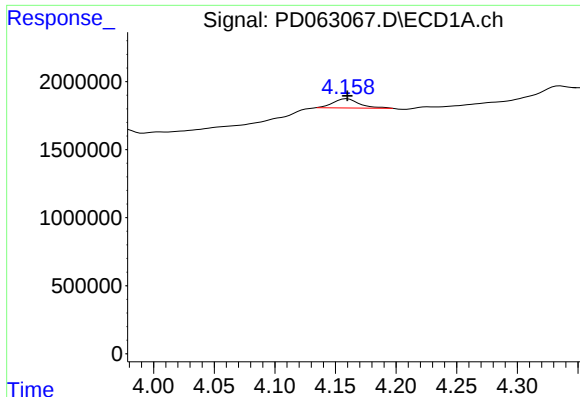

#3 gamma-BHC (Lindane)


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 1024658
Conc: 0.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

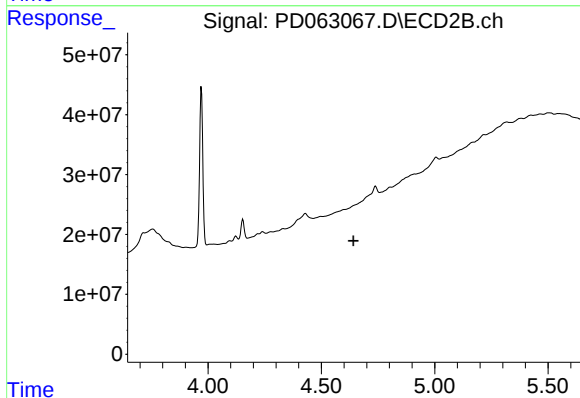


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

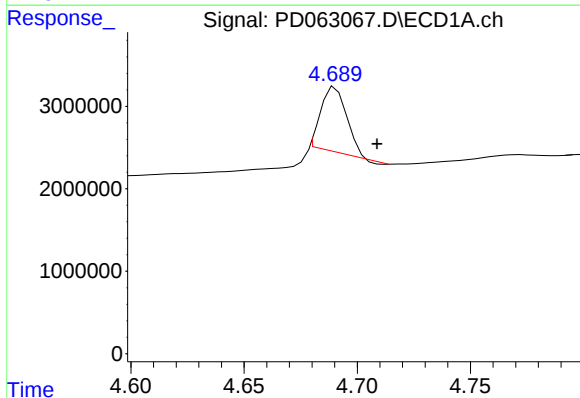


#5 Aldrin

R.T.: 4.691 min
Delta R.T.: -0.018 min
Response: 6137177
Conc: 4.01 ng/ml

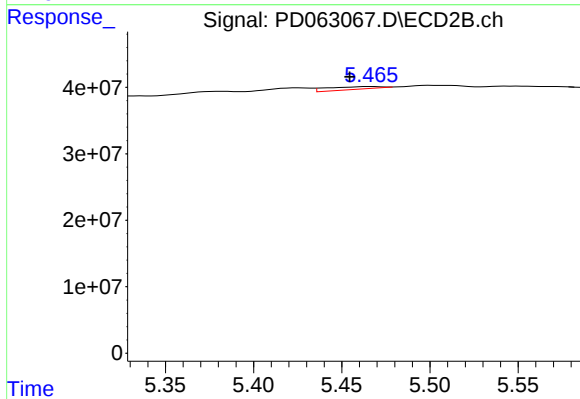

#5 Aldrin


R.T.: 5.467 min
Delta R.T.: 0.013 min
Response: 8366150
Conc: 0.50 ng/ml

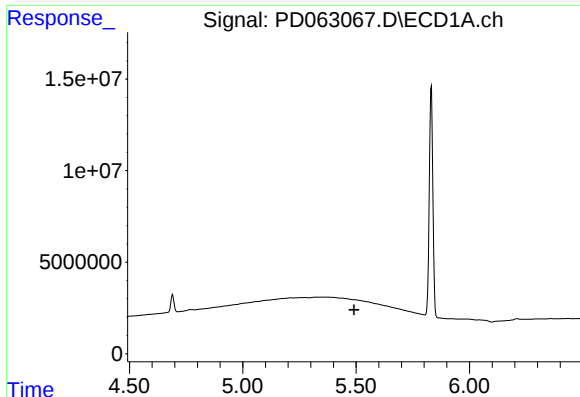

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

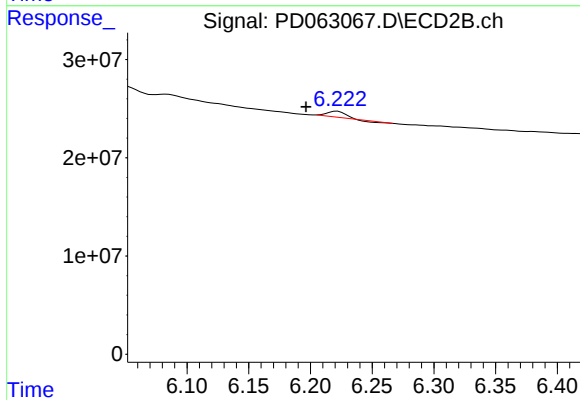


#9 Endosulfan I

R.T.: 6.222 min
Delta R.T.: 0.025 min
Response: 2492059
Conc: 0.18 ng/ml

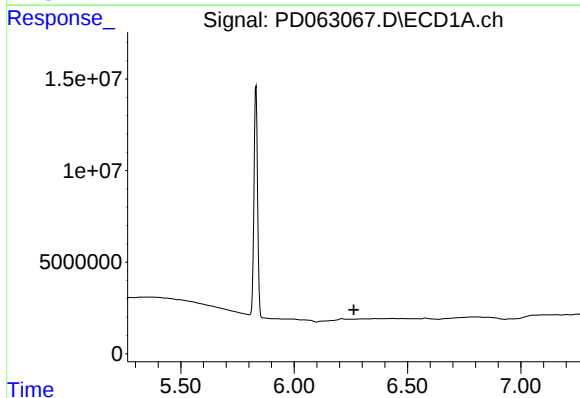


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.264 min
Response: 0
Conc: N.D.

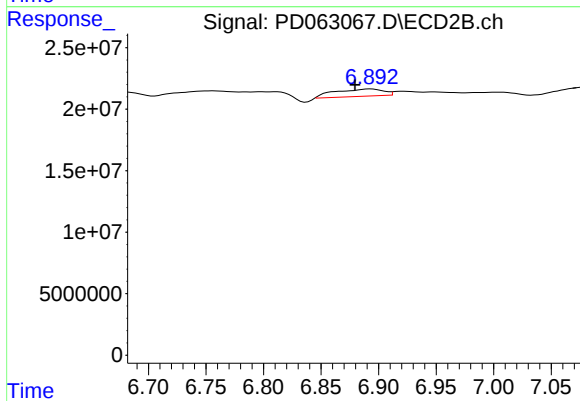

#15 Endosulfan II


R.T.: 6.893 min
Delta R.T.: 0.014 min
Response: 17359573
Conc: 1.45 ng/ml

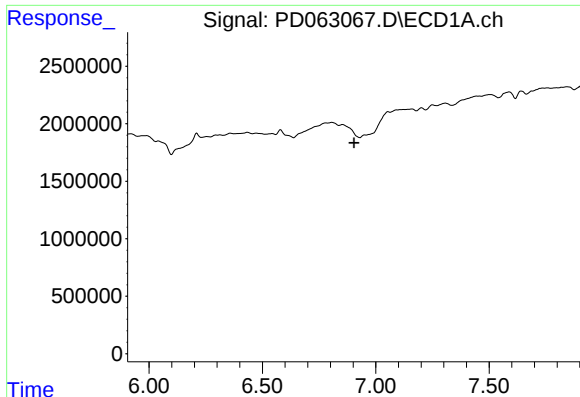

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

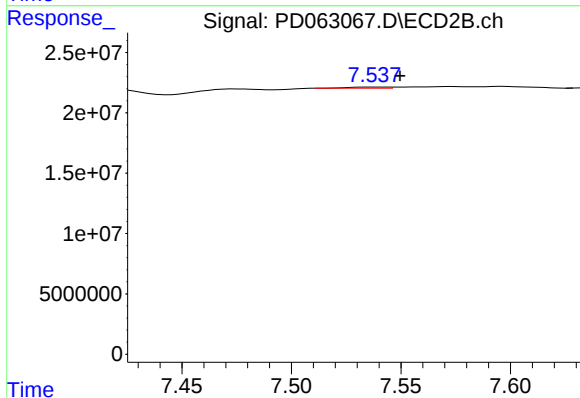


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: -0.012 min
Response: 1178321
Conc: 0.21 ng/ml

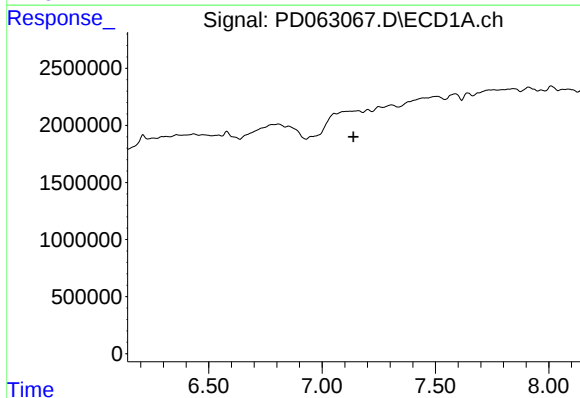


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.139 min
Response: 0
Conc: N.D.

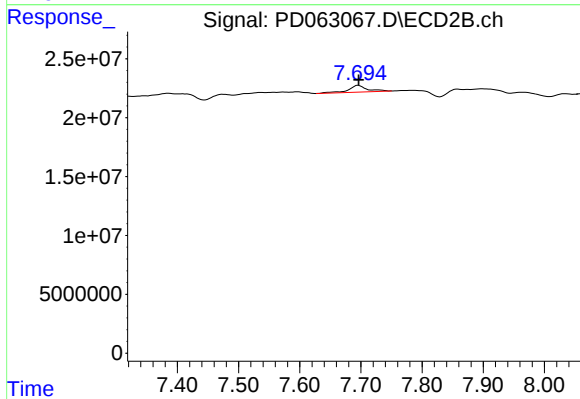

#21 Endrin ketone


R.T.: 7.696 min
Delta R.T.: 0.000 min
Response: 12393576
Conc: 1.03 ng/ml

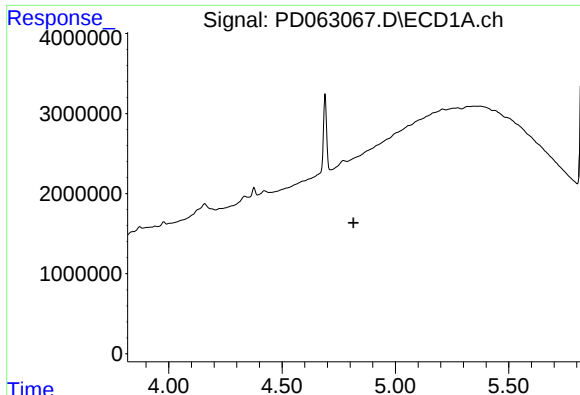

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

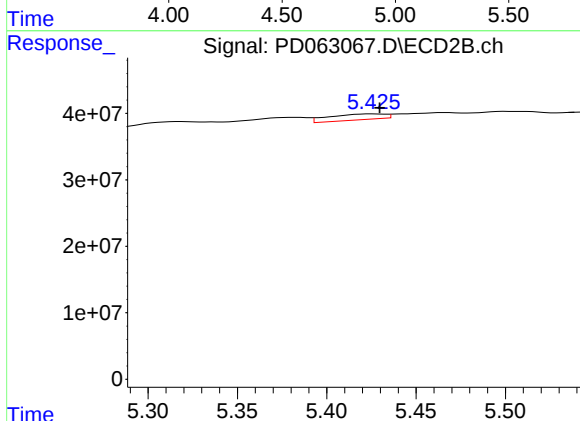


#24 Chlordane-2

R.T.: 5.426 min
Delta R.T.: -0.003 min
Response: 19027131
Conc: 39.04 ng/ml

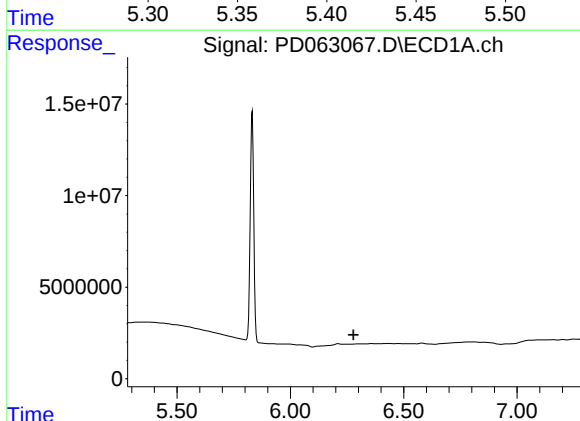


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

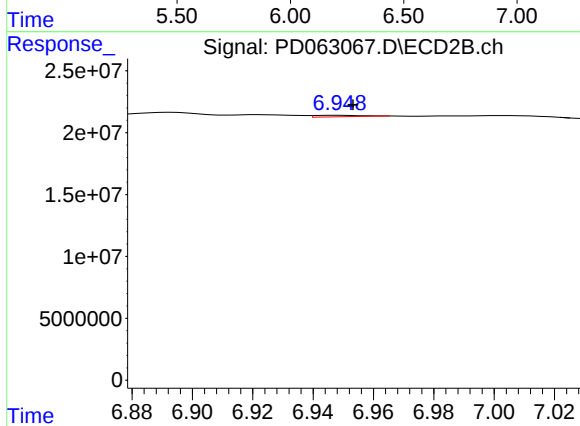

#27 Chlordane-5


R.T.: 6.949 min
Delta R.T.: -0.004 min
Response: 1596997
Conc: 3.75 ng/ml

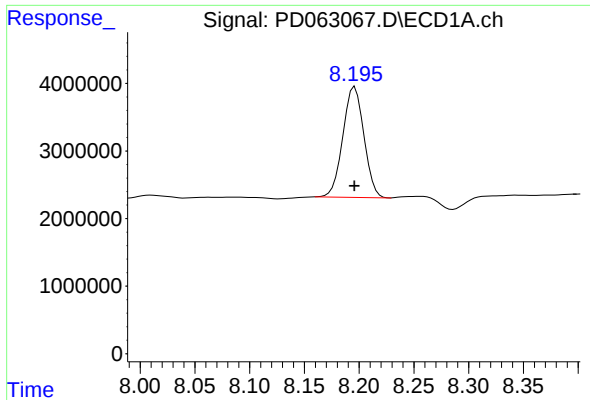

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 21907638
Conc: 17.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
VAN-REIPEN-B

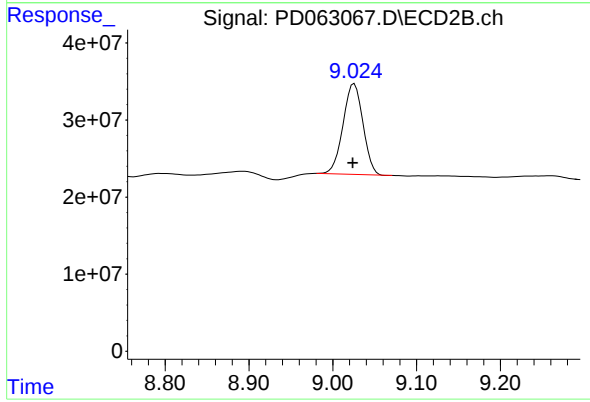

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 193876902
Conc: 19.00 ng/ml