

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
 Data File : PD063075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 18:42
 Operator : AR\AJ
 Sample : M2436-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 04:52:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	15562680	155.9E6	14.128	13.454
28)	SA Decachlor...	8.196	9.025	15993530	152.7E6	12.708	14.963
Target Compounds							
12)	B 4,4'-DDE	5.600	6.302	7872100	137.3E6	5.487	9.096 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
Data File : PD063075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 18:42
Operator : AR\AJ
Sample : M2436-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 04:52:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

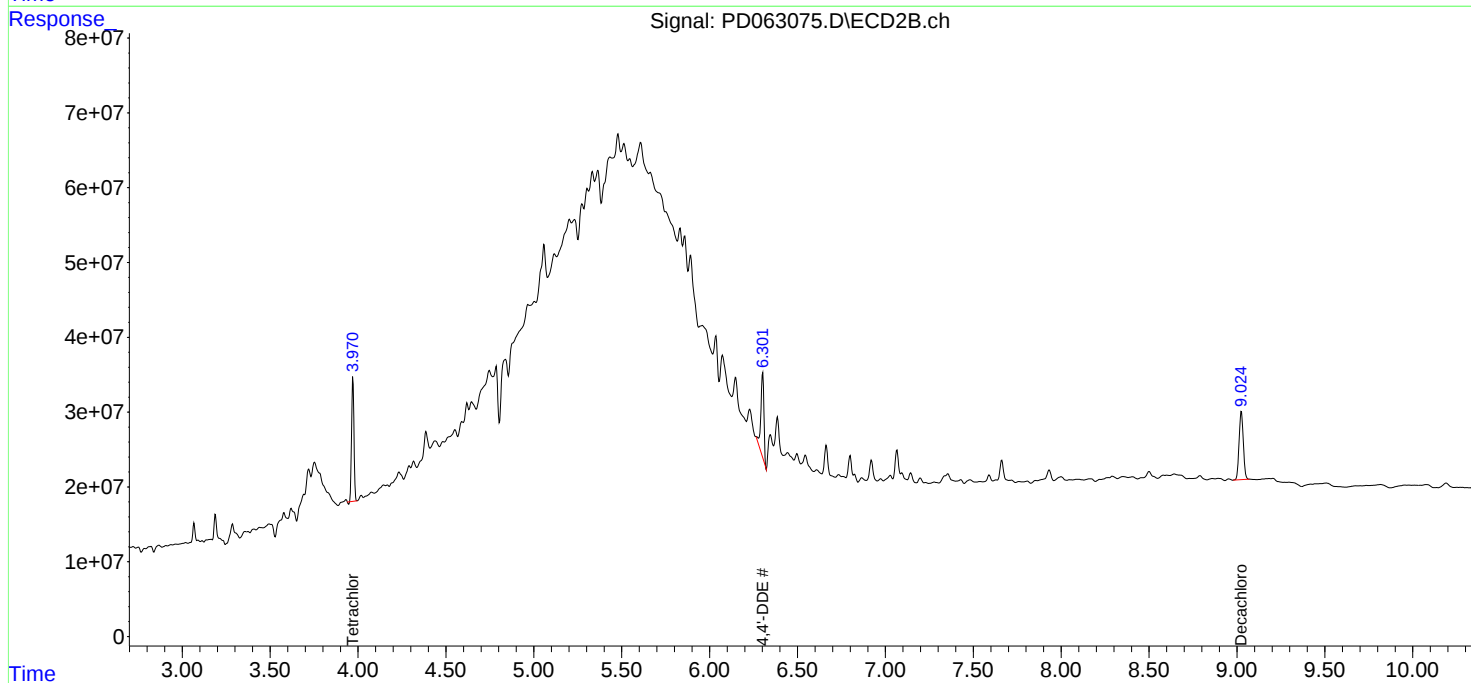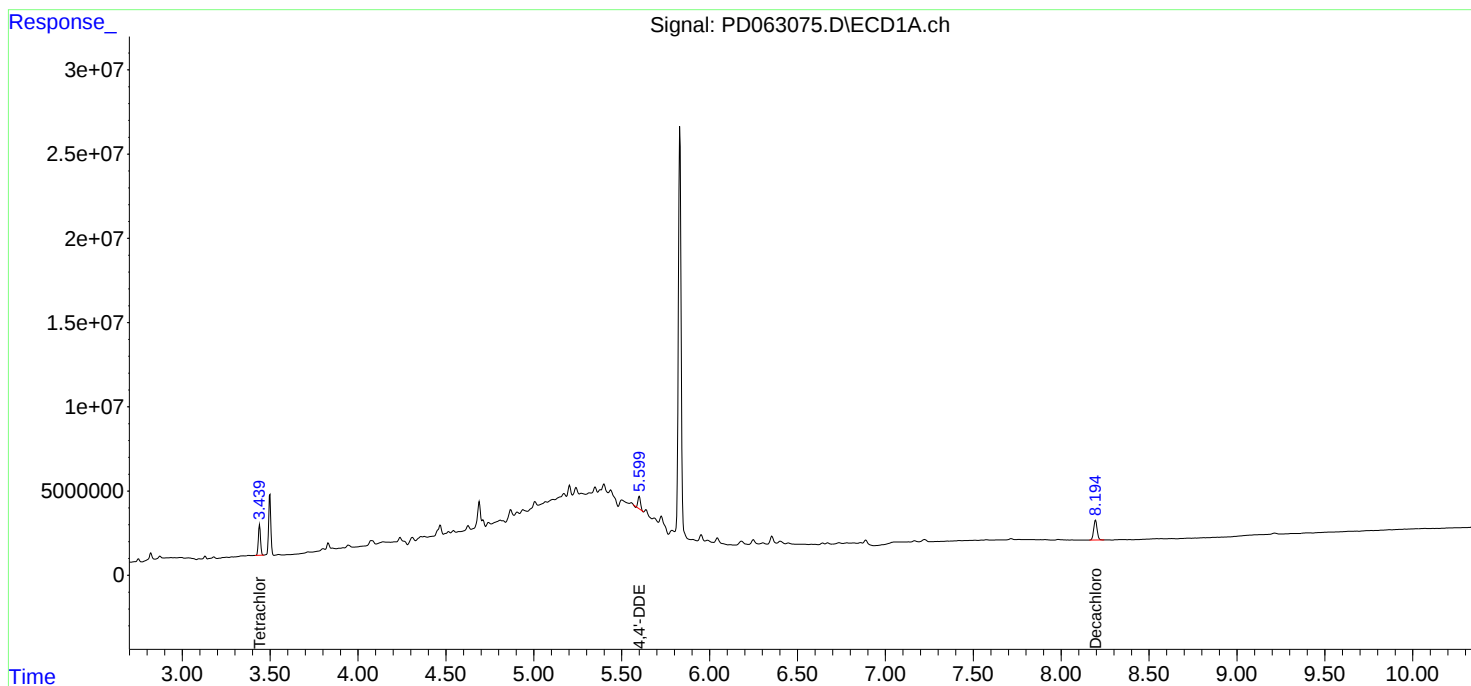


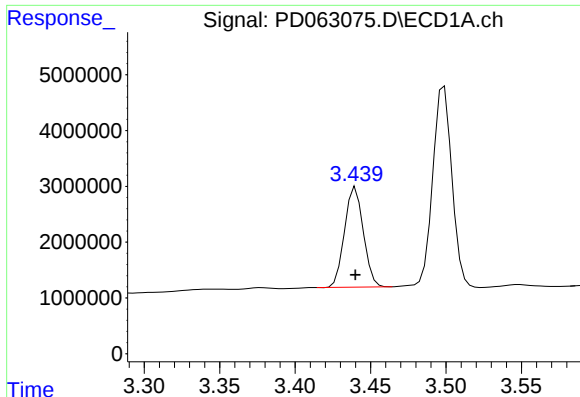

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 15562680
Conc: 14.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2A

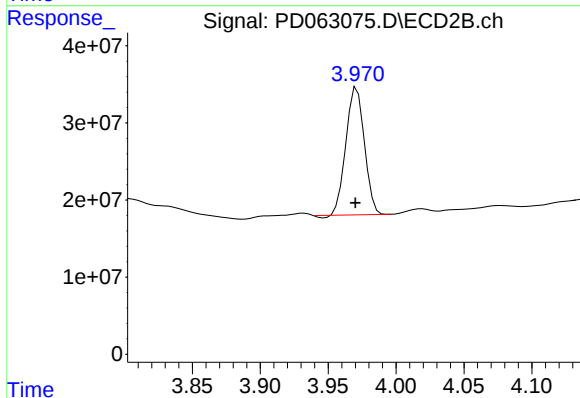


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.001 min
Response: 155904688
Conc: 13.45 ng/ml

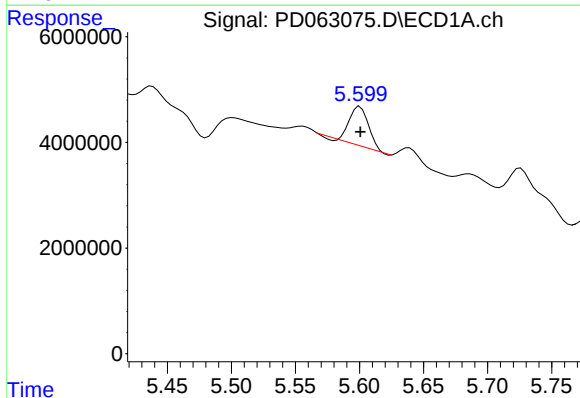


#12 4,4'-DDE

R.T.: 5.600 min
Delta R.T.: 0.000 min
Response: 7872100
Conc: 5.49 ng/ml

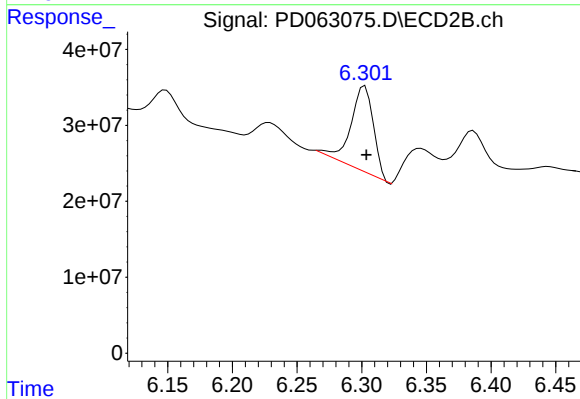

#12 4,4'-DDE


R.T.: 6.302 min
Delta R.T.: -0.001 min
Response: 137292819
Conc: 9.10 ng/ml

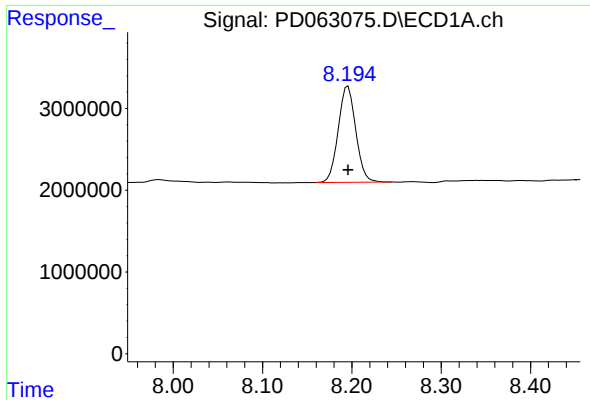

#28 Decachlorobiphenyl

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 15993530
Conc: 12.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2A

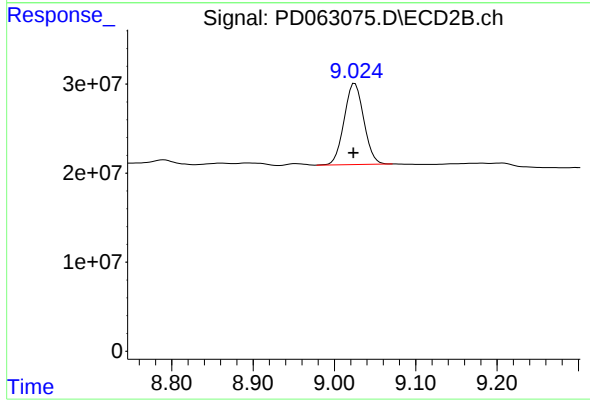

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.002 min
Response: 152650772
Conc: 14.96 ng/ml