

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
 Data File : PD063088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 22:39
 Operator : AR\AJ
 Sample : M2383-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 KTW-02

Manual Integrations
 APPROVED

Ankita
 5/27/2021 9:12:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 07:23:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.968	33014013	416.0E6	29.971m	35.897m
28) SA Decachlor...	8.194	9.026	17375972	191.1E6	13.806	18.736m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
Data File : PD063088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 22:39
Operator : AR\AJ
Sample : M2383-08
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
KTW-02


Manual Integrations
APPROVED

Ankita
5/27/2021 9:12:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 07:23:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

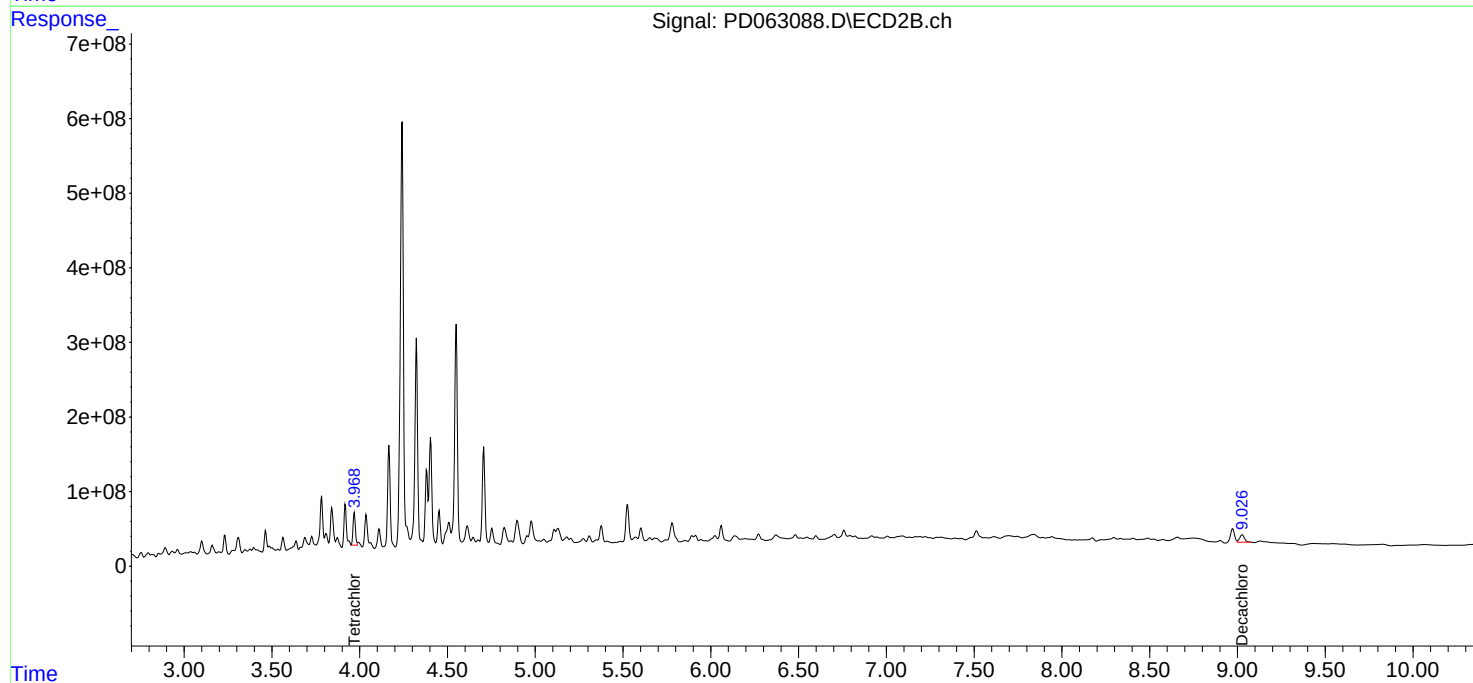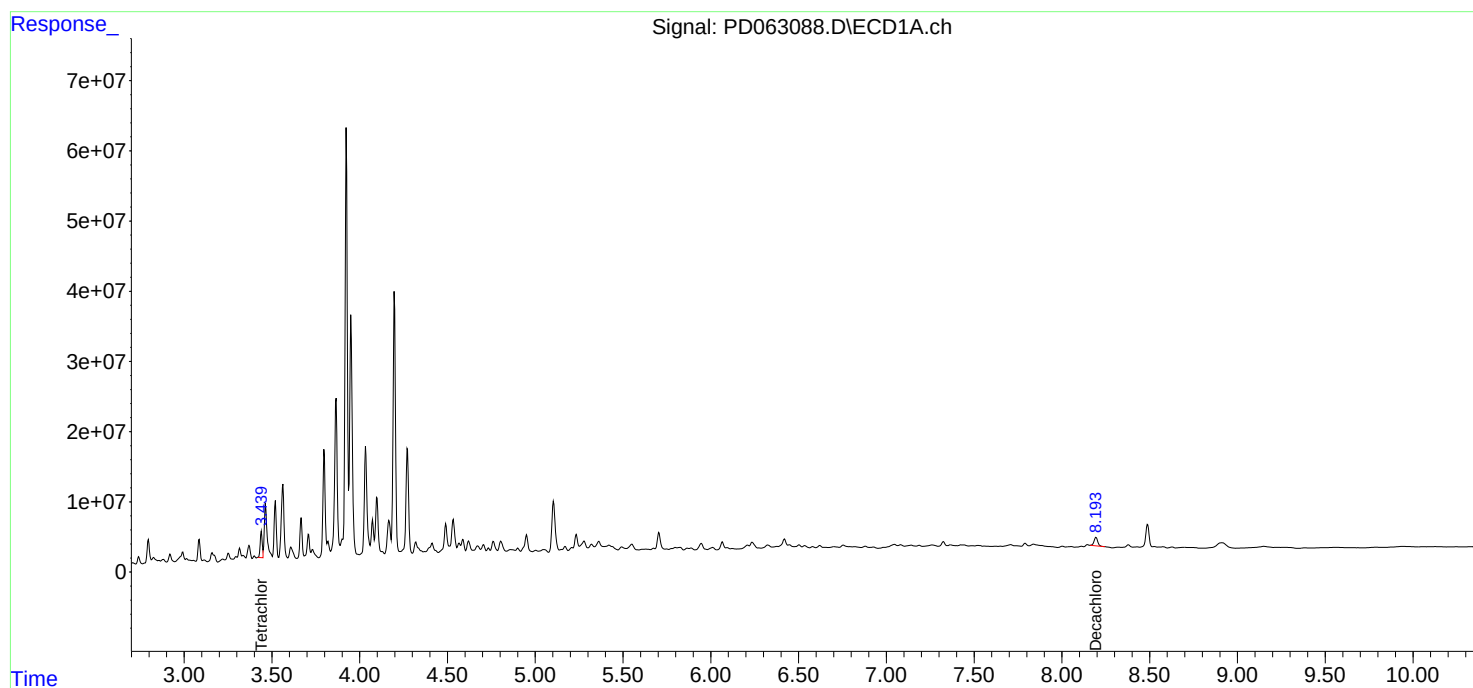

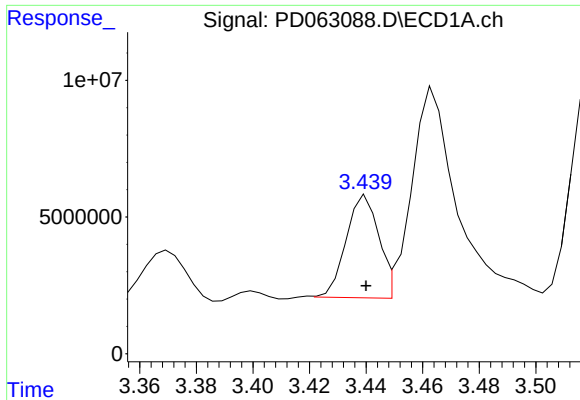


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 33014013
Conc: 29.97 ng/ml m

Instrument :
ECD_D
ClientSampleId :
KTW-02


Manual Integrations
APPROVED

Ankita
5/27/2021 9:12:03 AM

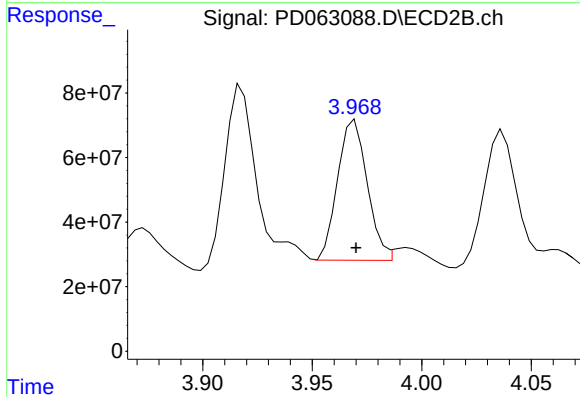


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 415981193
Conc: 35.90 ng/ml m

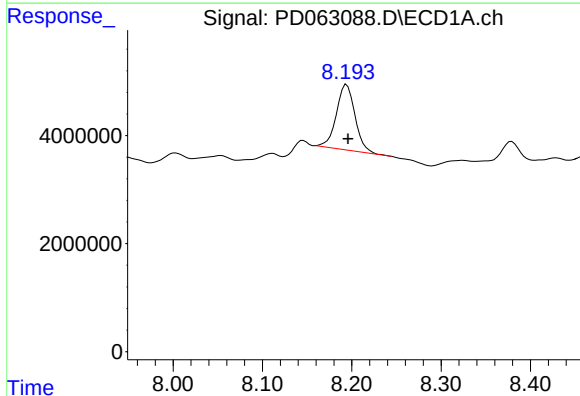

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 17375972
Conc: 13.81 ng/ml

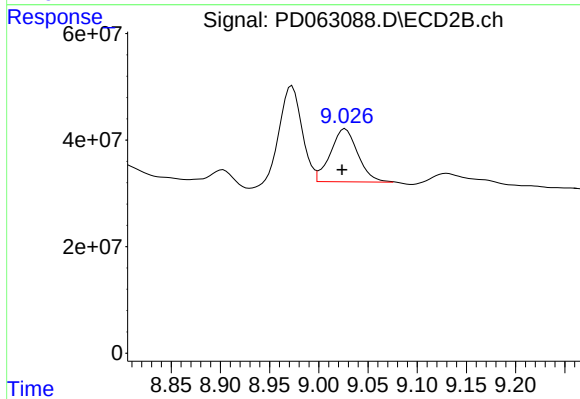

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 191142939
Conc: 18.74 ng/ml m