

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
 Data File : PD063095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 00:17
 Operator : AR\AJ
 Sample : M2392-23
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-08-COMP

Manual Integrations
 APPROVED

Ankita
 5/19/2021 3:21:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 07:26:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
 Quant Title : GC Extractables
 QLast Update : Tue May 18 07:12:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.971	15502105	158.9E6	14.073	13.714
28)	SA Decachlor...	8.195	9.024	14530358	139.2E6	11.545	13.642
Target Compounds							
11)	B alpha-Chl...	5.434	6.148	970239	15259533	0.672m	1.030 #
12)	B 4,4'-DDE	5.599	6.302	1008522	14628652	0.703m	0.969 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051921\
Data File : PD063095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 00:17
Operator : AR\AJ
Sample : M2392-23
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-08-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:21:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 07:26:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051721.M
Quant Title : GC Extractables
QLast Update : Tue May 18 07:12:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

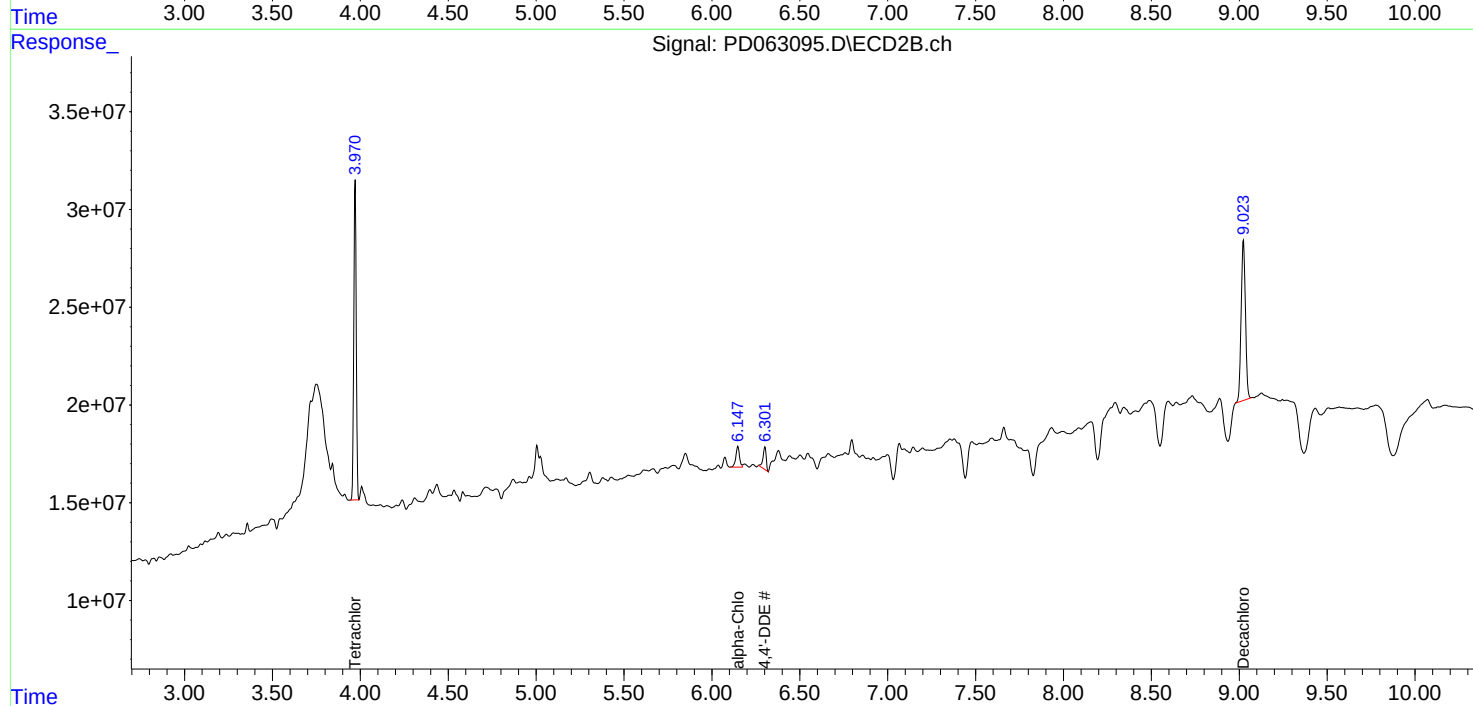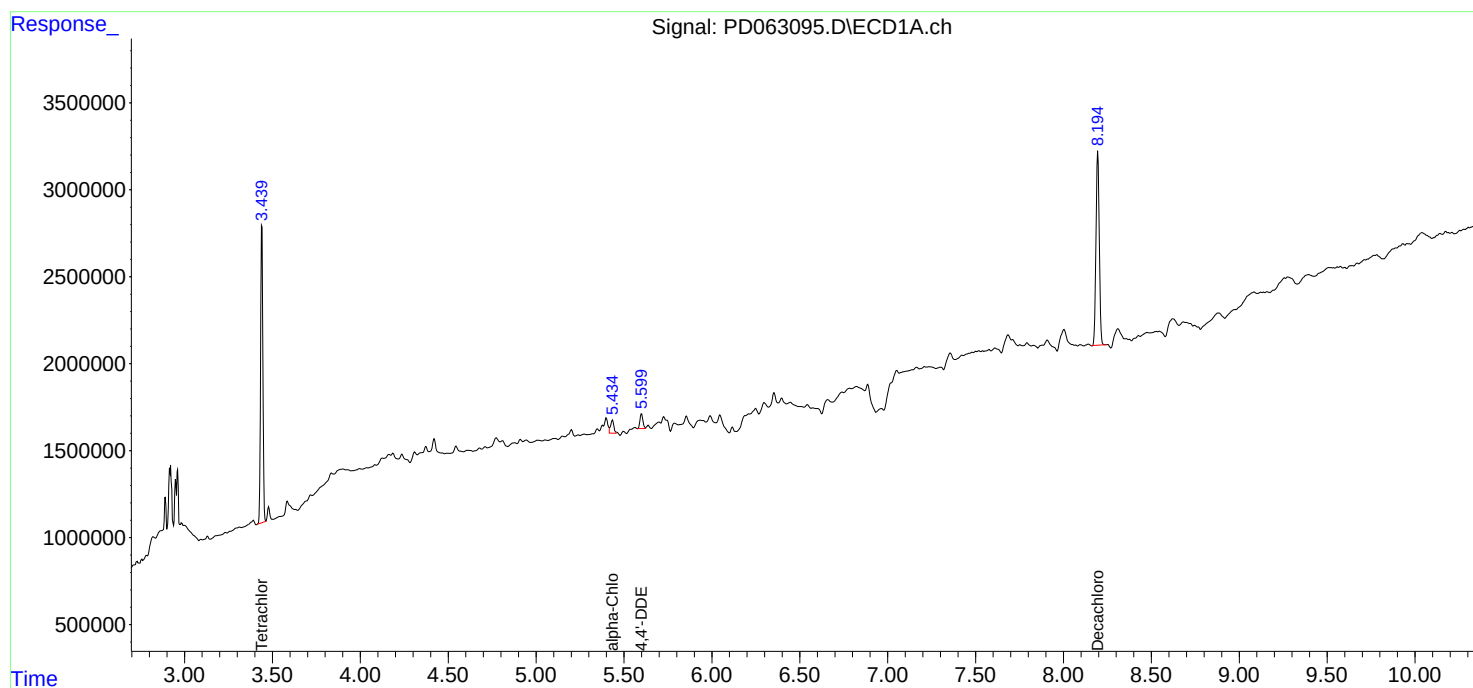

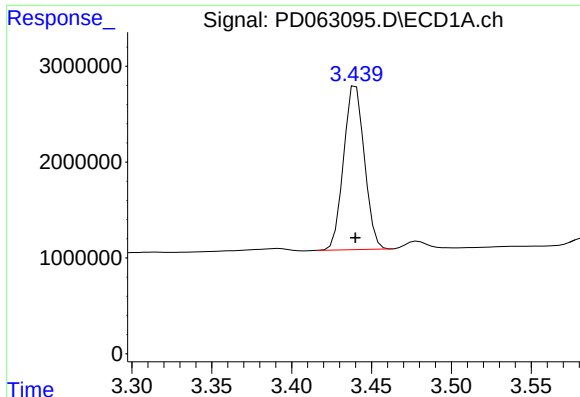


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 15502105
Conc: 14.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-08-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:21:00 PM

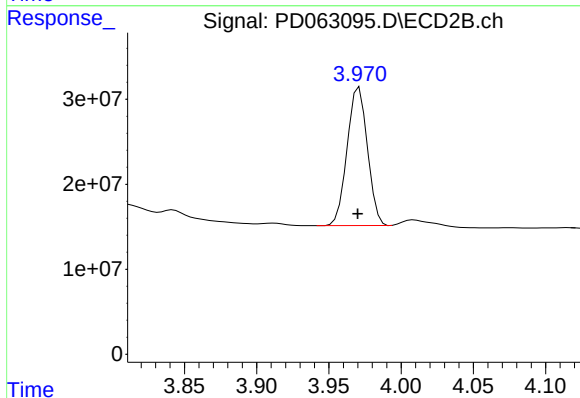


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 158920607
Conc: 13.71 ng/ml

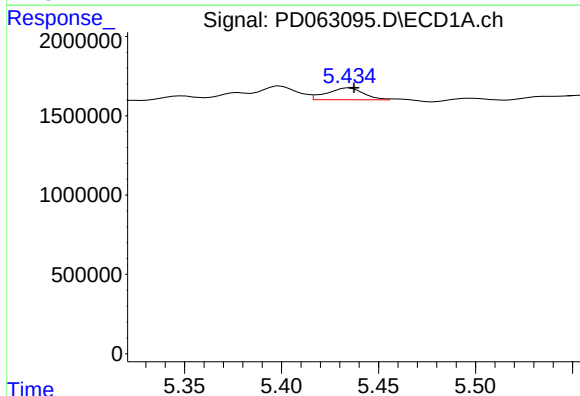


#11 alpha-Chlordane

R.T.: 5.434 min
Delta R.T.: -0.004 min
Response: 970239
Conc: 0.67 ng/ml m

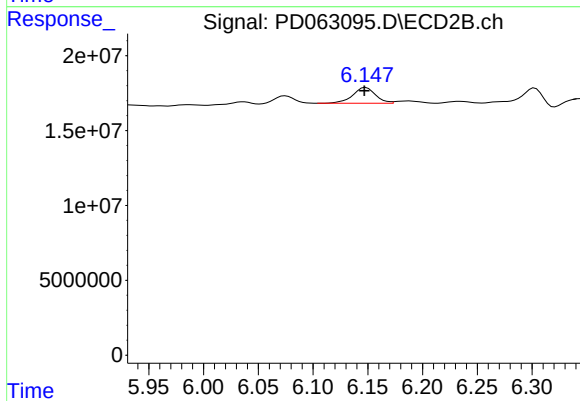

#11 alpha-Chlordane

R.T.: 6.148 min
Delta R.T.: 0.001 min
Response: 15259533
Conc: 1.03 ng/ml

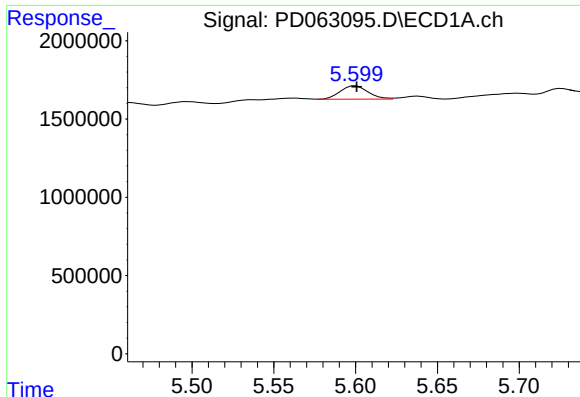


#12 4,4'-DDE

R.T.: 5.599 min
Delta R.T.: -0.002 min
Response: 1008522
Conc: 0.70 ng/ml m

Instrument :
ECD_D
ClientSampleId :
SB-08-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:21:00 PM

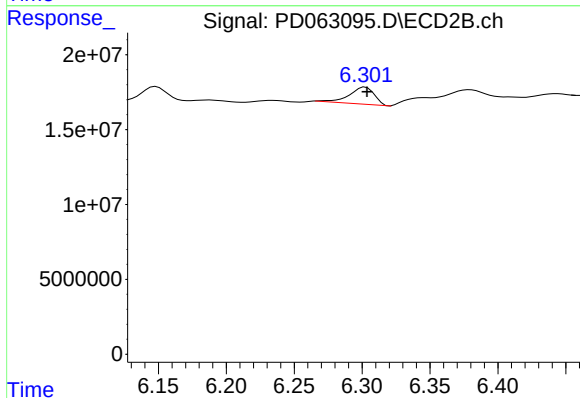


#12 4,4'-DDE

R.T.: 6.302 min
Delta R.T.: -0.001 min
Response: 14628652
Conc: 0.97 ng/ml

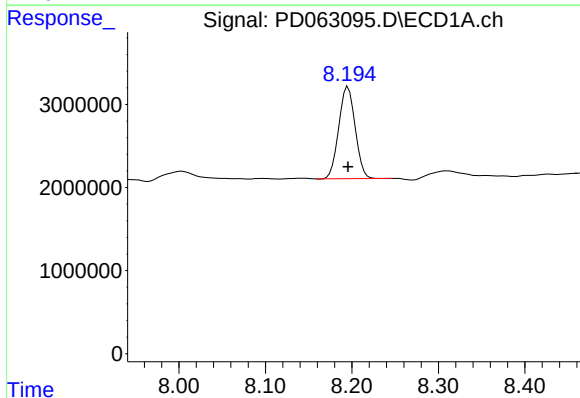

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 14530358
Conc: 11.55 ng/ml

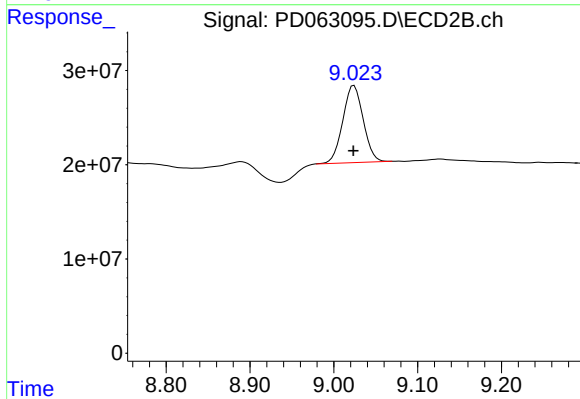

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 139171244
Conc: 13.64 ng/ml